

EXDA Metadata Report

Project: VH2D-Project-Wk-22-2026

Generated: 2026-06-06 10:47:50

Includes: Plan, DAQ Systems, Sensors Mapping, Gas Mixing

Responsible Researcher: PhD Student Javier I. Camacho

Project Objective:

LU / DBI / Kistler pressure DAQ systems characterisation.

Project Description:

The primary objectives of the experiments are:

1. Internal Over-pressure Development

Measurement of internal over-pressure development during vented hydrogen deflagrations in a partially confined enclosure for homogeneous flammable hydrogen-air mixtures with hydrogen concentrations up to 19 vol.%.

2.Flame Propagation (Under Consideration)

Measurement of flame propagation characteristics, including potential estimation of flame time-of-arrival (TOA) at selected locations.

3.Instrumentation Evaluation

Evaluation and cross-comparison of different pressure measurement systems and data acquisition configurations, including sensor characteristics and the influence of measurement chain dynamics (e.g., time constant (τ) effects, sampling rate).

4. Measurement Uncertainty Factors

Investigation of experimental factors that may affect the accuracy and reliability of pressure measurements, including structural vibration effects and thermal protection methods.

5. Venting Behavior

Investigation of vent opening behavior and the influence of vent rupture mechanisms on pressure development, including comparison between pressure-driven thin-film rupture and controlled vent opening using a hot-wire cutting system.



Campaign Overview - Experiment_Plan_v000

Generated: 2026-06-06 10:47:49



Start: 2026-05-25

Deadline: 2026-05-29


3
Canceled Runs

1
Error Runs

13
Preparation Runs

89%
Completion (24/27)

Campaign Schedule

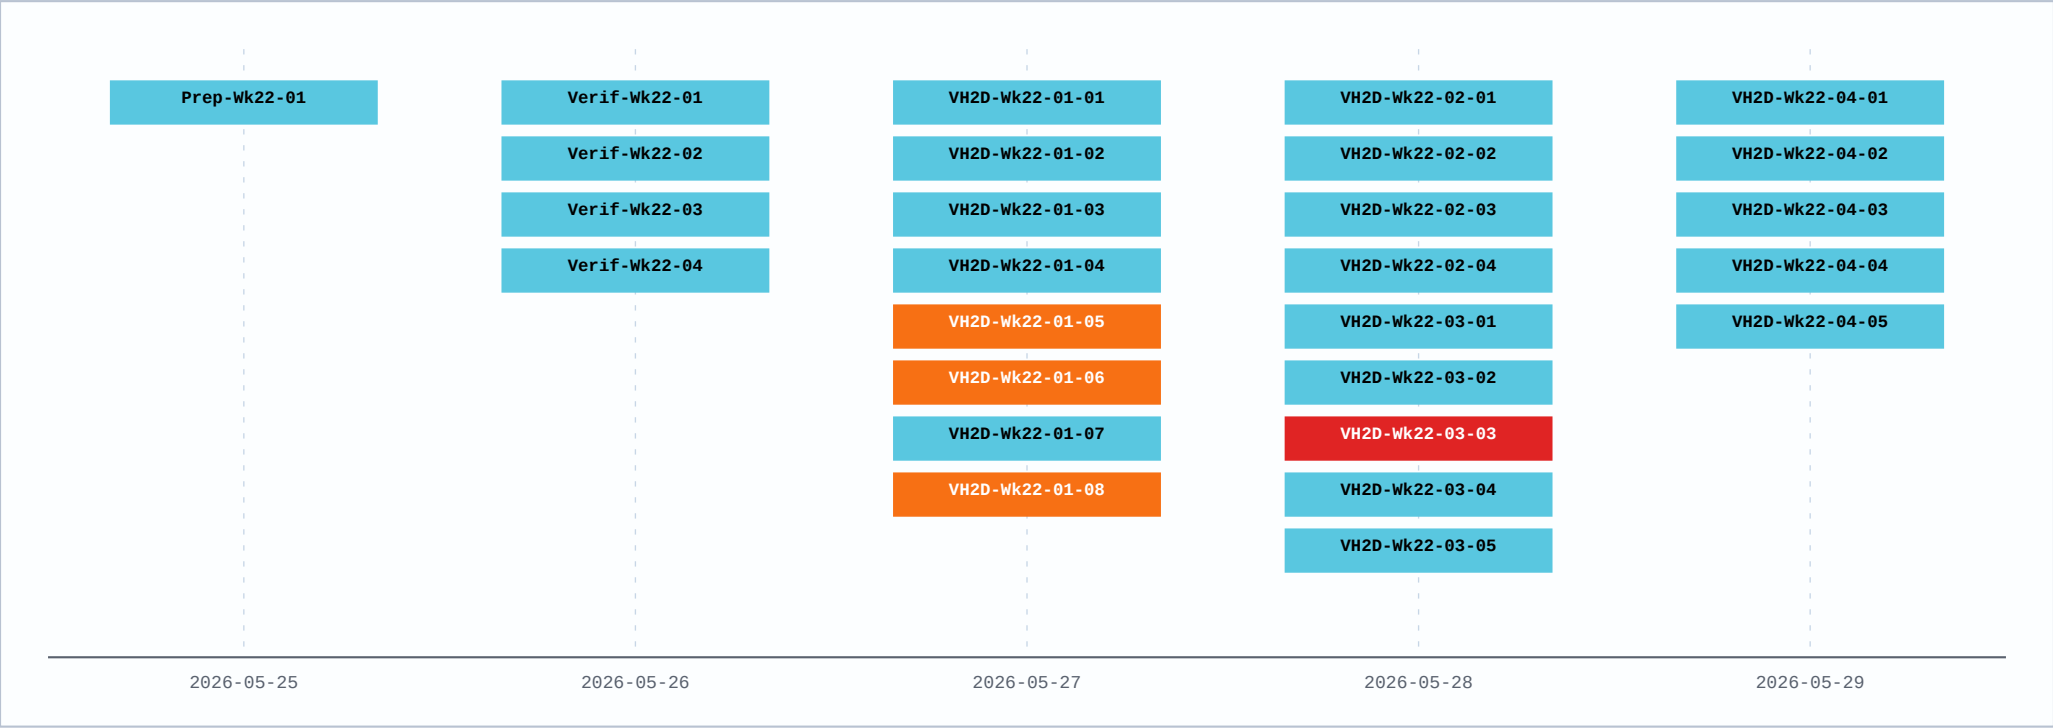

Done Canceled Error

EXDA Plan Export - Experiment_Plan_v000

Responsible Researcher: PhD Student Javier I. Camacho
Objective: LU / DBI / Kistler pressure DAQ systems characterisation.
Start: 2026-05-25 | Deadline: 2026-05-29
Total Experiments: 27
Generated: 2026-06-06 10:47:49

Group: Prep-Wk22

Group Objective: Preparation

[1/1] Run: Prep-Wk22-01

Status: DONE | Done: Yes | Preparation: Yes | Schedule: 2026-05-25
H2: 13.5 %vol | H2 Injected: 8.275657522940918 g | MFC Flow: 20 SLPM
Ignition: Back Wall | Vent: Thin Film with Hotwire NOT Activated | P0: 101325 Pa | T0: 292.15 K
Recirc Stop -> Ignition: - s | Case ID / CFD Hash: -
Error: No | Canceled: No | Data Files: 3
Short Description: Preliminar Test
Run Notes: Recirc stop · ignition time (s): No Recorded injected 8.276 gr temp 292.15 K
Error Note: -
Canceled Note: -
Data Files:

- Prep-Wk22-01/H2BGA/Prep-01-H2BGA-U.csv
- Prep-Wk22-01/DAQ-1/Prep-01.exp/data/Prep-01-DAQ-1.tpc5
- Prep-Wk22-01/DAQ-2/Prep-01-DAQ-2.mf4

Group: Verif-Wk22

Group Objective: Performance Verification

[1/4] Run: Verif-Wk22-01

Status: DONE | Done: Yes | Preparation: Yes | Schedule: 2026-05-26
H2: 13.5 %vol | H2 Injected: 8.216595905954765 g | MFC Flow: 20 SLPM
Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 294.25 K
Recirc Stop -> Ignition: 312 s | Case ID / CFD Hash: -
Error: No | Canceled: No | Data Files: 5
Short Description: -
Run Notes: Physical Range -1,1 bar
Error Note: -
Canceled Note: -

Data Files:

- Verif-Wk22-01/DAQ-1/DAQ-1-Verif-01.tpc5
- Verif-Wk22-01/DAQ-2/DAQ-2-Verif_01.mf4
- Verif-Wk22-01/H2BGA/H2BGA-L-Verif-01-260526-120036.csv
- Verif-Wk22-01/H2BGA/H2BGA-M-Verif-01-260526-115955.csv
- Verif-Wk22-01/H2BGA/H2BGA-U-Verif-01-260526-115817.csv

[2/4] Run: Verif-Wk22-02

Status: DONE | Done: Yes | Preparation: Yes | Schedule: 2026-05-26

H2: 14 %vol | H2 Injected: 9.383538505159276 g | MFC Flow: 20 SLPM

Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 293.15 K

Recirc Stop -> Ignition: 321 s | Case ID / CFD Hash: -

Error: No | Canceled: No | Data Files: 3

Short Description: -

Run Notes: Physical Range -1,1 bar

Error Note: -

Canceled Note: -

Data Files:

- Verif-Wk22-02/H2BGA/H2BGA-U-M-L-Verif-02-260526-144155.csv
- Verif-Wk22-02/DAQ-1/DAQ-1-Verif-02.tpc5
- Verif-Wk22-02/DAQ-2/DAQ-2-Verif_02/DAQ-2-Verif_02.mf4

[3/4] Run: Verif-Wk22-03

Status: DONE | Done: Yes | Preparation: Yes | Schedule: 2026-05-26

H2: 16 %vol | H2 Injected: 10.637876563061878 g | MFC Flow: 20 SLPM

Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 294.15 K

Recirc Stop -> Ignition: 263 s | Case ID / CFD Hash: -

Error: No | Canceled: No | Data Files: 3

Short Description: -

Run Notes: Channel 2 Physical Range -1, ,1 bar Channel 2 Physical Range -0.5, ,0.5 bar Leak on Blind Sensor

Flange Connection 3L & 5L Volume Correction +0.06708

Error Note: -

Canceled Note: -

Data Files:

- Verif-Wk22-03/DAQ-1/DAQ-1-Verif-03.tpc5
- Verif-Wk22-03/DAQ-2/DAQ-2-Verif-03/DAQ-2-Verif-03.mf4
- Verif-Wk22-03/H2BGA/H2BGA-U-M-L-Verif-03-260526-160316.csv

[4/4] Run: Verif-Wk22-04

Status: DONE | Done: Yes | Preparation: Yes | Schedule: 2026-05-26

H2: 18 %vol | H2 Injected: 12.070196519467626 g | MFC Flow: 20 SLPM
Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 291.65 K
Recirc Stop -> Ignition: 233 s | Case ID / CFD Hash: -
Error: No | Canceled: No | Data Files: 3
Short Description: -
Run Notes: P1 swapped for P5
Error Note: -
Canceled Note: -
Data Files:
- Verif-Wk22-04/DAQ-1/DAQ-1-Verif-04.tpc5
- Verif-Wk22-04/DAQ-2/DAQ-2-Verif-04/DAQ-2-Verif-04.mf4
- Verif-Wk22-04/H2BGA/H2BGA-U-M-L-Verif-04-260526-174304.csv

Group: VH2D-Wk22-01

Group Objective: Vented deflagration concentration series (Hotwire)

[1/8] Run: VH2D-Wk22-01-01

Status: DONE | Done: Yes | Preparation: Yes | Schedule: 2026-05-27
H2: 16 %vol | H2 Injected: 10.674164731450286 g | MFC Flow: 20 SLPM
Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 293.15 K
Recirc Stop -> Ignition: - s | Case ID / CFD Hash: -
Error: No | Canceled: No | Data Files: 3
Short Description: -
Run Notes: -
Error Note: -
Canceled Note: -
Data Files:
- VH2D-Wk22-01-01/H2BGA/H2BGA-U-M-L-VH2D-01-01-260527-140320.csv
- VH2D-Wk22-01-01/DAQ-2-3/DAQ-2-3-VH2D-01-01.mf4
- VH2D-Wk22-01-01/DAQ-1/DAQ-1-VH2D-01-01.tpc5

[2/8] Run: VH2D-Wk22-01-02

Status: DONE | Done: Yes | Preparation: Yes | Schedule: 2026-05-27
H2: 16 %vol | H2 Injected: 10.714368741738232 g | MFC Flow: 20 SLPM
Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 292.05 K
Recirc Stop -> Ignition: 228 s | Case ID / CFD Hash: -
Error: No | Canceled: No | Data Files: 3
Short Description: -
Run Notes: -

Error Note: -

Canceled Note: -

Data Files:

- VH2D-Wk22-01-02/DAQ-1/DAQ-1-VH2D-01-02.tpc5
- VH2D-Wk22-01-02/H2BGA/H2BGA-U-M-L-VH2D-01-02-260527-150043.csv
- VH2D-Wk22-01-02/DAQ-2-3/DAQ-2-3-VH2D-01-02.mf4

[3/8] Run: VH2D-Wk22-01-03

Status: DONE | Done: Yes | Preparation: Yes | Schedule: 2026-05-27

H2: 18 %vol | H2 Injected: - g | MFC Flow: 20 SLPM

Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 293 K

Recirc Stop -> Ignition: 201 s | Case ID / CFD Hash: -

Error: No | Canceled: No | Data Files: 2

Short Description: -

Run Notes: -

Error Note: -

Canceled Note: -

Data Files:

- VH2D-Wk22-01-03/DAQ-1/DAQ-1-VH2D-01-03.tpc5
- VH2D-Wk22-01-03/DAQ-2-3/DAQ-2-3-VH2D-01-03.mf4

[4/8] Run: VH2D-Wk22-01-04

Status: DONE | Done: Yes | Preparation: Yes | Schedule: 2026-05-27

H2: 18 %vol | H2 Injected: 12.103396303602311 g | MFC Flow: 20 SLPM

Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 290.85 K

Recirc Stop -> Ignition: 168 s | Case ID / CFD Hash: -

Error: No | Canceled: No | Data Files: 3

Short Description: -

Run Notes: PP1 and PP3 swapped DAQ-3 sampling rate 62.5kHz changed to 200kHz

Error Note: -

Canceled Note: -

Data Files:

- VH2D-Wk22-01-04/DAQ-1/DAQ-1-VH2D-01-04.tpc5
- VH2D-Wk22-01-04/DAQ-2-3/DAQ-2-3-VH2D-01-04.mf4
- VH2D-Wk22-01-04/H2BGA/H2BGA-U-M-L-VH2D-01-04-260527-164423.csv

[5/8] Run: VH2D-Wk22-01-05

Status: CANCELED | Done: No | Preparation: Yes | Schedule: 2026-05-27

H2: 19 %vol | H2 Injected: - g | MFC Flow: 20 SLPM

Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 293 K

Recirc Stop -> Ignition: - s | Case ID / CFD Hash: -
Error: No | Canceled: Yes | Data Files: 0
Short Description: -
Run Notes: DAQ-3 sampling rate 62.5kHz changed to 200kHz
Error Note: -
Canceled Note: Time restriction
Data Files: -

[6/8] Run: VH2D-Wk22-01-06

Status: CANCELED | Done: No | Preparation: Yes | Schedule: 2026-05-27
H2: 19 %vol | H2 Injected: - g | MFC Flow: - SLPM
Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 293 K
Recirc Stop -> Ignition: - s | Case ID / CFD Hash: -
Error: No | Canceled: Yes | Data Files: 0
Short Description: -
Run Notes: -
Error Note: -
Canceled Note: Time restriction
Data Files: -

[7/8] Run: VH2D-Wk22-01-07

Status: DONE | Done: Yes | Preparation: Yes | Schedule: 2026-05-27
H2: 20 %vol | H2 Injected: 13.461640414306215 g | MFC Flow: 20 SLPM
Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 290.56 K
Recirc Stop -> Ignition: - s | Case ID / CFD Hash: -
Error: No | Canceled: No | Data Files: 3
Short Description: -
Run Notes: PP1 and PP3 swapped
Error Note: -
Canceled Note: -
Data Files:
- VH2D-Wk22-01-07/DAQ-1/DAQ-1-VH2D-01-07.tpc5
- VH2D-Wk22-01-07/DAQ-2-3/VH2D-01-07.mf4
- VH2D-Wk22-01-07/H2BGA/H2BGA-U-M-L-VH2D-01-07-260527-180934.csv

[8/8] Run: VH2D-Wk22-01-08

Status: CANCELED | Done: No | Preparation: Yes | Schedule: 2026-05-27
H2: 20 %vol | H2 Injected: - g | MFC Flow: - SLPM
Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 293 K
Recirc Stop -> Ignition: - s | Case ID / CFD Hash: -

Error: No | Canceled: Yes | Data Files: 0
Short Description: -
Run Notes: -
Error Note: -
Canceled Note: Time restriction
Data Files: -

Group: VH2D-Wk22-02

Group Objective: Vented deflagration concentration series (LU vs Kistler)

[1/4] Run: VH2D-Wk22-02-01

Status: DONE | Done: Yes | Preparation: No | Schedule: 2026-05-28
H2: 18 %vol | H2 Injected: 12.27804 g | MFC Flow: 20 SLPM
Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 289.95 K
Recirc Stop -> Ignition: 243 s | Case ID / CFD Hash: -
Error: No | Canceled: No | Data Files: 4
Short Description: -
Run Notes: Added 12.278 gr Correlation> M= 69.638 C - 0.2568
Error Note: -
Canceled Note: -
Data Files:
- VH2D-Wk22-02-01/DAQ-1/DAQ-1-VH2D-02-01.tpc5
- VH2D-Wk22-02-01/DAQ-2-3/DAQ-2-3-VH2D-02-01.mf4
- VH2D-Wk22-02-01/DAQ-4/DAQ-4-VH2D-02-01.mf4
- VH2D-Wk22-02-01/H2BGA/H2BGA-U-M-L-VH2D-02-01-260528-105051.csv

[2/4] Run: VH2D-Wk22-02-02

Status: DONE | Done: Yes | Preparation: No | Schedule: 2026-05-28
H2: 18 %vol | H2 Injected: 12.27804 g | MFC Flow: 20 SLPM
Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 291.15 K
Recirc Stop -> Ignition: 231 s | Case ID / CFD Hash: -
Error: No | Canceled: No | Data Files: 4
Short Description: -
Run Notes: P3 and P7 swapped Added 12.278 gr Correlation> M= 69.638 C - 0.2568
Error Note: -
Canceled Note: -
Data Files:
- VH2D-Wk22-02-02/DAQ-1/DAQ-1-VH2D-02-02.tpc5
- VH2D-Wk22-02-02/DAQ-2-3/DAQ-2-3-VH2D-02-02.mf4

- VH2D-Wk22-02-02/DAQ-4/DAQ-4-VH2D-02-02.mf4
- VH2D-Wk22-02-02/H2BGA/H2BGA-U-M-L-VH2D-02-02-260528-115959.csv

[3/4] Run: VH2D-Wk22-02-03

Status: DONE | Done: Yes | Preparation: No | Schedule: 2026-05-28
H2: 20 %vol | H2 Injected: 13.670800000000002 g | MFC Flow: 20 SLPM
Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 293.15 K
Recirc Stop -> Ignition: 232 s | Case ID / CFD Hash: -
Error: No | Canceled: No | Data Files: 4
Short Description: -
Run Notes: P3 and P7 swapped Added 13.671 gr Correlation> M= 69.638 C - 0.2568
Error Note: -
Canceled Note: -
Data Files:
- VH2D-Wk22-02-03/DAQ-1/DAQ-1-VH2D-02-03.tpc5
- VH2D-Wk22-02-03/DAQ-2-3/DAQ-2-3-VH2D-02-03.mf4
- VH2D-Wk22-02-03/DAQ-4/DAQ-4-VH2D-02-03.mf4
- VH2D-Wk22-02-03/H2BGA/H2BGA-U-M-L-VH2D-02-03-260528-134340.csv

[4/4] Run: VH2D-Wk22-02-04

Status: DONE | Done: Yes | Preparation: No | Schedule: 2026-05-28
H2: 20 %vol | H2 Injected: 13.670800000000002 g | MFC Flow: 20 SLPM
Ignition: back | Vent: thin film | P0: 101325 Pa | T0: 292.15 K
Recirc Stop -> Ignition: 221 s | Case ID / CFD Hash: -
Error: No | Canceled: No | Data Files: 4
Short Description: -
Run Notes: P3 and P7 swapped Added 13.671 gr Correlation> M= 69.638 C - 0.2568
Error Note: -
Canceled Note: -
Data Files:
- VH2D-Wk22-02-04/DAQ-1/DAQ-1-VH2D-02-04.tpc5
- VH2D-Wk22-02-04/DAQ-2-3/DAQ-2-3-VH2D-02-04.mf4
- VH2D-Wk22-02-04/DAQ-4/DAQ-4-VH2D-02-04.mf4
- VH2D-Wk22-02-04/H2BGA/H2BGA-U-M-L-VH2D-02-04-260528-144105.csv

Group: VH2D-Wk22-03

Group Objective: Vented deflagration concentration series (LU vs DBI)

[1/5] Run: VH2D-Wk22-03-01

Status: DONE | Done: Yes | Preparation: No | Schedule: 2026-05-28
H2: 18 %vol | H2 Injected: 12.27804 g | MFC Flow: 20 SLPM
Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 292.45 K
Recirc Stop -> Ignition: 230 s | Case ID / CFD Hash: -
Error: No | Canceled: No | Data Files: 3
Short Description: -
Run Notes: Added 12.278 gr Correlation> M= 69.638 C - 0.2568
Error Note: -
Canceled Note: -
Data Files:
- VH2D-Wk22-03-01/DAQ-1/DAQ-1-VH2D-03-01.tpc5
- VH2D-Wk22-03-01/DAQ-2-3/DAQ-2-3-VH2D-03.mf4
- VH2D-Wk22-03-01/H2BGA/H2BGA-U-M-L-VH2D-03-01-260528-160918.csv

[2/5] Run: VH2D-Wk22-03-02

Status: DONE | Done: Yes | Preparation: No | Schedule: 2026-05-28
H2: 18 %vol | H2 Injected: 12.27804 g | MFC Flow: 20 SLPM
Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 292.25 K
Recirc Stop -> Ignition: 232 s | Case ID / CFD Hash: -
Error: No | Canceled: No | Data Files: 3
Short Description: -
Run Notes: PP3 moved to 5m radius Added 12.278 gr Correlation> M= 69.638 C - 0.2568
Error Note: -
Canceled Note: -
Data Files:
- VH2D-Wk22-03-02/DAQ-1/DAQ-1-VH2D-03-02.tpc5
- VH2D-Wk22-03-02/DAQ-2-3/DAQ-2-3-VH2D-03-02.mf4
- VH2D-Wk22-03-02/H2BGA/H2BGA-U-M-L-VH2D-03-02-260528-164833.csv

[3/5] Run: VH2D-Wk22-03-03

Status: ERROR | Done: Yes | Preparation: No | Schedule: 2026-05-28
H2: 20 %vol | H2 Injected: 13.670800000000002 g | MFC Flow: 20 SLPM
Ignition: Back Wall | Vent: Thin Film | P0: 101325 Pa | T0: 292.15 K
Recirc Stop -> Ignition: - s | Case ID / CFD Hash: -
Error: Yes | Canceled: No | Data Files: 3
Short Description: Attention!!! Hot-wire short circuit. Check carefully data could compromised.
Run Notes: Added 13.671 gr Correlation> M= 69.638 C - 0.2568 Attention!!! Hot-wire short circuit. Check carefully data could compromised.
Error Note: Attention!!! Hot-wire short circuit. Check carefully data could compromised.
Canceled Note: -

Data Files:

- VH2D-Wk22-03-03/DAQ-1/DAQ-1-VH2D-03-03.tpc5
- VH2D-Wk22-03-03/DAQ-2-3/DAQ-2-3-VH2D-03-03.mf4
- VH2D-Wk22-03-03/H2BGA/H2BGA-U-M-L-VH2D-03-03-260528-173139.csv

[4/5] Run: VH2D-Wk22-03-04

Status: DONE | Done: Yes | Preparation: No | Schedule: 2026-05-28
H2: 20 %vol | H2 Injected: 13.670800000000002 g | MFC Flow: 20 SLPM
Ignition: vack | Vent: thin | P0: 101325 Pa | T0: 291.65 K
Recirc Stop -> Ignition: 221 s | Case ID / CFD Hash: -
Error: No | Canceled: No | Data Files: 3
Short Description: -
Run Notes: Added 13.671 gr Correlation> M= 69.638 C - 0.2568
Error Note: -
Canceled Note: -
Data Files:

- VH2D-Wk22-03-04/DAQ-1/DAQ-1-VH2D-03-04.tpc5
- VH2D-Wk22-03-04/DAQ-2-3/DAQ-2-3-VH2D-03-04.mf4
- VH2D-Wk22-03-04/H2BGA/H2BGA-U-M-L-VH2D-03-04-260528-181435.csv

[5/5] Run: VH2D-Wk22-03-05

Status: DONE | Done: Yes | Preparation: No | Schedule: 2026-05-28
H2: 20 %vol | H2 Injected: 13.670800000000002 g | MFC Flow: 20 SLPM
Ignition: Back Wall | Vent: Thin Film | P0: 101325 Pa | T0: 291.45 K
Recirc Stop -> Ignition: 321 s | Case ID / CFD Hash: -
Error: No | Canceled: No | Data Files: 3
Short Description: -
Run Notes: Added 13.671 gr Correlation> M= 69.638 C - 0.2568
Error Note: -
Canceled Note: -
Data Files:

- VH2D-Wk22-03-05/DAQ-1/DAQ-1-VH2D-03-05.tpc5
- VH2D-Wk22-03-05/DAQ-2-3/DAQ-2-3-VH2D-03-05.mf4
- VH2D-Wk22-03-05/H2BGA/H2BGA-U-M-L-VH2D-03-05-260528-184939.csv

Group: VH2D-Wk22-04

Group Objective: Vented deflagration concentration series (LU vs DBI)

[1/5] Run: VH2D-Wk22-04-01

Status: DONE | Done: Yes | Preparation: No | Schedule: 2026-05-29
H2: 16 %vol | H2 Injected: 10.885280000000002 g | MFC Flow: 20 SLPM
Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 291.75 K
Recirc Stop -> Ignition: 245 s | Case ID / CFD Hash: -
Error: No | Canceled: No | Data Files: 3
Short Description: -
Run Notes: Added 10.885 gr Correlation> M= 69.638 C - 0.2568 Missing data from H2CM. !!! Mean Value: 16.1 Vol.%
Error Note: -
Canceled Note: -
Data Files:
- VH2D-Wk22-04-01/DAQ-1/DAQ-1-VH2D-04-01.tpc5
- VH2D-Wk22-04-01/DAQ-2-3/DAQ-2-3-VH2D-04-01_Rec_01.mf4
- VH2D-Wk22-04-01/H2BGA/H2BGA-U-M-L-VH2D-04-01-260529-104759.csv

[2/5] Run: VH2D-Wk22-04-02

Status: DONE | Done: Yes | Preparation: No | Schedule: 2026-05-29
H2: 16 %vol | H2 Injected: 10.885280000000002 g | MFC Flow: 20 SLPM
Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 292.75 K
Recirc Stop -> Ignition: 502 s | Case ID / CFD Hash: -
Error: No | Canceled: No | Data Files: 3
Short Description: -
Run Notes: Added 10.885 gr Correlation> M= 69.638 C - 0.2568 1024 hPa HR 53%
Error Note: -
Canceled Note: -
Data Files:
- VH2D-Wk22-04-02/DAQ-1/DAQ-1-VH2D-04-02.tpc5
- VH2D-Wk22-04-02/DAQ-2-3/DAQ-2-3-VH2D-04-02_Rec_01.mf4
- VH2D-Wk22-04-02/H2BGA/H2BGA-U-M-L-VH2D-04-02-260529-115753.csv

[3/5] Run: VH2D-Wk22-04-03

Status: DONE | Done: Yes | Preparation: No | Schedule: 2026-05-29
H2: 21 %vol | H2 Injected: 14.367180000000001 g | MFC Flow: 20 SLPM
Ignition: Back | Vent: thin plastic | P0: 101325 Pa | T0: 293.05 K
Recirc Stop -> Ignition: 261 s | Case ID / CFD Hash: -
Error: No | Canceled: No | Data Files: 3
Short Description: -
Run Notes: Added 14.367 gr Correlation> M= 69.638 C - 0.2568 1023 hPa HR 57%
Error Note: -
Canceled Note: -

Data Files:

- VH2D-Wk22-04-03/DAQ-1/DAQ-1-VH2D-04-03.tpc5
- VH2D-Wk22-04-03/DAQ-2-3/DAQ-2-3-VH2D-04-03_Rec_01.mf4
- VH2D-Wk22-04-03/H2BGA/H2BGA-U-M-L-VH2D-04-03-260529-125215.csv

[4/5] Run: VH2D-Wk22-04-04

Status: DONE | Done: Yes | Preparation: No | Schedule: 2026-05-29
H2: 21 %vol | H2 Injected: 14.367180000000001 g | MFC Flow: 20 SLPM
Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 293.75 K
Recirc Stop -> Ignition: 252 s | Case ID / CFD Hash: -
Error: No | Canceled: No | Data Files: 3
Short Description: -
Run Notes: Added 14.367 gr Correlation> M= 69.638 C - 0.2568 1023 hPa HR 44%
Error Note: -
Canceled Note: -
Data Files:

- VH2D-Wk22-04-04/DAQ-1/DAQ-1-VH2D-04-04.tpc5
- VH2D-Wk22-04-04/DAQ-2-3/DAQ-2-3-VH2D-04-04_Rec_01.mf4
- VH2D-Wk22-04-04/H2BGA/H2BGA-U-M-L-VH2D-04-04-260529-135315.csv

[5/5] Run: VH2D-Wk22-04-05

Status: DONE | Done: Yes | Preparation: No | Schedule: 2026-05-29
H2: 12 %vol | H2 Injected: 8.09976 g | MFC Flow: 10 SLPM
Ignition: Back Wall | Vent: Thin Film with Hotwire Activated | P0: 101325 Pa | T0: 295.05 K
Recirc Stop -> Ignition: - s | Case ID / CFD Hash: -
Error: No | Canceled: No | Data Files: 3
Short Description: Non Homogenous Flammable Mixture
Run Notes: Added xxxx gr for a 12vol.% 1020 hPa HR 41% Non H0mogeneous
Error Note: -
Canceled Note: -
Data Files:

- VH2D-Wk22-04-05/DAQ-1/DAQ-1-VH2D-04-05.tpc5
- VH2D-Wk22-04-05/DAQ-2-3/DAQ-2-3-VH2D-04-05_Rec_01.mf4
- VH2D-Wk22-04-05/H2BGA/H2BGA-M-U-L-M-VH2D-04-05-260529-150229.csv

EXDA DAQ Systems Export

Project: VH2D-Project-Wk-22-2026

Responsible Researcher: PhD Student Javier I. Camacho

Total DAQ Systems: 5

Reference PDF: LU-DBI Measurement Chain (frontend/public/LU-DBI_MeasurementChain_v001.pdf)


Reference PDF: Mixture Sampling Sub-System (frontend/public/MixtureSampling_Sub-System_000.pdf)

Generated: 2026-06-06 10:47:49

Name	Quantity	Vendor	Model	Serial	Fs (Hz)	Ch	Owner	Last Cal.	Cal Cert ID	Active	Notes
DAQ-1	pressure	Elsys -	TraNET	441309	1000000	8	LU	2024-10-21	-	Yes	2 equipment
		Kistler	204S8								
DAQ-2	pressure	Kistler	5165A4	6306100	200000	4	DBI	-	-	Yes	200 kHz from
											VH2D-02
DAQ-3	pressure	Kistler	5165A4	5358310	200000	4	Kistler	-	-	Yes	200 kHz from
											VH2D-02
DAQ-4	pressure	Kistler	-	-	2500000	8	Kistler	-	-	Yes	-
H2BGA	concentration	JCT	JTCD-300	14362	1	1	LU	2025-07-21	-	Yes	H2BGA-Hydrogen
											Binary Gas
											Analyser

DAQ Reference Diagram - LU-DBI Measurement Chain

Source: frontend/public/LU-DBI_MeasurementChain_v001.pdf

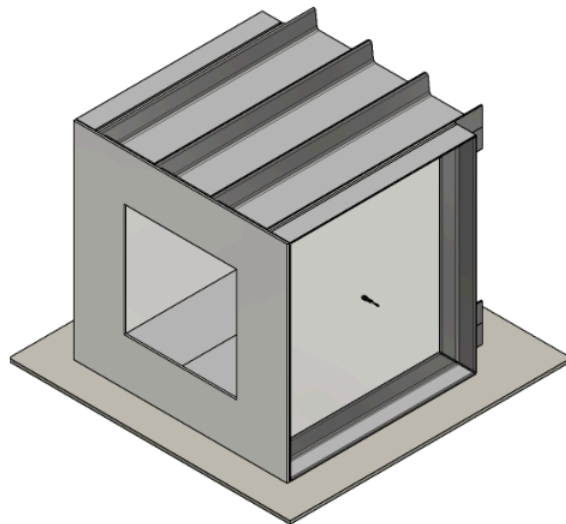


Explosion Chamber


Dimensions (Internal): 900 x 900 x 900 [mm]

Material: Steel


LU-Measurement Chain

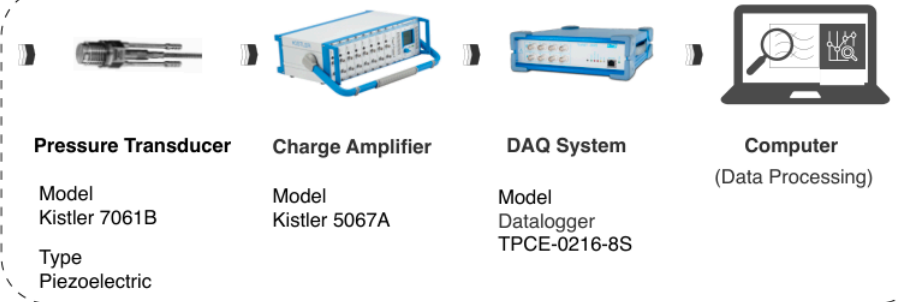

DBI-Measurement Chain

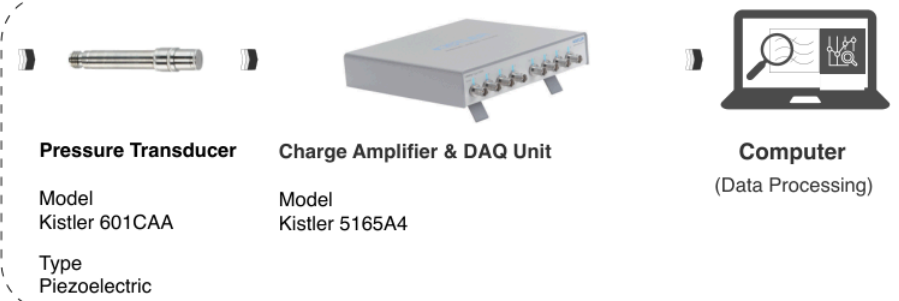


Kistler-Measurement Chain

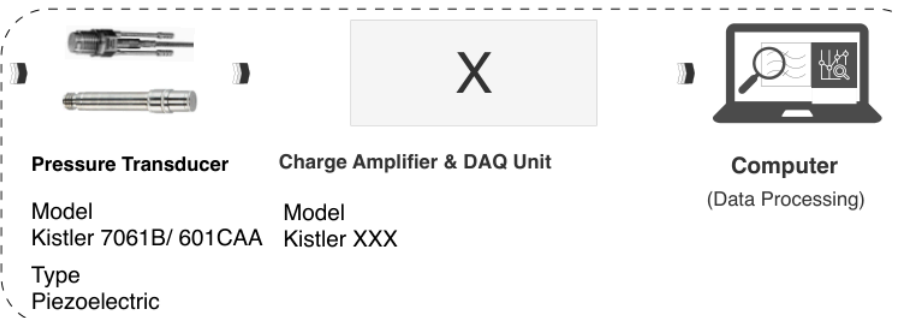

DAQ Reference Diagram - Mixture Sampling Sub-System

Source: frontend/public/MixtureSampling_Sub-System_000.pdf

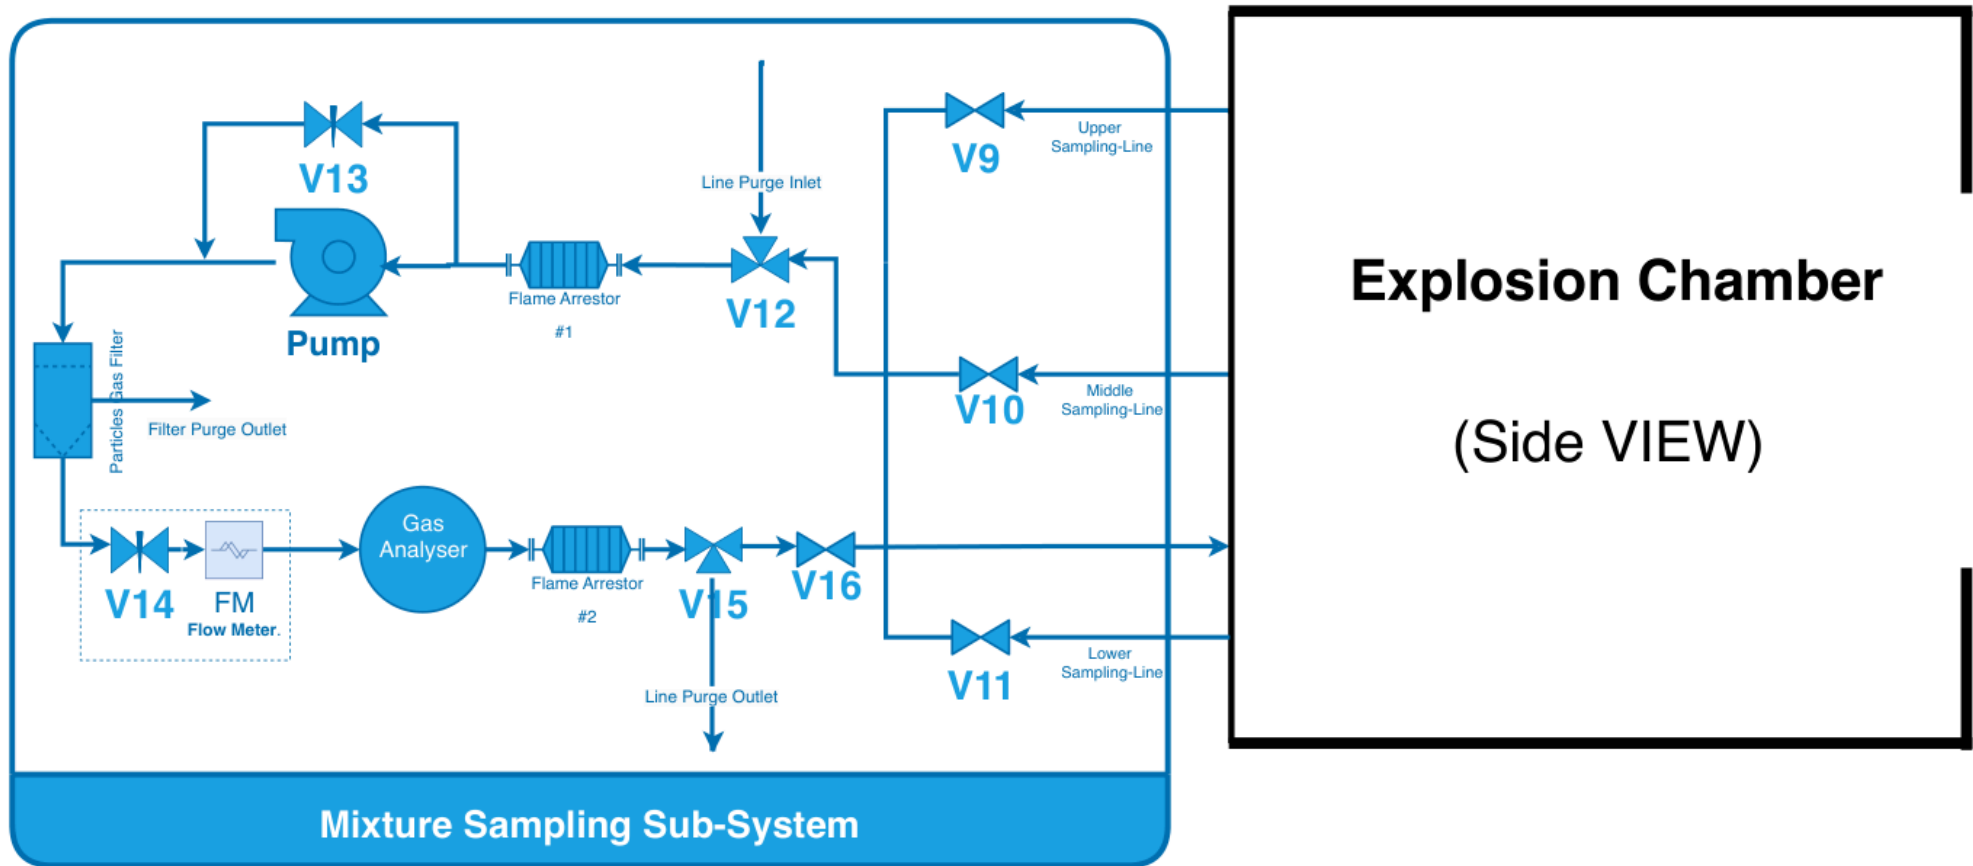

EXDA Sensors Mapping Export

Project: VH2D-Project-Wk-22-2026

Responsible Researcher: PhD Student Javier I. Camacho

Total Groups: 6

Total Sensor IDs: 21

Total Sensor Mappings: 67

Sensor Mounting Reference File: frontend/public/SensorMountingLocation-000.pdf

Generated: 2026-06-06 10:47:49

Group: Prep-Wk22

Group	Sensor	Qty	DAQ	Ch	S/N	Sensitivity	Location	Coord.(x,y,z)m	Mount	Active	Blind	Trig Method	Status
Prep-Wk22	P1	pressure	DAQ-1	CH1	1254024	-80.88 pC/bar	5L	(-0.45,0.399,0.593)	flush	Yes	No	-	Complete
Prep-Wk22	P2	pressure	DAQ-2	CH2	6266801	-37.02 pC/bar	6L	(-0.450,0.403,0.290)	flush	Yes	No	M-Duino	Complete
Prep-Wk22	Trig-1	voltage	DAQ-1	CH5	-	- pC/bar	-	(-, -, -)	N/A	Yes	No	M-Duino	Complete
Prep-Wk22	Trig-2	voltage	DAQ-2	CH4	-	- pC/bar	-	(-, -, -)	N/A	Yes	No	M-Duino	Complete

Group: Verif-Wk22

Group	Sensor	Qty	DAQ	Ch	S/N	Sensitivity	Location	Coord.(x,y,z)m	Mount	Active	Blind	Trig Method	Status
Verif-Wk22	P1	pressure	DAQ-1	CH1	1254024	-80.88 pC/bar	5L swaped to 3L on Verif-04	(0.45,0.593,0.396)	flush	No	No	-	Complete
Verif-Wk22	P2	pressure	DAQ-2	CH1	6266801	-37.02 pC/bar	6L	(0.450,0.290,0.403)	flush	Yes	No	-	Complete
Verif-Wk22	P3	pressure	DAQ-1	CH2	1008977	-81.58 pC/bar	3L swaped to 5L on Verif-04	(-0.45,0.396,0.427)	other	Yes	Yes	-	Complete
Verif-Wk22	P4	pressure	DAQ-2	CH2	6266802	-37.39 pC/bar	4L	(-0.45,0.416,0.447)	flush	Yes	No	-	Complete
Verif-Wk22	P5	pressure	DAQ-1	CH3	1946319	-79.12 pC/bar	3L	(-0.45,0.416,0.447)	flush	Yes	No	-	Complete

Verif-W k22	P6	pressure	DAQ-2	CH3	-	- pC/bar	-	(-, -, -)	flush	Yes	No	-	Incomplete
Verif-W k22	P7	pressure	DAQ-2	CH3	-	- pC/bar	-	(-, -, -)	flush	Yes	No	-	Incomplete
Verif-W k22	P8	pressure	DAQ-3	CH1	-	- pC/bar	-	(-, -, -)	flush	Yes	No	-	Incomplete
Verif-W k22	PP0	pressure	Kistler LabAmp	CH6	-	- pC/bar	-	(0,2,0.68)	flush	Yes	No	-	Incomplete
Verif-W k22	PP15	pressure	Kistler LabAmp	CH7	-	- pC/bar	-	(0,2,0.68)	flush	No	No	-	Incomplete
Verif-W k22	PP30	pressure	Kistler LabAmp	CH8	-	- pC/bar	-	(0,2,0.68)	flush	No	No	-	Incomplete
Verif-W k22	Trig-1	voltage	DAQ-1	CH5	-	- pC/bar	-	(-, -, -)	N/A	Yes	No	M-Duino	Complete
Verif-W k22	Trig-2	voltage	DAQ-2	CH4	-	- pC/bar	-	(-, -, -)	N/A	Yes	No	M-Duino	Complete
Verif-W k22	Trig-3	voltage	DAQ-3	CH2	-	- pC/bar	-	(-, -, -)	N/A	Yes	No	M-Duino	Complete

Group Reference Note: Verification

Group: VH2D-Wk22-01

Group	Sensor	Qty	DAQ	Ch	S/N	Sensitivi-	Location	Coord.(x,y,z)m	Mount	Active	Blind	Trig Method	Status
VH2D-Wk 22-01	P1	pressure	DAQ-1	CH1	1254024	-80.88 pC/bar	5L swaped to 3L on Verif-04	(0.45,0.593,0. 396)	flush	No	No	-	Complete
VH2D-Wk 22-01	P2	pressure	DAQ-2	CH1	6266801	-37.02 pC/bar	6L	(0.450,0.290,0 .403)	flush	Yes	No	-	Complete
VH2D-Wk 22-01	P3	pressure	DAQ-1	CH2	1008977	-81.58 pC/bar	3L swaped to 5L on Verif-04	(-0.45,0.396,0 .427)	flush	Yes	No	-	Complete
VH2D-Wk 22-01	P4	pressure	DAQ-2	CH2	6266802	-37.39 pC/bar	4L	(-0.45,0.416,0 .447)	recessed	Yes	Yes	-	Complete
VH2D-Wk 22-01	P5	pressure	DAQ-1	CH3	1946319	-79.12 pC/bar	3L	(-0.45,0.416,0 .447)	recessed	Yes	Yes	-	Complete
VH2D-Wk 22-01	P6	pressure	DAQ-2	CH3	6266803	-37.66 pC/bar	2L	(-0.450,0.376, 0.447)	recessed	Yes	No	-	Complete

VH2D-Wk 22-01	P7	pressure	DAQ-2	CH4	931538	-80.73 pC/bar	1R	(0.45,0.381,0. 447)	recessed	Yes	No	-	Complete
VH2D-Wk 22-01	P8	pressure	DAQ-3	CH1	6266804	-37.55 pC/bar	4R	(0.450,0.361,0 .433)	recessed	Yes	No	-	Complete
VH2D-Wk 22-01	P9	pressure	DAQ-1	CH1	1008976	-78.79 pC/bar	1L	(-0.45,0.396,0 .467)	recessed	Yes	No	-	Complete
VH2D-Wk 22-01	PP1	pressure	Kistler LabAmp	CH6	-	3264 mV/bar	-	(0,2,0.68)	other	Yes	No	-	Incomplete
VH2D-Wk 22-01	PP2	pressure	Kistler LabAmp	CH7	-	3478 mV/bar	-	(0,2,0.68)	other	No	No	-	Incomplete
VH2D-Wk 22-01	PP3	pressure	Kistler LabAmp	CH8	-	- mV/bar	3461	(0,2,0.68)	other	No	No	M-Duino	Incomplete
VH2D-Wk 22-01	Trig-1	voltage	DAQ-1	CH5	-	- pC/bar	-	(-, -, -)	N/A	Yes	No	M-Duino	Complete
VH2D-Wk 22-01	Trig-2	voltage	DAQ-2	CH4	-	- pC/bar	-	(-, -, -)	N/A	Yes	No	M-Duino	Complete
VH2D-Wk 22-01	Trig-3	voltage	DAQ-3	CH2	-	- pC/bar	-	(-, -, -)	N/A	Yes	No	M-Duino	Complete

Group Reference Note: Vented deflagration concentration series (Hotwire)

=====
Group: VH2D-Wk22-02

Group	Sensor	Qty	DAQ	Ch	S/N	Sensitivi-	Location	Coord.(x,y,z)m	Mount	Active	Blind	Trig Method	Status
VH2D-Wk 22-02	P3	pressure	DAQ-1	CH2	1008977	-81.58 pC/bar	5L	(-0.45,0.396,0 .427)	flush	Yes	No	M-Duino	Complete
VH2D-Wk 22-02	P3-Swap ped DAQ	pressure	DAQ-4	CH1	1008977	-81.58 pC/bar	5L	(-0.45,0.396,0 .427)	flush	Yes	No	M-Duino	Complete
VH2D-Wk 22-02	P7	pressure	DAQ-4	CH1	931538	-80.73 pC/bar	5R	(0.45,0.381,0. 447)	flush	Yes	No	M-Duino	Complete
VH2D-Wk 22-02	P7-Swap ped DAQ	pressure	DAQ-1	CH2	931538	-80.73 pC/bar	5R	(0.45,0.381,0. 447)	flush	Yes	No	M-Duino	Complete
VH2D-Wk 22-02	Trig-1	voltage	DAQ-1	CH5	-	- pC/bar	-	(-, -, -)	N/A	Yes	No	M-Duino	Complete
VH2D-Wk 22-02	Trig-4	voltage	DAQ-4	CH8	-	- pC/bar	-	(-, -, -)	N/A	Yes	No	M-Duino	Complete

Group Reference Note: LU vs Kistler

=====
Group: VH2D-Wk22-03

Group	Sensor	Qty	DAQ	Ch	S/N	Sensitivity	Location	Coord.(x,y,z)m	Mount	Active	Blind	Trig Method	Status
VH2D-Wk 22-03	P2	pressure	DAQ-2	CH1	6266801	-37.02 pC/bar	6L	(0.450,0.290,0 .403)	flush	Yes	No	M-Duino	Complete
VH2D-Wk 22-03	P3	pressure	DAQ-1	CH2	1008977	-81.58 pC/bar	5L	(-0.45,0.396,0 .427)	flush	Yes	No	M-Duino	Complete
VH2D-Wk 22-03	P4	pressure	DAQ-2	CH2	6266802	-37.39 pC/bar	4L	(-0.45,0.416,0 .447)	recessed	Yes	Yes	M-Duino	Complete
VH2D-Wk 22-03	P5	pressure	DAQ-1	CH3	1946319	-79.12 pC/bar	3L	(-0.45,0.416,0 .447)	recessed	Yes	Yes	M-Duino	Complete
VH2D-Wk 22-03	P6	pressure	DAQ-2	CH3	6266803	-37.66 pC/bar	2L	(-0.450,0.376, 0.447)	recessed	Yes	No	M-Duino	Complete
VH2D-Wk 22-03	P7	pressure	DAQ-1	CH4	931538	-80.73 pC/bar	1R	(0.45,0.381,0. 447)	recessed	Yes	No	M-Duino	Complete
VH2D-Wk 22-03	P8	pressure	DAQ-3	CH1	6266804	-37.55 pC/bar	4R	(0.450,0.361,0 .433)	recessed	Yes	No	M-Duino	Complete
VH2D-Wk 22-03	P9	pressure	DAQ-1	CH1	1008976	-78.79 pC/bar	1L	(-0.45,0.396,0 .467)	recessed	Yes	No	M-Duino	Complete
VH2D-Wk 22-03	PP1	pressure	Kistler LabAmp	CH6	6652959	3264 mV/bar	3m60deg	(0,2,0.68)	other	Yes	No	M-Duino	Complete
VH2D-Wk 22-03	PP2	pressure	Kistler LabAmp	CH7	6652961	3478 mV/bar	3m30deg	(0,2,0.68)	other	No	No	M-Duino	Complete
VH2D-Wk 22-03	PP3	pressure	Kistler LabAmp	CH8	6652960	3461 mV/bar	3m0deg	(0,2,0.68)	other	No	No	M-Duino	Complete
VH2D-Wk 22-03	Trig-1	voltage	DAQ-1	CH5	-	- pC/bar	-	(-, -, -)	N/A	Yes	No	M-Duino	Complete
VH2D-Wk 22-03	Trig-2	voltage	DAQ-2	CH4	-	- pC/bar	-	(-, -, -)	N/A	Yes	No	M-Duino	Complete
VH2D-Wk 22-03	Trig-3	voltage	DAQ-3	CH2	-	- pC/bar	-	(-, -, -)	N/A	Yes	No	M-Duino	Complete

Group Reference Note: Vented deflagration concentration series (Hotwire) LU vs DBI

=====
Group: VH2D-Wk22-04

Group	Sensor	Qty	DAQ	Ch	S/N	Sensitivity	Location	Coord.(x,y,z)m	Mount	Active	Blind	Trig Method	Status
VH2D-Wk 22-04	P2	pressure	DAQ-2	CH1	6266801	-37.02 pC/bar	6L	(0.450,0.290,0 .403)	flush	Yes	No	-	Complete
VH2D-Wk 22-04	P3	pressure	DAQ-1	CH2	1008977	-81.58 pC/bar	5L	(-0.45,0.396,0 .427)	flush	Yes	No	-	Complete


VH2D-Wk 22-04	P4	pressure	DAQ-2	CH2	6266802	-37.39 pC/bar	4L	(-0.45,0.416,0 .447)	recessed	Yes	Yes	-	Complete
VH2D-Wk 22-04	P5	pressure	DAQ-1	CH3	1946319	-79.12 pC/bar	3L	(-0.45,0.416,0 .447)	recessed	Yes	Yes	-	Complete
VH2D-Wk 22-04	P6	pressure	DAQ-2	CH3	6266803	-37.66 pC/bar	2L	(-0.450,0.376, 0.447)	recessed	Yes	No	-	Complete
VH2D-Wk 22-04	P7	pressure	DAQ-1	CH4	931538	-80.73 pC/bar	1R	(0.45,0.381,0. 447)	recessed	Yes	No	-	Complete
VH2D-Wk 22-04	P8	pressure	DAQ-3	CH1	6266804	-37.55 pC/bar	4R	(0.450,0.361,0 .433)	recessed	Yes	No	-	Complete
VH2D-Wk 22-04	P9	pressure	DAQ-1	CH1	1008976	-78.79 pC/bar	1L	(-0.45,0.396,0 .467)	recessed	Yes	No	-	Complete
VH2D-Wk 22-04	PP1	pressure	Kistler LabAmp	CH6	6652959	3264 mV/bar	3m	(0,2,0.68)	other	Yes	No	-	Complete
VH2D-Wk 22-04	PP2	pressure	Kistler LabAmp	CH7	6652961	3478 mV/bar	5m	(0,2,0.68)	other	No	No	-	Complete
VH2D-Wk 22-04	PP3	pressure	Kistler LabAmp	CH8	6652960	3461 mV/bar	7m	(0,2,0.68)	other	No	No	-	Complete
VH2D-Wk 22-04	Trig-1	voltage	DAQ-1	CH5	-	- pC/bar	-	(-, -, -)	N/A	Yes	No	M-Duino	Complete
VH2D-Wk 22-04	Trig-2	voltage	DAQ-2	CH4	-	- pC/bar	-	(-, -, -)	N/A	Yes	No	M-Duino	Complete
VH2D-Wk 22-04	Trig-3	voltage	DAQ-3	CH2	-	- pC/bar	-	(-, -, -)	N/A	Yes	No	M-Duino	Complete

Group Reference Note: Vented deflagration concentration series (Hotwire) LU vs DBI

Sensor Mounting Reference Diagram

Source: frontend/public/SensorMountingLocation-000.pdf

Pressure Sensor Location Mapping Overview

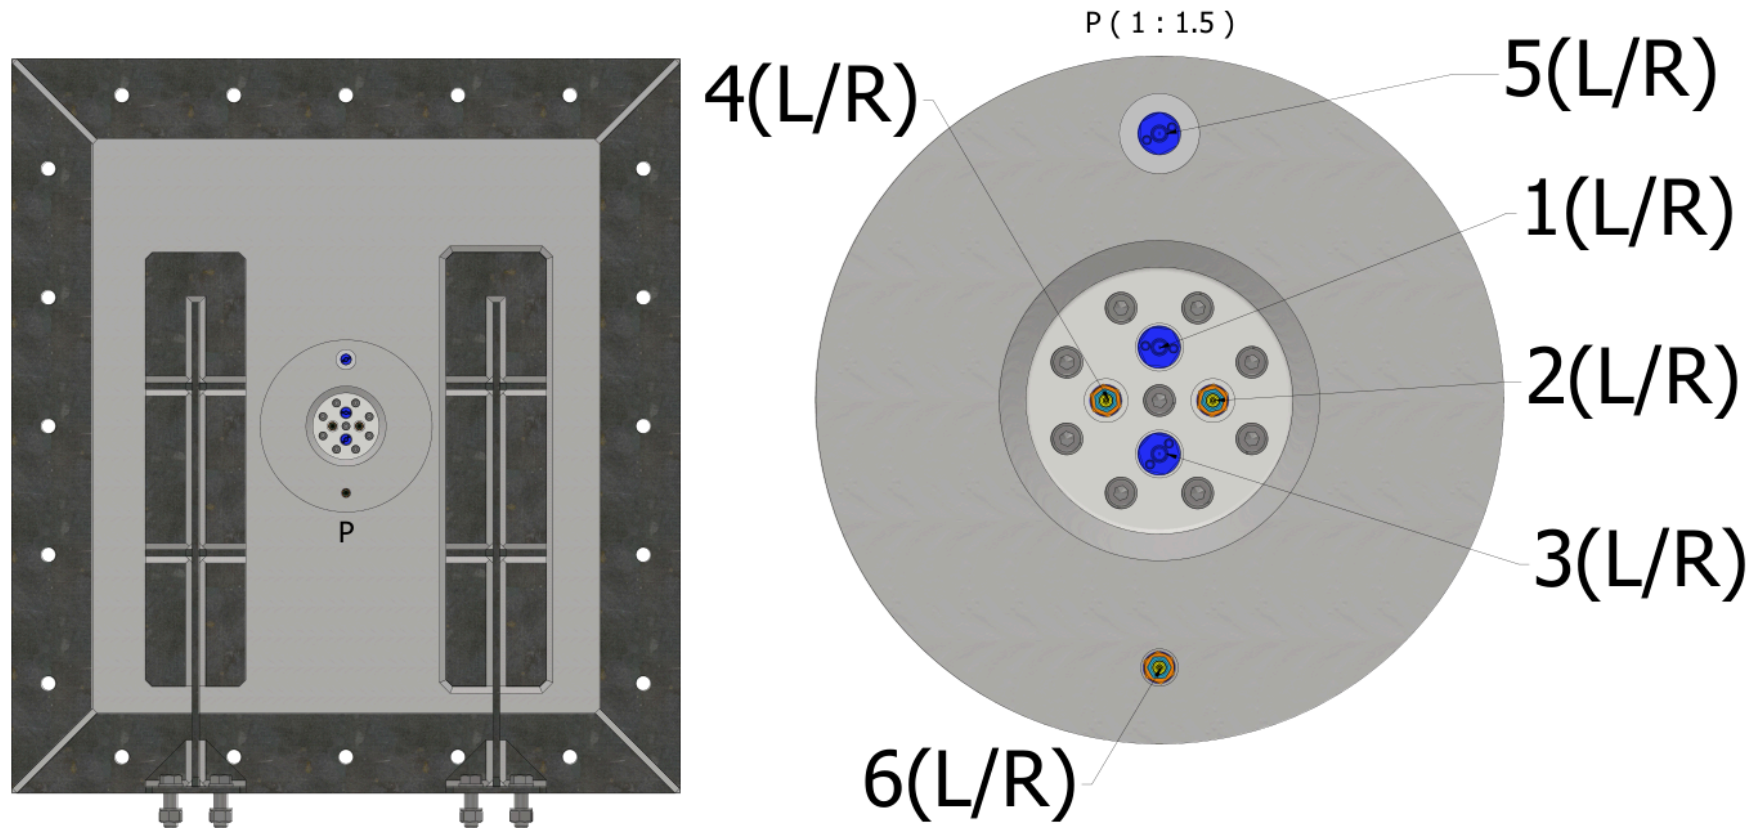

EXDA Gas Mixing Export

Project: VH2D-Project-Wk-22-2026

Responsible Researcher: PhD Student Javier I. Camacho

Total Records: 25

Generated: 2026-06-06 10:47:50

MATLAB Verified: Yes

Verification File A: scripts/GasMixingVerificationFiles/H2_MFC_Fill_Calculator_v000.m

Verification File B: scripts/GasMixingVerificationFiles/AuxFcn_H2_MFC_FillCalculator_000.m

Shared Chamber Setup (applies to all runs unless noted otherwise):

L=0.900 m, W=0.900 m, H=0.900 m, Pipes+=VARIES m³, Hotwire+=0.000 m³, Welded-=0.000 m³, Bolts-=0.000 m³, Vcorr=VARIES L

Note: setup values vary across runs; detailed per-run setup table is included below.

Core Gas Mixing Results

Group	Run/Test	H2%	RH%	Pch(Pa)	Tch(K)	H2est(g)	H2corr(g)	H2inj(L)	MFC	t(s)	t(min)	Model	Basis	a
Prep-Wk22	Prep-Wk22-01	13.50	-	101325	292.15	8.276	Not corrected by model	98.41	20.00	301.3	5.0	-	-	-
Verif-Wk22	Verif-Wk22-01	13.50	-	101325	294.25	8.217	Not corrected by model	98.42	20.00	299.2	5.0	-	-	-
Verif-Wk22	Verif-Wk22-02	14.00	-	101325	293.15	9.384	Not corrected by model	111.97	20.00	334.8	5.6	-	-	-
Verif-Wk22	Verif-Wk22-03	16.00	-	101325	294.15	10.638	Not corrected by model	127.37	20.00	387.3	6.5	-	-	-
Verif-Wk22	Verif-Wk22-04	18.00	-	101325	291.65	12.070	Not corrected by model	143.29	20.00	439.5	7.3	-	-	-
VH2D-Wk22-01	VH2D-Wk22-01-01	16.00	-	101325	293.15	10.674	Not corrected by model	127.37	20.00	388.6	6.5	-	-	-
VH2D-Wk22-01	VH2D-Wk22-01-02	16.00	-	101325	292.05	10.714	Not corrected by model	127.37	20.00	390.1	6.5	-	-	-
VH2D-Wk22-01	VH2D-Wk22-01-03	18.00	-	101325	291.35	12.083	Not corrected by model	143.29	20.00	439.9	7.3	-	-	-

VH2D-Wk22-01	VH2D-Wk22-01-04	18.00	-	101325	290.85	12.103	Not corrected by model	143.29	20.00	440.7	7.3	-	-	-
VH2D-Wk22-01	VH2D-Wk22-01-05	19.00	-	101325	290.55	12.789	Not corrected by model	151.26	20.00	465.6	7.8	-	-	-
VH2D-Wk22-01	VH2D-Wk22-01-07	20.00	-	101325	290.56	13.462	Not corrected by model	159.22	20.00	490.1	8.2	-	-	-
VH2D-Wk22-02	VH2D-Wk22-02-01	18.00	-	101325	289.95	12.141	12.278	143.29	20.00	447.0	7.5	linear_	fractio	69
VH2D-Wk22-02	VH2D-Wk22-02-02	18.00	-	101325	291.15	12.091	12.278	143.29	20.00	447.0	7.5	linear_	fractio	69
VH2D-Wk22-02	VH2D-Wk22-02-03	20.00	-	101325	293.15	13.343	13.671	159.22	20.00	497.7	8.3	linear_	fractio	69
VH2D-Wk22-02	VH2D-Wk22-02-04	20.00	-	101325	292.15	13.388	13.671	159.22	20.00	497.7	8.3	linear_	fractio	69
VH2D-Wk22-03	VH2D-Wk22-03-01	18.00	-	101325	292.45	12.037	12.278	143.29	20.00	447.0	7.5	linear_	fractio	69
VH2D-Wk22-03	VH2D-Wk22-03-02	18.00	-	101325	292.25	12.045	12.278	143.29	20.00	447.0	7.5	linear_	fractio	69
VH2D-Wk22-03	VH2D-Wk22-03-03	20.00	-	101325	292.15	13.388	13.671	159.22	20.00	497.7	8.3	linear_	fractio	69
VH2D-Wk22-03	VH2D-Wk22-03-04	20.00	-	101325	291.65	13.411	13.671	159.22	20.00	497.7	8.3	linear_	fractio	69
VH2D-Wk22-03	VH2D-Wk22-03-05	20.00	-	101325	291.45	13.421	13.671	159.22	20.00	497.7	8.3	linear_	fractio	69
VH2D-Wk22-04	VH2D-Wk22-04-01	16.00	-	101325	291.75	10.725	10.885	127.37	20.00	396.3	6.6	linear_	fractio	69
VH2D-Wk22-04	VH2D-Wk22-04-02	16.00	-	101325	292.75	10.689	10.885	127.37	20.00	396.3	6.6	linear_	fractio	69
VH2D-Wk22-04	VH2D-Wk22-04-03	21.00	-	101325	293.05	14.015	14.367	167.18	20.00	523.1	8.7	linear_	fractio	69
VH2D-Wk22-04	VH2D-Wk22-04-04	21.00	-	101325	293.75	13.981	14.367	167.18	20.00	523.1	8.7	linear_	fractio	69
VH2D-Wk22-04	VH2D-Wk22-04-05	12.00	-	101325	295.05	7.954	8.100	95.53	10.00	589.8	9.8	linear_	fractio	69

Per-Run Chamber Setup (because values vary)

Group	Run/Test	L (m)	W (m)	H (m)	Pipes+ (m3)	Hotwire+ (m3)	Welded- (m3)	Bolts- (m3)	Vcorr(L)	Notes
Prep-Wk22	Prep-Wk22-01	0.900	0.900	0.900	0.000	0.000	0.000	0.000	729.00	-
Verif-Wk22	Verif-Wk22-01	0.900	0.900	0.900	0.000	0.000	0.000	0.000	729.00	-
Verif-Wk22	Verif-Wk22-02	0.900	0.900	0.900	0.071	0.000	0.000	0.000	799.80	-
Verif-Wk22	Verif-Wk22-03	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-
Verif-Wk22	Verif-Wk22-04	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-
VH2D-Wk22	VH2D-Wk22-01	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-
VH2D-Wk22	VH2D-Wk22-01	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-
VH2D-Wk22	VH2D-Wk22-01	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-
VH2D-Wk22	VH2D-Wk22-01	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-
VH2D-Wk22	VH2D-Wk22-01	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-
VH2D-Wk22	VH2D-Wk22-01	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-
VH2D-Wk22	VH2D-Wk22-02	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-
VH2D-Wk22	VH2D-Wk22-02	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-

VH2D-Wk22.	VH2D-Wk22-02-.	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-	
VH2D-Wk22.	VH2D-Wk22-02-.	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-	
VH2D-Wk22.	VH2D-Wk22-03-.	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-	
VH2D-Wk22.	VH2D-Wk22-03-.	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-	
VH2D-Wk22.	VH2D-Wk22-03-.	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-	
VH2D-Wk22.	VH2D-Wk22-03-.	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-	
VH2D-Wk22.	VH2D-Wk22-03-.	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-	
VH2D-Wk22.	VH2D-Wk22-04-.	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-	
VH2D-Wk22.	VH2D-Wk22-04-.	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-	
VH2D-Wk22.	VH2D-Wk22-04-.	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-	
VH2D-Wk22.	VH2D-Wk22-04-.	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-	
VH2D-Wk22.	VH2D-Wk22-04-.	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-	
VH2D-Wk22.	VH2D-Wk22-04-.	0.900	0.900	0.900	0.067	0.000	0.000	0.000	796.08	-	MFC set to 7.954 g (12
											vol.%) but stopped at vol.
											8% at location measured by
											H2CM. This was the initial
											plan, but the total hydrogen
											mass was injected.