

2nd Item Number	Shelf Days	Text Line 01	Text Line 02	Text Line 03	Text Line 04	Text Line 05	Text Line 06	Text Line 07	Text Line 08	Text Line 09	Text Line 10	Text Line 11	Text Line 20
Item Number	Shelf Life	Nom Volume	Max Volume	Diameter	Label Item P/N	Height	Projection	Width	Tolerance	Saline Vol	Gel Volume	Max Projection	GTIN
3340902	1825	165cc	-	-	334-0902	8.5cm	4.6cm	9.0cm	-	-	-	-	00081317005148
3340952	1825	195cc	-	-	334-0952	8.9cm	4.8cm	9.5cm	-	-	-	-	00081317005155
3341002	1825	225cc	-	-	334-1002	9.4cm	5.1cm	10.0cm	-	-	-	-	00081317005162
3341052	1825	260cc	-	-	334-1052	9.9cm	5.3cm	10.5cm	-	-	-	-	00081317005179
3341102	1825	300cc	-	-	334-1102	10.3cm	5.6cm	11.0cm	-	-	-	-	00081317005186
3341152	1825	345cc	-	-	334-1152	10.8cm	5.8cm	11.5cm	-	-	-	-	00081317005193
3341202	1825	390cc	-	-	334-1202	11.3cm	6.0cm	12.0cm	-	-	-	-	00081317005209
3341252	1825	440cc	-	-	334-1252	11.8cm	6.2cm	12.5cm	-	-	-	-	00081317005216
3341302	1825	495cc	-	-	334-1302	12.2cm	6.5cm	13.0cm	-	-	-	-	00081317005223
3341352	1825	555cc	-	-	334-1352	12.7cm	6.7cm	13.5cm	-	-	-	-	00081317005230
3341402	1825	620cc	-	-	334-1402	13.2cm	6.9cm	14.0cm	-	-	-	-	00081317005247
3341452	1825	685cc	-	-	334-1452	13.6cm	7.1cm	14.5cm	-	-	-	-	00081317005254

1 - Remove LPNBR & Latex Symbols throughout



Through out replace MENTOR (R) to MENTOR(TM)

REVISIONS				
REV	C.O.	DESCRIPTION	DRAWN	DATE
A	15031	RELEASED FOR PRODUCTION	WP	10/15/10
B	PLM	REVISED PER C.O.	WP	SEE PLM
C	PLM	REVISED PER C.O.	WP	SEE PLM
D	PLM	For ISO 14607:2024 Standard	TBD	PLM

LAST SAVED BY: wpcd ON Tuesday March 07, 2017 9:42:49 AM



THERMOFORM LABEL [EART 107503-001]

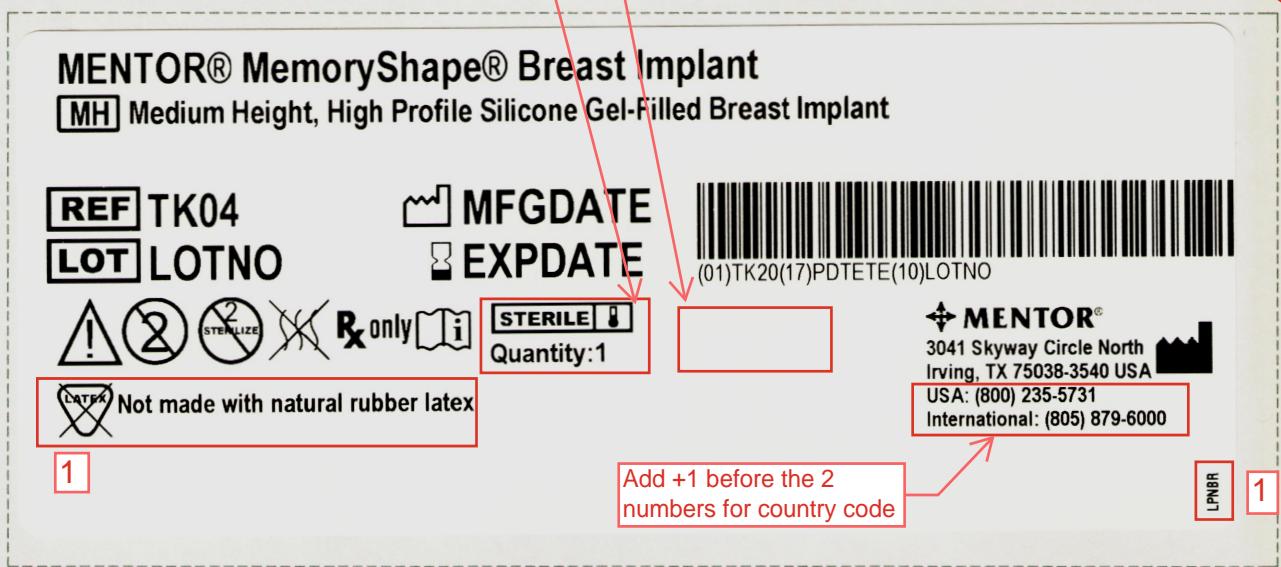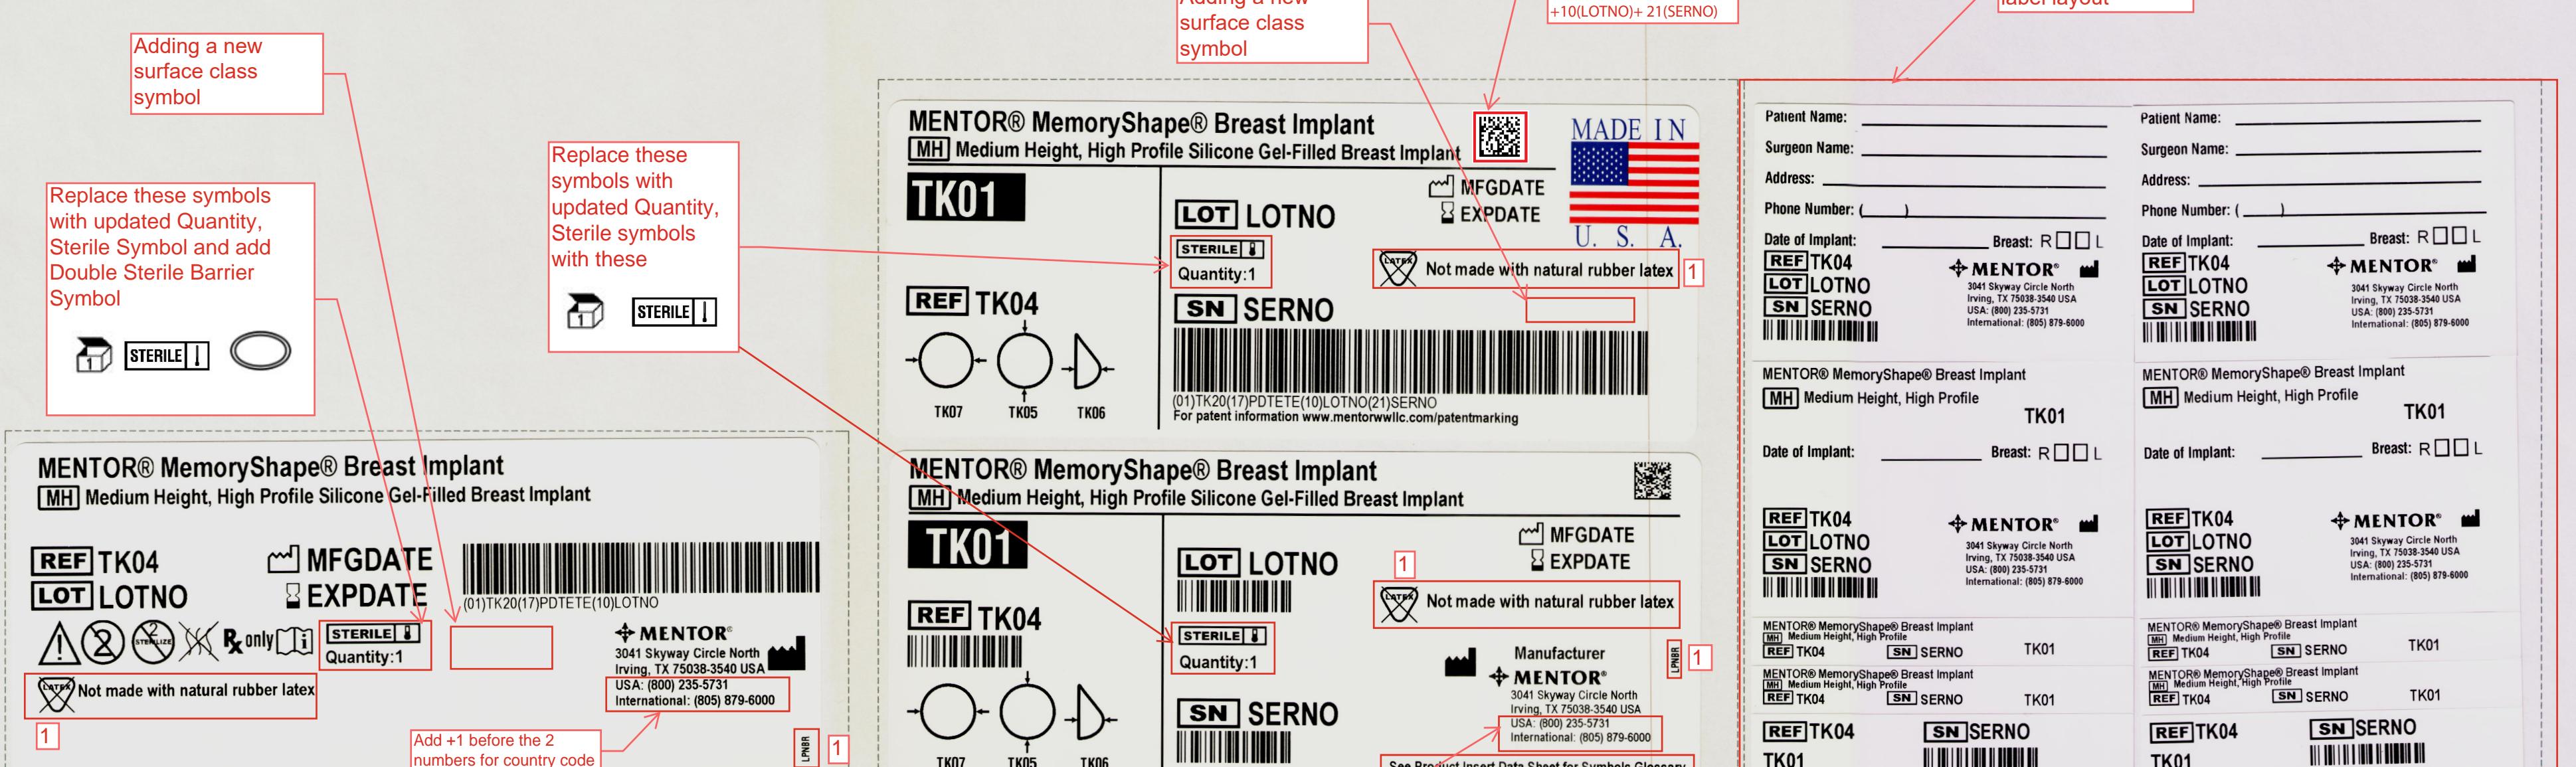


OUTER LID LABEL [EART 107503-005]

- MFG INSPECT PER QCIC000163
- FIRST ARTICLE INSPECT PER QCIC000001
- OTHER FIELDS
LOTNO = LOT NUMBER
SERNO = SERIAL NUMBER
MFGDATE = MANUFACTURING DATE
EXPDATE = EXPIRATION DATE
- ALL OF THE VARIABLE TEXT IS DISPLAYED AS ITS FIELD NAME.
THE SPECIFIC DATA TO BE INSERTED INTO THESE FIELDS IS DOCUMENTED IN THE MATRIX OF THIS PRINTED LABEL DRAWING.

5. 2D barcode contains : 01(TK20)+17(EXPDATE)+11(MFGDATE)+10(LOTNO)+ 21(SERNO) on the flag label, non-flag label and Patient stickers in the combo labels



COMBO LABEL (SET) [EART 107503-004]

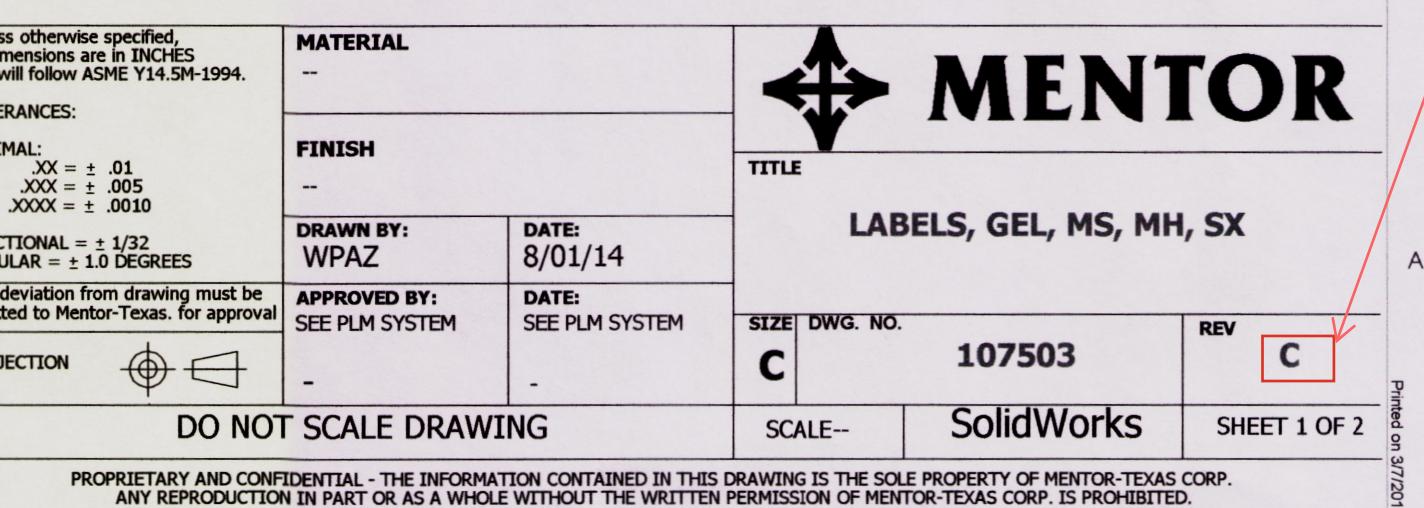

Revision Change as per the Drawing update

Printed on 3/7/2017

8
7
6
5
4

1 - Remove LPNBR & Latex Symbols throughout

Through out replace MENTOR (R) to
MENTOR(TM)

Replace these symbols with updated Quantity, Sterile Symbol and add Double Sterile Barrier Symbol

**OUTER LID LABEL
[EART 107503-010]**

MENTOR® MemoryShape® Breast Implant
MH Medium Height, High Profile Silicone Gel-Filled Breast Implant

REF TK04 **SN** SERNO **MFGDATE** **EXPDATE**

STERILE **Quantity:1**

(01)TK20(17)PDTETE(21)SERNO

! **STERILIZE** Rx only **LATEX** Not made with natural rubber latex

1

Adding a new

MENTOR®
3041 Skyway Circle North
Irving, TX 75038-3540 USA
USA: (800) 235-5731
International: (805) 879-6000

1

**THERMOFORM LABEL
[EART 107503-006]**

SN SERNO
LOT LOTNO
REF TK04
TK01

**CARTON END LABEL
[EART 107503-007]**

MENTOR® MemoryShape® Breast Implant
MH Medium Height, High Profile Silicone Gel-Filled Breast Implant

TK01

REF TK04

TK05

TK06

LOT **LOTNO**

STERILE



Quantity: 1

SN **SERNO**

Not made with natural rubber latex

1

(01)TK20(17)PDTETE(10)LOTNO(21)SERNO
For patent information www.mentorwwllc.com/patentmarking

Patient Name:	<hr/>	Patient Name:	<hr/>
Surgeon Name:	<hr/>	Surgeon Name:	<hr/>
Address:	<hr/>	Address:	<hr/>
Phone Number:	(<hr/>)	Phone Number:	(<hr/>)
Date of Implant:	<hr/> Breast: R <input type="checkbox"/> <input checked="" type="checkbox"/> L	Date of Implant:	<hr/> Breast: R <input type="checkbox"/> <input checked="" type="checkbox"/> L
REF	TK04	REF	TK04
LOT	LOTNO	LOT	LOTNO
SN	SERNO	SN	SERNO
			
MENTOR® Mammoplasty System		MENTOR® Mammoplasty System	

**CARTON END LABEL
PART 107503-0081**

MENTOR® MemoryShape® Breast Implant
MH Medium Height, High Profile Silicone Gel-Filled Breast Implant

TK01

REF TK04

LOT **LOTNO** **1**

MFGDATE
EXPDATE

STERILE **Quantity: 1**


SN **SERNO**

LATEX Not made with natural rubber latex

Manufacturer
MENTOR
3041 Skyway Circle North
Irving, TX 75038-3540 USA
USA: (800) 235-5731
International: (805) 879-6000

See Product Insert Data Sheet for Symbols Glossary

Add +1 before the numbers for count

CORD (SET) 603-009]		Date of Implant: _____ Breast: R <input type="checkbox"/> <input checked="" type="checkbox"/> L	Date of Implant: _____ Breast: R <input type="checkbox"/> <input checked="" type="checkbox"/> L
REF TK04 LOT LOTNO SN SERNO 		 MENTOR® 3041 Skyway Circle North Irving, TX 75038-3540 USA USA: (800) 235-5731 International: (805) 879-6000	
MENTOR® MemoryShape® Breast Implant MH Medium Height, High Profile REF TK04 SN SERNO TK01		MENTOR® MemoryShape® Breast Implant MH Medium Height, High Profile REF TK04 SN SERNO TK01	
MENTOR® MemoryShape® Breast Implant MH Medium Height, High Profile REF TK04 SN SERNO TK01		MENTOR® MemoryShape® Breast Implant MH Medium Height, High Profile REF TK04 SN SERNO TK01	
REF TK04 TK01		REF TK04 TK01	

Revision Change as per
the Drawing update

Unless otherwise specified, all dimensions are in INCHES and will follow ASME Y14.5M-1994.		MATERIAL --		 MENTOR
TOLERANCES:		FINISH --		
DECIMAL: .XX = ± .01 .XXX = ± .005 .XXXX = ± .0005 FRACTIONAL = ± 1/32 ANGULAR = ± 1.0 DEGREES		DRAWN BY: WPAZ	DATE: 08/01/14	TITLE LABELS, GEL, MS, MH, SX
Any deviation from drawing must be submitted to Mentor-Texas for approval		APPROVED BY: SEE PLM SYSTEM	DATE: SEE PLM SYSTEM	SIZE C DRAWING NO. 107503 REV C
PROJECTION				
DO NOT SCALE DRAWING			SCALE=1:1	SolidWorks
PROPRIETARY AND CONFIDENTIAL - THE INFORMATION CONTAINED IN THIS DRAWING IS THE SOLE PROPERTY OF MENTOR-TEXAS CORP. ANY REPRODUCTION IN PART OR AS A WHOLE WITHOUT THE WRITTEN PERMISSION OF MENTOR-TEXAS CORP. IS PROHIBITED.				