

Certificate of Analysis

Nova Cell Peptides
Nova Cell Peptides
NCBL Sciences OÜ
Estonia
info@novacell-peptides.com

Liquilabs s.r.o.
Inovační 122
252 41 Zlatníky-Hodkovice
Czechia
www.liquilabs.cz



[Verify Results Online](#)

Sample Identification

Sample Name KLOW Blend 80 mg
Batch Number KL-042603
Date Published 2026-06-23 12:15

Results for LYO-0230

Peptides	Result	Unit	Uncertainty	Acceptable Range
BPC-157 Assay Peptide Screening 0.1% TFA	10.89	mg	[± 0.05]	
GHK-Cu Assay Peptide Screening 0.1% TFA	67.6	mg	[± 0.3]	
KPV Assay Peptide Screening 0.1% TFA	9.73	mg	[± 0.05]	
BPC-157 Purity Peptide Screening 0.1% TFA	> 99.8	%		
GHK-Cu Purity Peptide Screening 0.1% TFA	> 99.8	%		
KPV Purity Peptide Screening 0.1% TFA	> 99.8	%		
BPC-157 Identification by RT Peptide Screening 0.1% TFA	0.996		[± 0.005]	
GHK-Cu Identification by RT Peptide Screening 0.1% TFA	0.997		[± 0.005]	
KPV Identification by RT Peptide Screening 0.1% TFA	0.996		[± 0.005]	
Thymosin Beta 4 (TB-500) Assay Peptide Screening 0.1% TFA	12.39	mg	[± 0.06]	
Thymosin Beta 4 (TB-500) Purity Peptide Screening 0.1% TFA	> 99.8	%		
Thymosin Beta 4 (TB-500) Identification by RT Peptide Screening 0.1% TFA	0.995		[± 0.005]	
Mass Spectrometry	Result	Unit	Uncertainty	Acceptable Range
Molecular Ion Mass Identification (BPC-157) Mass Spectrometry Identity	1418	Da	[± 1]	
Molecular Ion Mass Identification (GHK-Cu) Mass Spectrometry Identity	341	Da	[± 1]	
Molecular Ion Mass Identification (KPV) Mass Spectrometry Identity	342	Da	[± 1]	
Molecular Ion Mass Identification (TB-500) Mass Spectrometry Identity	4963	Da	[± 1]	

Analysis Report




Sample Information


Injection Volume : 0,5
Data File : LYO-0230_008.lcd
Method File : Peptide screening_202602_Polar_Blend A.lcm
Date Acquired : 12.06.2026 16:55:49

Chromatogram

uAU

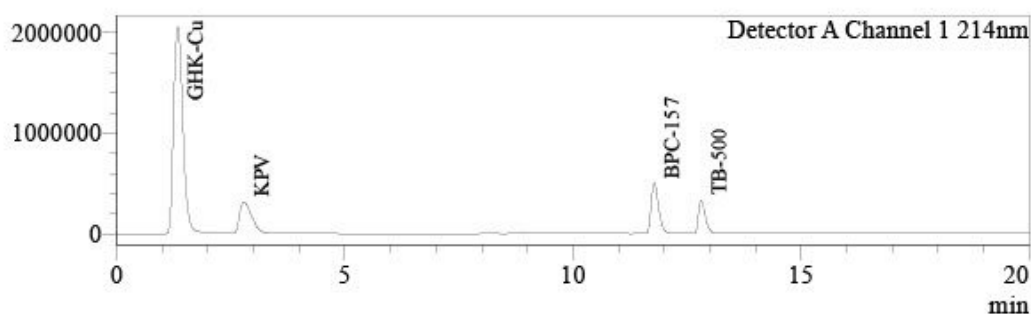

uAU

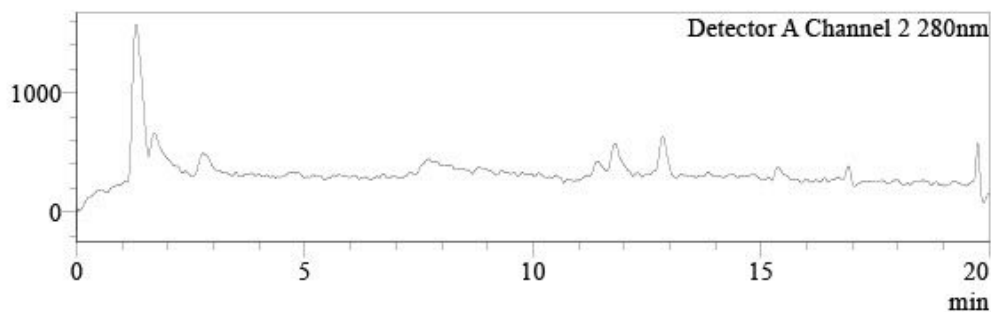

Peak Table

Detector A Channel 1 214nm

Peak#	Name	Ret. Time	Conc.	Unit	Area%
1	GHK-Cu	1.341	67.642	mg/L	66.241
2	KPV	2.789	9.733	mg/L	13.102
3	BPC-157	11.781	10.829	mg/L	12.888
4	TB-500	12.810	12.389	mg/L	7.769
Total					100,000

Peak Table

Detector A Channel 2 280nm


Peak#	Name	Ret. Time	Conc.	Unit
Total				

Qualitative Analysis Report



Sample Information

Injection Volume	: 2
Data File	: LYO-0230_015.lcd
Method File	: Peptide screening_V7.lcm
Date Acquired	: 6/12/2026 5:17:27 PM

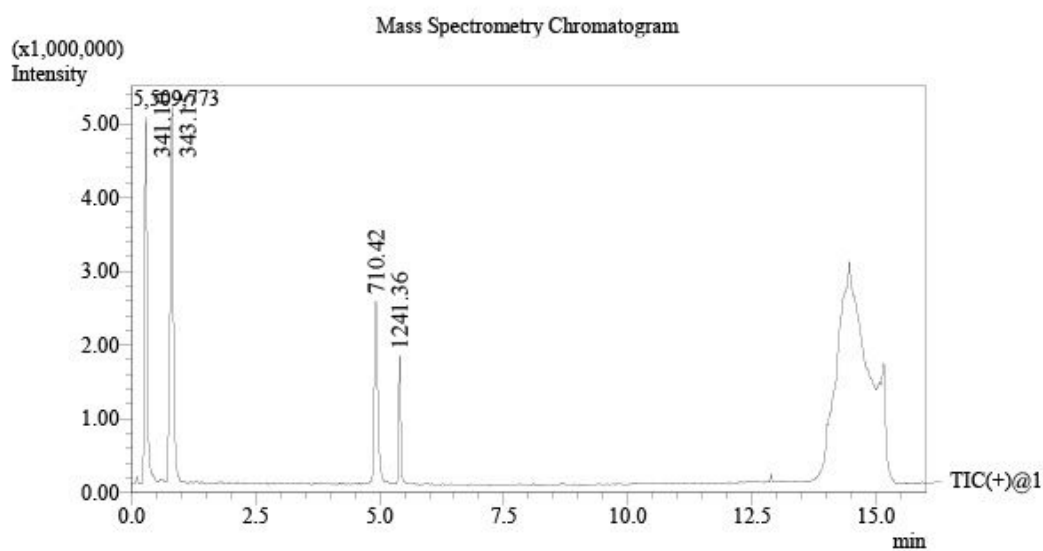


Substance Identification

Detected substance

Ret.Time: 0.210

Base Peak: 341.1 Da

Scan Range: 280.00 - 2000.00 Polarity: Positive

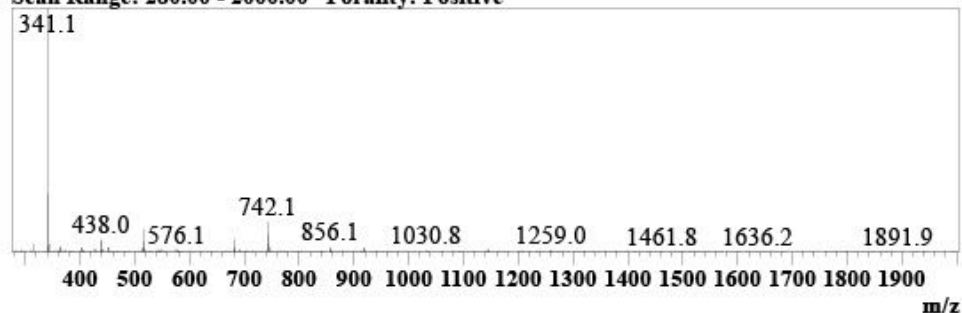

Identified Substance


Compound Name: GHK-Cu

Similarity: 94%

Formula: C₁₄H₂₄CuN₆O₄

CAS: 49557-75-7

Mol.Weight: 401 Da

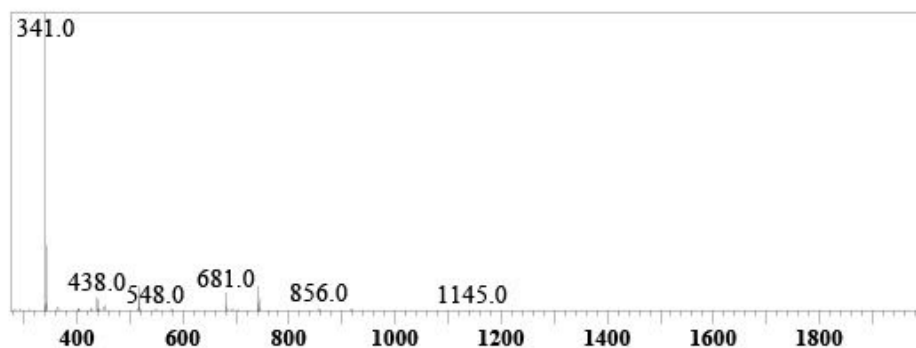


Detected substance

Ret.Time: 0.706

Base Peak: 343.1 Da

Scan Range: 280.00 - 2000.00 Polarity: Positive

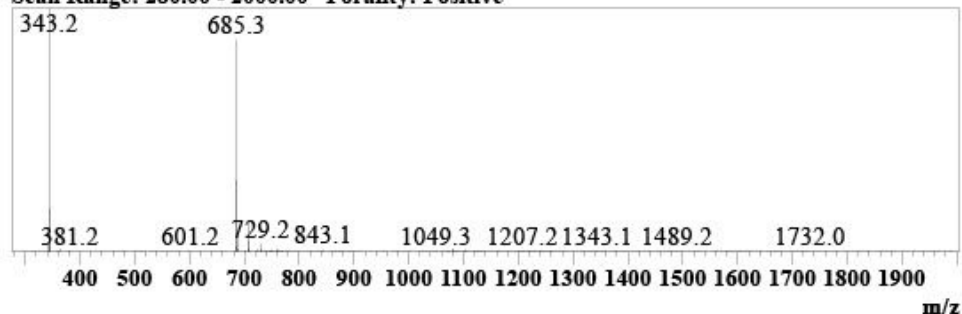

Identified Substance


Compound Name: KPV



Similarity: 97%

Formula: C₁₆H₃₀N₄O₄

CAS: 67727-97-3

Mol.Weight: 342 Da

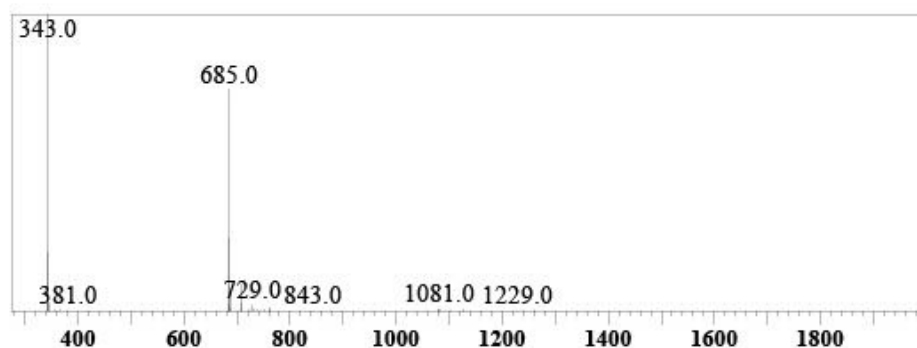

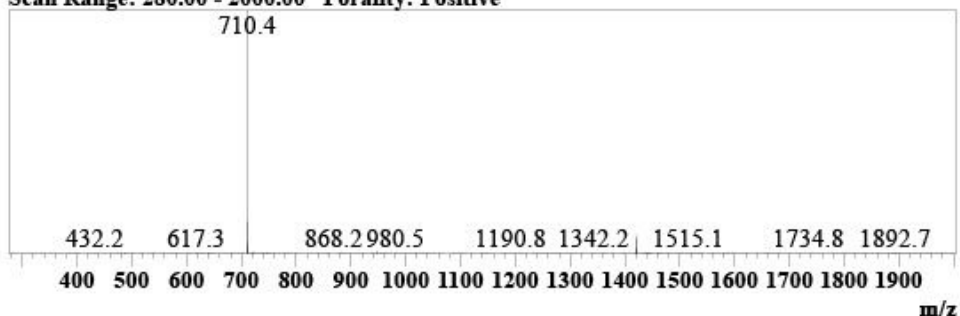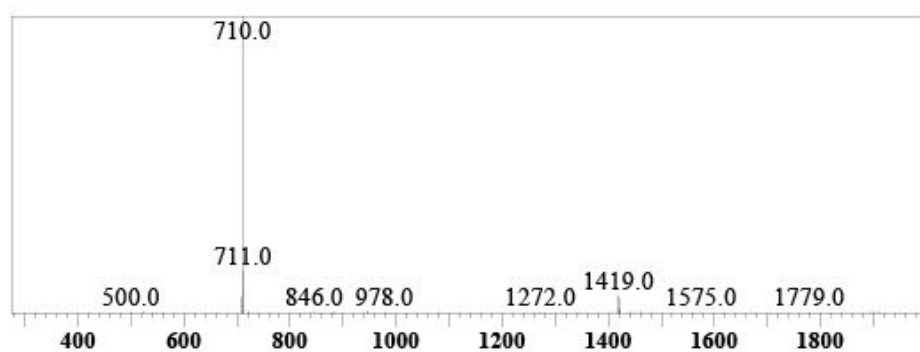
Detected substance**Ret.Time: 4.836****Base Peak: 710.4 Da****Scan Range: 280.00 - 2000.00 Polarity: Positive****Identified Substance****Compound Name: BPC-157****Similarity: 96%****Formula: C₆₂H₉₈N₁₆O₂₂****CAS: 137525-51-0****Mol.Weight: 1418 Da**

Detected substance

Ret.Time: 5.338

Base Peak: 1241.4 Da

Scan Range: 280.00 - 2000.00 Polarity: Positive

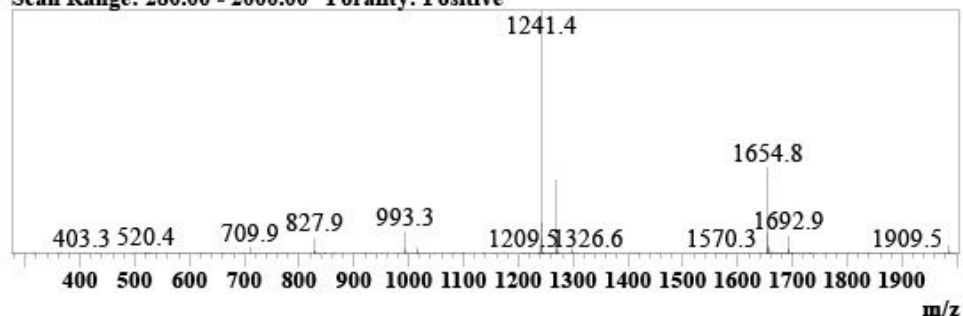

Identified Substance


Compound Name: Thymosin Beta 4

Similarity: 87%

Formula: C₂₁₂H₃₅₀N₅₆O₇₈S

CAS: 77591-33-4

Mol.Weight: 4963 Da

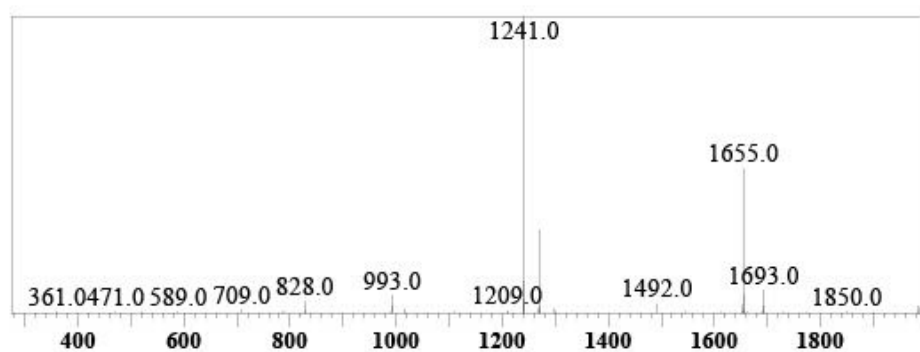

Responsibles



Mr. Ján Galbavý
CEO

Analysis results relate only to the samples tested.

This document shall not be reproduced except in full, without the written approval of Liquilabs s.r.o.