PHILIPS

OmniWire

Pressure guide wire

Models:
89185/89185J



Instructions for use

Symbol; Símbolo; Símbolo; 符號; 符号	Standard; Estándar; Norma; 標準; 标准	Reference; Referencia; Referência; 參考編號; 参考	Name; Nombre; Títulos; 標題; 标题	Description; Descripción; Descrição; 說明; 说明
	ISO 15223-1	5.1.5	Batch code; Código de lote; Código do lote; 批號; 批次代码	Indicates the manufacturer's batch code so that the batch or lot can be identified.; Indica el código de lote del fabricante para que el lote pueda ser identificado.; Indica o código de lote do fabricante para possibilitar a respetiva identificação.; 表示製造商的批號，以供識別批次。; 指示制造商的批次代码，可由此识别批次。
	ISO 15223-1	5.1.6	Catalog number; Número de catálogo; Número de catálogo; 貨號; 产品目录号	Indicates the manufacturer's catalogue number so that the medical device can be identified.; Indica el número de catálogo del fabricante para que el dispositivo médico pueda ser identificado.; Indica o número de catálogo do fabricante para possibilitar a identificação do dispositivo médico.; 表示製造商的貨號，以供識別醫療設備。; 指示制造商的产品目录号，可由此识别医疗设备。
	ISO 15223-1	5.1.7	Serial number; Número de serie; Número de série.; 序號; 序列号	Indicates the manufacturer's serial number so that a specific medical device can be identified.; Indica el número de serie del fabricante para que se pueda identificar un dispositivo médico específico.; Indica o número de série do fabricante para possibilitar a identificação de um dispositivo médico específico.; 表示製造商的序號，以供識別特定的醫療設備。; 指示制造商的序列号，可由此识别具体的医疗设备。
	ISO 15223-1	5.1.1	Manufacturer/Manufactured for; Fabricante/Fabricado para; Fabricante/ Fabricado para; 製造商/廠商; 制造商/ 经销商	Indicates the medical device manufacturer, as defined in EU Directives 90/385/EEC, 93/42/EEC and 98/79/EC.; Indica el fabricante del dispositivo médico, como se define en las Directivas 90/385/CEE, 93/42/CEE y 98/79/CE.; Indica o fabricante do dispositivo médico, conforme definido nas Diretivas 90/385/CEE, 93/42/CEE e 98/79/CE da UE.; 表示依 EU 指令 90/385/EEC、93/42/EEC 和 98/79/EC 所定義的醫療設備製造商。; 指示符合欧盟指令 90/385/EEC、93/42/EEC 和 98/79/EC 的医疗设备制造商信息。
	ISO 15223-1	5.2.8	Do not use if package damaged; No utilizar si el envase está dañado; Não utilizar se a embalagem estiver danificada; 包裝破損則請勿使用; 如果包装损坏，请勿使用	Indicates a medical device that should not be used if the package has been damaged or opened.; Indica que un dispositivo médico no debe utilizarse si el envase está dañado o abierto; Indica um dispositivo médico que não deve ser utilizado se a embalagem tiver sido danificada ou aberta.; 表示如果包裝已破損或開啟，則不應使用該醫療設備。; 指示如果包装已经损坏或打开，则不应使用该医疗设备。
	ISO 15223-1	5.2.3	Sterilized using ethylene oxide; Esterilizado con óxido de etileno; Esterilizado com óxido de etileno; 已使用環氧乙烷滅菌; 环氧乙烷灭菌	Indicates a medical device that has been sterilized using ethylene oxide.; Indica que un dispositivo médico ha sido esterilizado con óxido de etileno.; Indica um dispositivo médico que foi esterilizado com óxido de etileno.; 表示已使用環氧乙烷對該醫療設備進行滅菌。; 指示医疗设备已经过环氧乙烷灭菌。
	ISO 15223-1	5.3.4	Keep dry; Mantener seco; Manter seco; 保持乾燥; 保持干燥	Indicates a medical device that needs to be protected from moisture.; Indica que un dispositivo médico debe protegerse de la humedad.; Indica um dispositivo médico que deve ser protegido da humidade.; 表示該醫療設備需防潮。; 指示需要防潮的医疗设备。
	ISO 15223-1	5.3.2	Keep away from sunlight; No exponer a la luz solar; Manter afastado da luz solar; 避免陽光照射; 远离阳光	Indicates a medical device that needs protection from light sources.; Indica que un dispositivo médico debe protegerse de los fotoemisores.; Indica um dispositivo médico que deve ser protegido de fontes de luz.; 表示該醫療設備需避免陽光照射。; 指示医疗设备需要避光。

Symbol; Símbolo; Símbolo; 符號; **符号**	Standard; Estándar; Norma; 標準; **标准**	Reference; Referencia; Referência; 參考編號; **參考**	Name; Nombre; Títulos; 標題; **标题**	Description; Descripción; Descrição; 說明; **说明**
	ISO 15223-1	5.4.2	Do not re-use ; No reutilizar; Não reutilizar; 不可重複使用; 不得重复使用	Indicates a medical device that is intended for one use, or for use on a single patient during a single procedure.; Indica que un dispositivo médico es de un solo uso o que debe utilizarse en un único paciente durante un único procedimiento.; Indica um dispositivo médico destinado a uma única utilização ou à utilização num único paciente durante um único procedimento.; 表示該醫療設備僅供單次使用，或是在單一程序期間供單一病患使用。; 指示医疗设备仅供一次性使用，或在单次手术中用于同一患者。
	ISO 15223-1	5.2.6	Do not resterilize; No volver a esterilizar; Não reesterilizar; 不可重新滅菌; 请勿重复灭菌	Indicates a medical device that is not to be resterilized.; Indica un dispositivo médico que no se puede volver a esterilizar.; Indica um dispositivo médico que não deve ser reesterilizado.; 表示該醫療設備僅供單次使用，或是在單一程序期間供單一病患使用。; 指示医疗设备仅供一次性使用，或在单次手术中用于同一患者。
	ISO 15223-1	5.6.3	Non-pyrogenic; Apirógeno; Não pirogénico; 非致熱原性; 无热原	Indicates a medical device that is non-pyrogenic.; Indica que un dispositivo médico es apirógeno.; Indica um dispositivo médico não-pirogénico.; 表示該醫療設備具非致熱原性。; 指示医疗设备无热原。
	ISO 7000	3500	Electronic instructions for use; Instrucciones de uso electrónicas; Seguir as instruções de utilização; 電子版使用說明; 电子版使用说明书	To indicate on product or product packaging that relevant information for use of the product is available in electronic form rather than, or in addition to, printed paper form.; Para indicar en un producto o en el envase de un producto que la información relevante sobre su uso está disponible en formato electrónico en lugar de, o además de, impreso en papel.; Indica no produto ou na embalagem do produto que as informações relevantes para a utilização do produto estão disponíveis em formato eletrónico e não em formato impresso, ou em complemento ao formato de papel impresso.; 在產品或產品包裝上以電子形式而非紙本形式 (或是除紙本外另有電子版)，註明與產品使用相關的資訊。; 在产品或产品包装上注明产品使用的相关信息以电子形式提供，不提供或不同时提供纸质打印的形式。
	ISO 15223-1	5.1.4	Use by date; Fecha de caducidad; Data de validade; 有效日期; 在此日期前使用	Indicates the date after which the medical device is not to be used.; Indica la fecha a partir de la cual no se debe utilizar el dispositivo médico.; Indica a data após a qual o dispositivo médico não deve ser utilizado.; 表示在該日期之後，即不可再使用此醫療設備。; 指示医疗设备应停止使用的日期。
	IEC 60878	2794	Package Contents: Pressure guide wire with connector and torque device; One (1) Secondary Torque Device; One (1); Contenido del envase: Cable guía de presión con conector y dispositivo de par de torsión, uno (1) Dispositivo de par de torsión secundario, uno (1); Conteúdo da embalagem: Fio-guia de pressão com conector e dispositivo de torção; um (1) Dispositivo de torção secundário; um (1); 包裝內容物： 含接頭和扭轉裝置的壓力導引線；一個 (1) 次要扭轉裝置；一個 (1)； 包装内容物： 带接头和扭矩装置的压力导丝；一 (1) 条 备用扭矩装置；一 (1) 件	To indicate the package contents.; Indica el contenido del envase.; Para indicar o conteúdo da embalagem.; 表示包裝內容物。; 指示包装内容物。


Symbol; Símbolo; Símbolo; 符號; 符号	Standard; Estándar; Norma; 標準; 标准	Reference; Referencia; Referência; 參考編號; 参考	Name; Nombre; Títulos; 標題; 标题	Description; Descripción; Descrição; 說明; 说明
	IEC 60601-1	Table D.2, Symbol 10	Follow instructions for use; Siga las Instrucciones de uso; Seguir as instruções de utilização; 請遵循使用說明; 遵照使用说明	Refer to instruction manual/booklet.; Consulte el manual o el folleto de instrucciones.; Consultar o manual/folheto de instruções.; 請參閱說明手冊/說明書。; 参见说明手册/小册子。
	IEC 60417	6049	Date of manufacture and country of origin (Costa Rica); Fecha de fabricación y país de origen (Costa Rica); Data de fabrico e país de origem (Costa Rica); 製造日期和原產地 (哥斯大黎加); 生产日期和原产国（哥斯达黎加）	To identify the country of manufacture of products.; Para identificar el país en el que se han fabricado los productos.; Identificar o país de fabrico dos produtos.; 識別製造日期和原產地。; 标明生产日期和原产国。
	21 CFR 801.15(c)(1)(i)F	NA, –; NA; 不適用; 不适用	Prescription only; Solo bajo prescripción médica; Apenas com receita médica; 限處方用; 仅凭处方购买	Caution: Federal (USA) law restricts this device to sale by or on the order of a physician.; Precaución: En EE. UU., las leyes federales limitan la venta de este dispositivo a los médicos o por prescripción facultativa.; Atenção: A legislação federal (dos EUA) limita a venda deste dispositivo a médicos ou por ordem destes.; 小心事項：美國聯邦法律限制本裝置僅能由醫師販售，或依照醫師的醫囑販售。; 小心：美国联邦法律严格限制由医师销售或订购本设备。
	None; Ninguno; Nenhum; 不適用; 不适用	NA, –; NA; 不適用; 不适用	Not made with natural rubber latex; No está fabricado con látex de caucho natural; Fabricado sem látex de borracha natural; 非天然橡膠乳膠製成; 非天然胶乳制成	Not made with natural rubber latex; No está fabricado con látex de caucho natural; Fabricado sem látex de borracha natural; 非天然橡膠乳膠製成。; 非天然胶乳制成。
	None; Ninguno; Nenhum; 不適用; 不适用	NA, –; NA; 不適用; 不适用	Part number, Número de referencia; Referência; 零件編號; 部件号	Part number, Número de referencia; Referência; 零件編號; 部件号
	None; Ninguno; Nenhum; 不適用; 不适用	NA, –; NA; 不適用; 不适用	Unique device identifier; Identificador único del dispositivo; Identificador único do dispositivo; 唯一裝置識別碼; 唯一设备标识符	Unique device identifier; Identificador único del dispositivo; Identificador único do dispositivo; 唯一裝置識別碼; 唯一设备标识符
	None; Ninguno; Nenhum; 不適用; 不适用	NA, –; NA; 不適用; 不适用	Medical device; Dispositivo médico; Dispositivo médico; 醫療設備; 医疗设备	Medical device; Dispositivo médico; Dispositivo médico; 醫療設備; 医疗设备
	ASTM-F2503-13	7.3.3/3.1.14	MR unsafe; No es seguro para la realización de RM; MR Unsafe (Inseguro para RM); 在 MR 環境下不安全; MR 不安全	An item which poses unacceptable risks to the patient, medical staff or other persons within the MR environment.; Un elemento que supone riesgos inaceptables para el paciente, el personal médico u otras personas dentro del entorno de RM.; Um item que representa riscos inaceitáveis para o paciente, o pessoal médico ou outras pessoas dentro do ambiente de RM.; 在 MR (磁共振) 環境下會對病患、醫療人員或其他人員造成重大風險的物品。; 对 MR（磁共振）环境中的患者、医务人员或其他人员造成不可接受风险的物品。
	None; Ninguno; Nenhum; 不適用; 不适用	NA, –; NA; 不適用; 不适用	Length; Longitud; Comprimento; 長度; 长度	Length; Longitud; Comprimento; 長度; 长度

Symbol; Símbolo; Símbolo; 符號; 符号	**Standard; Estándar; Norma; 標準; 标准**	**Reference; Referencia; Referência; 參考編號; 参考**	**Name; Nombre; Títulos; 標題; 标题**	**Description; Descripción; Descrição; 說明; 说明**
	None; Ninguno; Nenhum; 不適用; 不适用	NA, –; NA; 不適用; 不适用	Outer diameter; Diámetro externo; Diâmetro externo; 外徑; 外径	Outer diameter; Diámetro externo; Diâmetro externo; 外徑; 外径
	None; Ninguno; Nenhum; 不適用; 不适用	NA, –; NA; 不適用; 不适用	Importer; Importador; Importador; 進口商; 进口商	Indicates the entity importing the *medical device* into the locale.; Indica la entidad que importa el dispositivo médico a la zona de uso.; Indica a entidade que importa o dispositivo médico para o local.; 表示進口本醫療設備至當地之實體。; 指示将医疗设备进口到本地的实体。
	None; Ninguno; Nenhum; 不適用; 不适用	NA, –; NA; 不適用; 不适用	Straight tip; Punta recta; Extremidade reta; 直型尖端; 直形头端	Straight tip; Punta recta; Extremidade reta; 直型尖端; 直形头端
	None; Ninguno; Nenhum; 不適用; 不适用	NA, –; NA; 不適用; 不适用	J-Tip, Punta con forma de J; Extremidade em J; J 型尖端; J 形头端	J-Tip, Punta con forma de J; Extremidade em J; J 型尖端; J 形头端

Instructions for use

English

OmniWire pressure guide wire

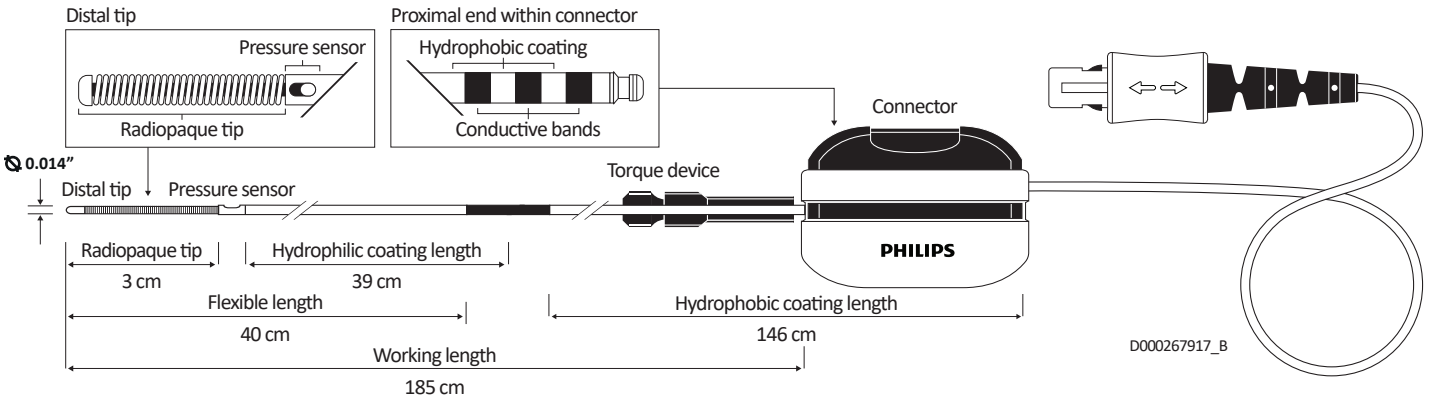

Caution:

1. U.S. Federal Law restricts this device to sale and use by or on the order of a physician.
2. Prior to use, read this entire package insert.

Indications for use:

The OmniWire pressure guide wire is indicated for use to measure pressure in blood vessels, including both coronary and peripheral vessels, during diagnostic angiography and/or any interventional procedures. It can also be used to facilitate the placement of catheters as well as other interventional devices in coronary and peripheral vessels. Blood pressure measurements provide hemodynamic information for the diagnosis and treatment of blood vessel disease.

Description:

The OmniWire pressure guide wire (hereafter referred to as the "pressure guide wire") is a steerable guide wire with a pressure sensor mounted 3 cm proximal to the tip. The pressure guide wire measures pressure when used with the IntraSight and Core Series of systems and is intended to be used in adult patients eligible for endovascular procedures. The pressure guide wire has a diameter of 0.014" (0.36 mm), a length of 185 cm and is available in straight or pre-shaped tips. It is coated with hydrophilic coating (39 cm length) on the distal portion to reduce surface friction and enhance lubricity. It is also coated with a hydrophobic coating (146 cm length) on the proximal portion to reduce surface friction. The pressure guide wire is packaged attached to the connector with an OmniWire-specific torque device to facilitate navigation through the vasculature.

The clinical application of OmniWire is to detect hemodynamically significant stenoses. Use of a pressure guide wire as an adjunct procedure to guide percutaneous interventions may limit adverse events associated with unneeded interventional procedures (e.g., stenting) and may improve clinical outcomes compared to angiography alone.

Contraindications:

The OmniWire pressure guide wire is not intended for use with atherectomy devices or for crossing a total vessel occlusion.

Adverse effects:

As with all catheterization procedures, complications may be encountered with the use of the pressure guide wire. The major risks of coronary angiography and coronary angioplasty include: coronary vessel dissection, occlusion, perforation, embolus, spasm, local and/or systemic infection, pneumothorax, serious arrhythmias, unplanned endovascular and/or surgical procedures, sterile inflammation or granulomas at the access site, pulmonary embolism, pulmonary infarction, myocardial embolism, myocardial infarction, embolic stroke, cerebral infarct, tissue necrosis and death. The major risks of peripheral angiography or peripheral angioplasty include: dissection, abrupt closure, perforation, embolus, spasm, unplanned endovascular and/or surgical procedures, sterile inflammation or granulomas at the access site, pulmonary embolism, pulmonary infarction, myocardial embolism, myocardial infarction, embolic stroke, cerebral infarct, tissue necrosis and death.

If a serious incident has occurred in relation to the device, it should be reported to the manufacturer and the competent authority of the Member State in which the user and/or patient is established. A serious incident means any incident that directly or indirectly led, might have led or, in case of recurrence, could lead to any of the following: the death of a patient, user or other person; the temporary or permanent serious deterioration of a patient's, user's, fetus or other person's state of health, or a serious public health threat.

Warnings:

- Use of the OmniWire pressure guide wire should be restricted to specialists who are familiar with, and have been trained to perform, the procedures for which this device is intended.
- This product is supplied sterile. If the pouch is unintentionally opened before use or damaged, compromising the sterile barrier, please discard the product.
- The pressure guide wire is designed for single use only. This product cannot be re-sterilized or re-used. Re-use and/or re-sterilization of unused product may result in, but is not limited to the following risks:
  - Critical harm to patient due to device separation, material deformation or infection/sepsis;
  - Inaccurate pressure readings due to pressure sensor damage;
  - Decreased mechanical performance (including but not limited to torqueability and trackability).
- Do not use expired product. If the product is expired, discard.
- The safety and effectiveness of the device has not been established for use in the neurovascular region.
- Only use the OmniWire connector with the OmniWire pressure guide wire.
- Only use the OmniWire torque device provided with the OmniWire pressure guide wire.
- Never advance, torque or withdraw a pressure guide wire that meets resistance.

- This device is coated with a hydrophilic coating at the distal end of the device for a length of 39 cm, and coated with a hydrophobic coating at the proximal end of the device for a length of 146 cm. Please refer to the "Instructions for use" section for further information on how to prepare and use this device to ensure it performs as intended. Failure to abide by the warnings in this labeling might result in damage to the device coating, which may necessitate intervention or result in serious adverse events.

Precautions:

- Do not use product that has been damaged in any way as this may result in vessel damage, inaccurate pressure measurements and/or poor mechanical performance.
- In order to minimize patient risk, exercise caution when using the pressure guide wire in a stented vessel. When advancing or withdrawing the pressure guide wire in a stented vessel, in the event that the stent is not fully apposed against the vessel wall, the pressure guide wire may become entangled in one or more stent struts. This may result in entrapment of the pressure guide wire, damage to the pressure guide wire and/or stent dislocation.
- Do not wipe the distal hydrophilic coated length of the pressure guide wire with dry gauze as this may damage the device coating.
- Do not use alcohol, antiseptic solutions, or other solvents to pretreat the pressure guide wire because this may cause unpredictable changes in the coating that could affect the device safety and performance.
- The use of an anticoagulant is recommended as per the local standard angiographic protocols and at the discretion of the physician to prevent thrombus formation.
- Simultaneous use of the pressure guidewire with electrosurgery devices is not recommended.
- Do not expose the device to a magnetic resonance environment. Device may not perform as intended and may present additional risks to patient.
- The pressure guide wire performance has been confirmed with 5 French guide catheters. When using any diagnostic or guide catheters, avoid side holes and take care to flush all residual contrast to ensure a reliable iFR/FFR.


Limitations:

- The pressure guide wire is only compatible with 0.014" (0.36 mm) ancillary devices.

Instructions for use:

Standard workflow


- Open the pressure guide wire pouch using sterile technique and place the tray on a flat surface in the sterile field.

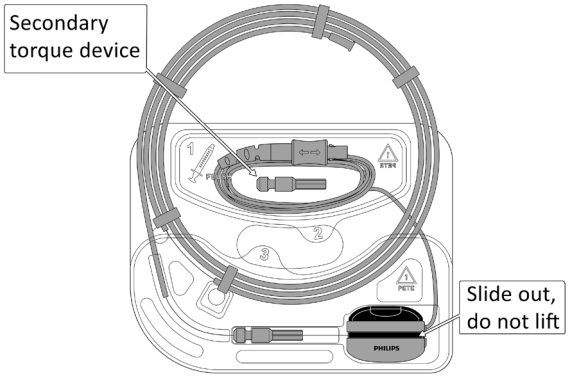


Warning: If any portion of the device (wire, torque device, or connector) makes contact with the non-sterile field or non-sterile personnel, discard.

- Prepare the pressure guide wire for use following the numbers on the tray:

1. Flush wire: Flush the pressure guide wire with normal sterile heparinized saline (labeled #1) using the wire flush port on the spiral dispenser.
2. Zero wire: Lift the numbered tab to remove the compartment lid (labeled #2), and withdraw the cable and secondary torque device. Place the secondary torque device in the sterile field. Use caution when removing the cable and secondary torque device from the compartment, as they are not secured in place. Connect the plug to a compatible instrument. This will automatically zero the pressure guide wire. During zeroing, the wire should remain stationary and on a flat surface. For system's operations refer to the proper "Operator's manual".

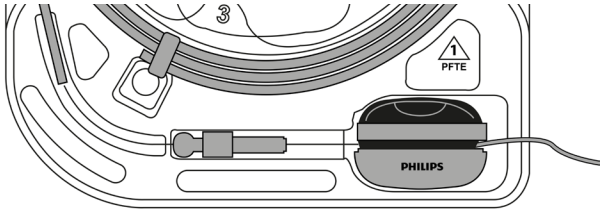

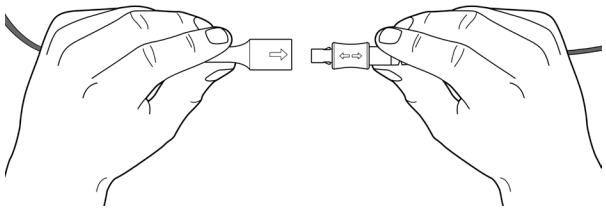

3. Remove product from tray: Lift the numbered tab to remove the compartment lid on the tray (labeled #3). Carefully slide the connector from the tray and slide the wire out of the spiral dispenser. Place wire and connector on the sterile field.

Precaution: When withdrawing the wire from the spiral dispenser, keep the connector and wire in the same plane to avoid kinking the wire.

Precaution: Do not grasp the tip of the pressure guide wire to remove it from the spiral dispenser. This may result in damage to the pressure sensor.


- At the physician's discretion, the 1 cm shapeable pressure guide wire tip may be carefully shaped using standard tip shaping practices. For best results, shape the tip in the direction of the sensor housing opening. Do not use a shaping instrument with a sharp edge. Take care when shaping the tip. Do not grip the sensor housing as this may damage the pressure sensor.
- Insert the pressure guide wire through the appropriate introducer components and guiding catheter into the desired blood vessel. Slowly advance the pressure guide wire tip under fluoroscopy using contrast injections to verify location.
- Ensure that the tip is rotating freely and no resistance is felt when torque is applied.
- In the event that resistance is felt, exercise caution when removing the device, and exchange the device for a new one to complete the procedure.

  Precaution: The pressure guide wire should not be advanced or withdrawn if resistance is encountered. The wire should never be forcibly advanced into or withdrawn from a vessel. Any time that resistance is encountered, the wire should be slowly withdrawn under fluoroscopic guidance. In some instances, the wire may kink and must be removed.
- Position the pressure sensor (located 3 cm from tip) adjacent to the tip of the guide catheter and perform normalization procedure with the instrument. For system's operations refer to the proper system "Operator's manual".
- In the event the pressure guide wire is "Not Recognized", squeeze connector and realign the pressure guide wire (see "Attaching pressure guide wire to connector" section for further instruction).
- Advance the pressure sensor to desired measurement location, making sure the sensor is distal to the stenosis, and perform pressure measurements with the instrument. Refer to "Operator's manual" for details on how to perform pressure measurements.
- After every procedure, slowly withdraw the pressure guide wire until the pressure sensor is just distal to the guide catheter tip. Verify that the pressures measured by the pressure guide wire and through the guide catheter are equal.

- If storing the wire for subsequent measurements, place the wire underneath a drape in the sterile field. Prior to reinsertion for multiple measurements, wipe wire with normal sterile heparinized saline using damp gauze.
- When the procedure is completed, withdraw the pressure guide wire and dispose of the pressure guide wire, torque device, and connector as biohazardous waste in accordance with local regulations.

Removing pressure guide wire from connector

- The pressure guide wire may be disconnected from the connector to facilitate wire maneuverability and to allow advancement of catheters and other ancillary devices over the proximal end of the wire.
  NOTE: If the plug remains connected to the instrument, it is not required to repeat zeroing and normalization.
- To remove the pressure guide wire, squeeze the connector and carefully lift the proximal end of the wire from the pressure guide wire channel.

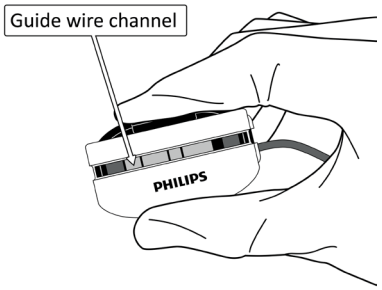

Warning: Do not flex the proximal (electrical connector) end of the pressure guide wire when not inserted in the connector. Excessive flexing can damage or break the internal components.

- If desired, loosen the torque device and withdraw it from the proximal end of the pressure guide wire.
  Precaution: When unloading the torque device, use caution to prevent coating damage.

Catheter delivery

- Thread catheter over the pressure guide wire taking care not to kink the proximal conductive bands of the wire.
  Warning: When using the pressure guide wire with ancillary devices (e.g. stenting), incorrect device advancement/withdrawal can impact the mechanical performance of the pressure guide wire, damage its coating, or result in resistance.

  Warning: Take care not to deploy any interventional device over the pressure guide wire sensor as it could result in sensor damage and inaccurate pressure measurements.

  Precaution: When loading or unloading an ancillary device over the wire, use caution to prevent coating damage.
- For catheter delivery, refer to applicable catheter device's "Instructions for use".

Attaching pressure guide wire to connector

- Install the included torque device over the proximal end of the pressure guide wire. The connector cannot be used to effectively torque the pressure guide wire as the wire rotates freely inside the body of the connector.
  Warning: Using a torque device other than the torque device provided will damage the wire. A secondary torque device is provided in the event the primary torque device is no longer available for use (e.g. compromised sterility).


  Precaution: When reloading the torque device, use caution to prevent coating damage.

  Warning: The connector provided in the package is unique to the individual pressure guide wire it is connected to and should not be used with any other pressure guide wires. Use of a different connector will result in inaccurate pressure measurement data.
- Clean the proximal end of the pressure guide wire with normal sterile heparinized saline. Prior to reconnecting, dry the proximal end of the pressure guide wire with a clean, dry cloth.


Warning: Do not flex the proximal (electrical connector) end of the pressure guide wire when not inserted in the connector. Excessive flexing can damage or break the internal components.

Precaution: Failure to dry the proximal end of the pressure guide wire will result in inaccurate pressure measurement data.


- Squeeze the connector to expose the pressure guide wire channel.
- Hold the pressure guide wire at a slight angle to the connector and place it in the channel with approximately 0.5 inches (1.3 cm) of the pressure guide wire protruding from the connector.
- Maintaining the angle, drag the pressure guide wire through the channel until the pressure guide wire alignment notch catches the locking clip in the connector. This will align the pressure guide wire.

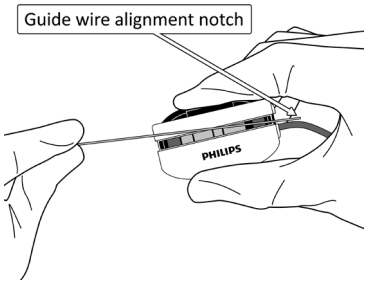

- Lower the pressure guide wire into the channel.

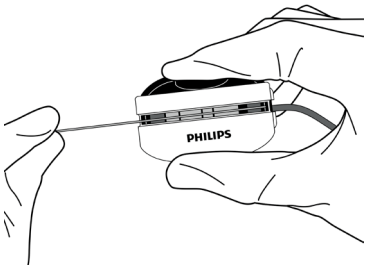

- Release the connector to lock the pressure guide wire in place

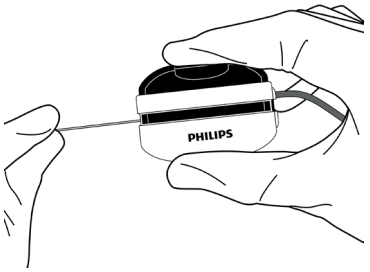

- A pressure signal will now be present on the display instrument. It is not required to repeat zeroing and normalization as long as the modular connector has not been removed from the instrument.
- In the event the pressure guide wire is "Not Recognized", squeeze connector and realign the pressure guide wire.

Technical specifications

Operating range	Pressure range: -30 to +300 mmHg
Pressure accuracy	±3 mmHg, range of -30 to +100 mmHg ±3 %, range of +100 to +300 mmHg

Storage and handling:

Products should be stored indoors at room temperature in their original packaging.

Limited warranty:

Subject to the conditions and limitations on liability stated herein, Philips warrants that the OmniWire pressure guide wire (the "wire"), shall materially conform to Philips's then current specification for the wire at the time of shipment. **Any liability of Philips with respect to the wire or the performance thereof under any warranty, negligence, strict liability or other theory will be limited exclusively to wire replacement or, if replacement is inadequate as a remedy or, in Philips' opinion, impractical, to a credit of the purchase price paid for the wire. Except for the foregoing, the wire is provided "as is" without warranty of any kind, expressed or implied, including without limitation, any warranty of fitness, merchantability, and fitness for a particular purpose of noninfringement. Further, Philips does not warrant, guarantee, or make any representations regarding the use, or the results of the use, of the wire or written materials in terms of correctness, accuracy, reliability, or otherwise.** Licensee understands that Philips is not responsible for and will have no liability for any items or any services provided by any persons other than Philips. Philips shall have no liability for delays or failures beyond its reasonable control. Additionally, this warranty does not apply if:

1. The wire is used in other than a manner described by Philips in the "Instructions for use" supplied with the wire or the wire is subject to misuse, negligence or to an accident.
2. The wire is used in a manner that is not in conformance with purchase specifications or specifications contained in the "Instructions for use".
3. The wire is re-used or re-sterilized.
4. The wire is repaired, altered, or modified by other than Philips authorized personnel or without Philips authorization.
5. The wire is not used by the stated "Use By" or "Expiration" date, or if the packaging is opened or damaged before use.

If claims under this warranty become necessary, contact Philips for instructions and issuance of a Return Material Authorization number if the wire is to be returned. Equipment will not be accepted for warranty purposes unless the return has been authorized by Philips.

Patent:

www.philips.com/patents

An electronic copy of these instructions can be found at:
www.philips.com/IFU

This product is licensed to the customer for single use only.

Additional questions regarding this product should be directed to Philips in the U.S.A.:

Legal Manufacturer:
Volcano Corporation
3721 Valley Centre Drive, Suite 500
San Diego, CA 92130 USA
(800) 228-4728
IGTD.CustomerInquiry@philips.com

USA & Canada:
(800) 228-4728
IGTD.CustomerInquiry@philips.com

International:
vecomplaints@philips.com or
IGTD.CustomerInquiry@philips.com

Australian Sponsor:
Philips Electronics Australia Ltd
65 Epping Road
North Ryde, NSW Australia 2113

© 2021 Koninklijke Philips N.V. All rights reserved.
Trademarks are the property of Koninklijke Philips N.V.

www.philips.com/IGTdevices
Revision date: 07/2021
300005796131.D