
Shockwave IVL

Shockwave C2 Aero Fly delivers elevated efficiency

Our 2x-faster Coronary IVL upgrade is ready for takeoff

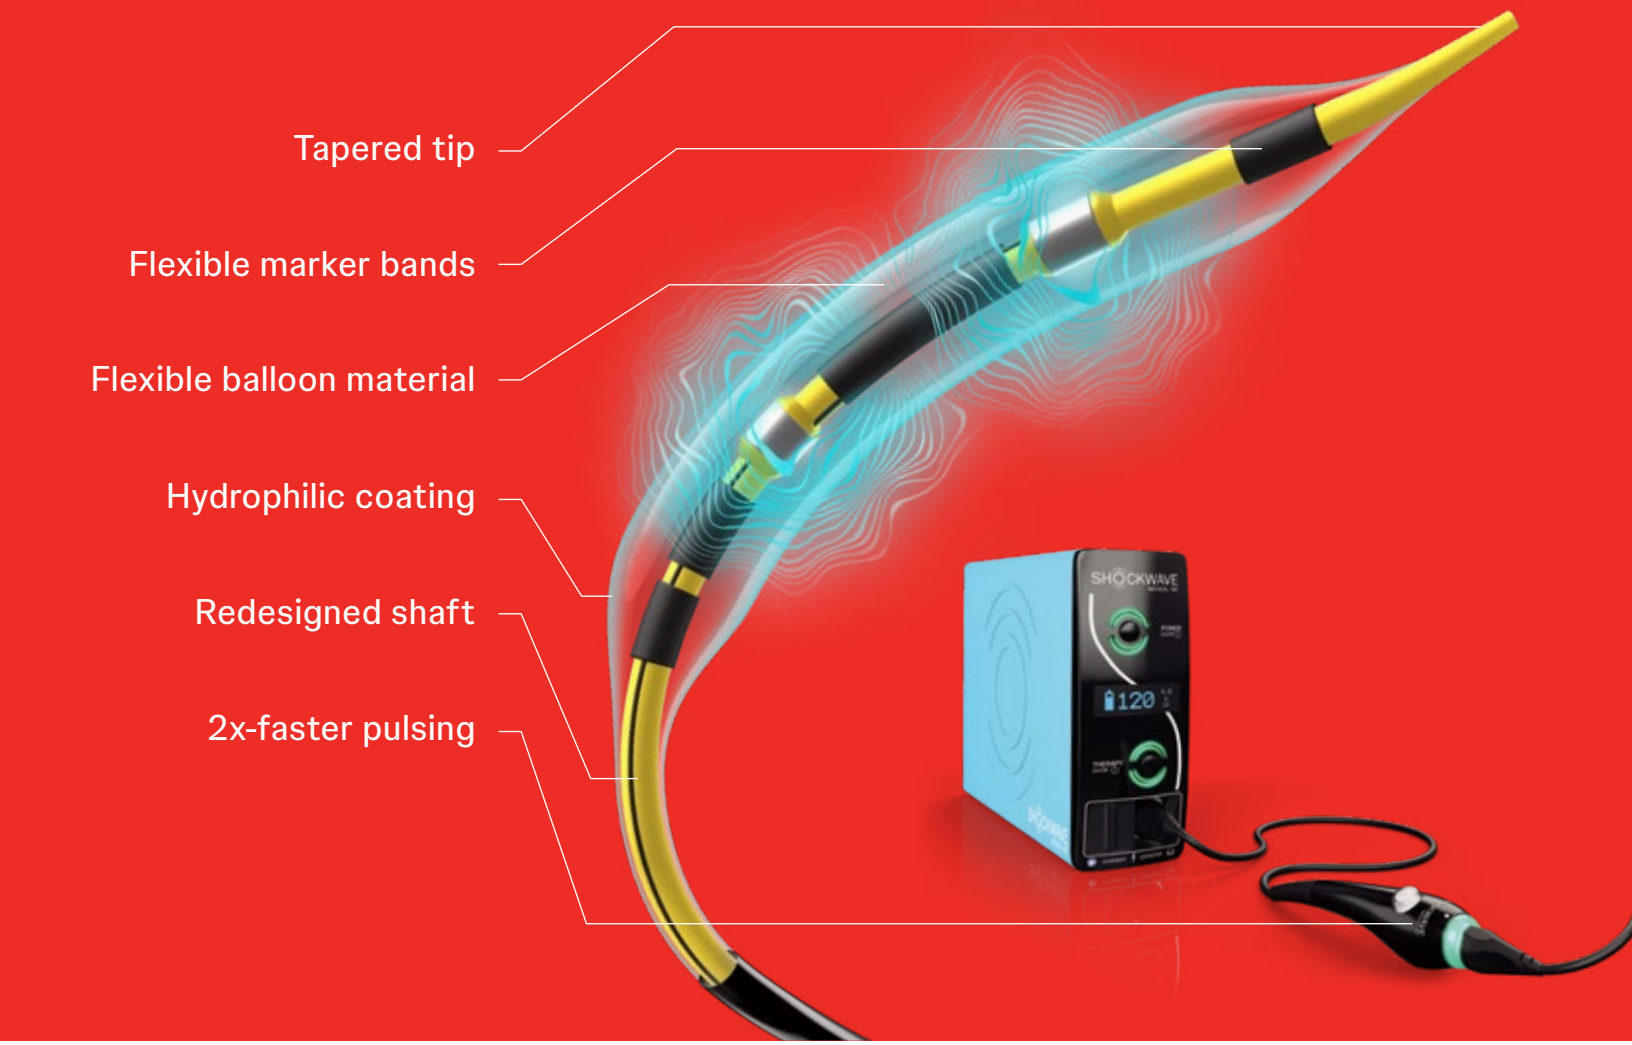

2x-faster pulsing

Improve procedural flow and support cath lab efficiency with upgraded pulsing speed

Best-in-class deliverability

Reach difficult anatomy using fewer exchanges with optimized profile and trackability[1]

Patient-focused innovation

Minimize ischemic times[2] with reduced periods of prolonged balloon inflation and shorter treatment duration


Johnson&Johnson MedTech

1. Based on simulated use bench testing. Based on feedback from physicians who participated in the Limited Market Release Survey
2. A shorter inflation time exposes the patient to less ischemic time compared to prior Shockwave devices.

The wait is over

More efficient treatment time[1]

Treatment calculation is for 120 cycles

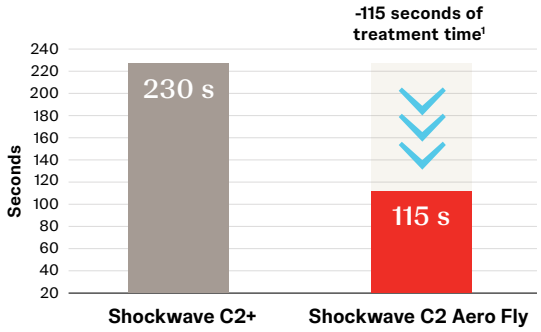

What this means for you

Shockwave™ C2 Aero Fly's reduced pause time between cycles coupled with 2Hz pulsing capabilities reduce overall ischemic time for the patient during the procedure[2]


Overall treatment time cut by 50%[1]

1. Treatment time includes pulsing time and pause time. Pause time may vary by patient need.
2. A shorter inflation time exposes the patient to less ischemic time compared to prior Shockwave devices.


Equidistant emitter placement

New catheter emitter configuration & tip design

Shockwave C2+

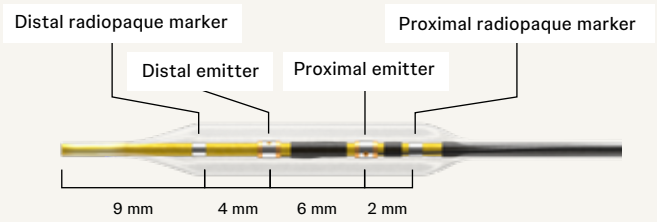

Shockwave C2 Aero Fly

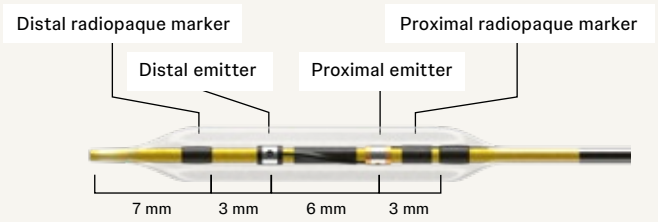

The distal emitter is also 3 mm closer to the tip on Shockwave C2 Aero Fly as compared to Shockwave C2+

New catalog numbers for Shockwave C2 Aero Fly

Catalog Number	Diameter (mm)	Length (mm)	Pulses (Max)	Guidewire Compatibility (in)	Guide Catheter Compatibility	Working Length (cm)	Tip Profile (in)	Max Crossing Profile (in)
C2AFIVL2512	2.5	12	120	0.014	6F	138	.022	0.044”
C2AFIVL3012	3.0	12	120	0.014	6F	138	.022	0.045”
C2AFIVL3512	3.5	12	120	0.014	6F	138	.022	0.045”
C2AFIVL4012	4.0	12	120	0.014	6F	138	.022	0.047”

In the United States: Rx only. Indications for Use—The Shockwave Intravascular Lithotripsy (IVL) System with the Shockwave C2, Shockwave C2+, Shockwave C2 Aero, and Shockwave C2 Aero Fly Coronary IVL Catheters is indicated for lithotripsy-enabled, low-pressure balloon dilatation of severely calcified, stenotic de novo coronary arteries prior to stenting. **Contraindications—** The Shockwave C2, Shockwave C2+, Shockwave C2 Aero, and Shockwave C2 Aero Fly Coronary IVL Systems are contraindicated for the following: These devices rea not intended for stent delivery. These devices are not intended for use in carotid or cerebrovascular arteries. **Warnings—** Use the IVL Generator in accordance with recommended settings as stated in the Operator's Manual. The risk of a dissection or perforation is increased in severely calcified lesions undergoing percutaneous treatment, including IVL. Appropriate provisional interventions should be readily available. Balloon loss of pressure was associated with a numerical increase in dissection which was not statistically significant and was not associated with MACE. Analysis indicates calcium length is a predictor of dissection and balloon loss of pressure. IVL generates mechanical pulses which may cause atrial or ventricular capture in bradycardic patients. In patients with implantable pacemakers and defibrillators, the asynchronous capture may interact with the sensing capabilities. Monitoring of the electrocardiographic rhythm and continuous arterial pressure during IVL treatment is required. In the event of clinically significant hemodynamic effects, temporarily cease delivery of IVL therapy. **Precautions—** Only to be used by physicians trained in angiography and intravascular coronary procedures. Use only the recommended balloon inflation medium. Hydrophilic coating to be wet only with normal saline or water and care must be taken with sharp objects to avoid damage to the hydrophilic coating. Appropriate anticoagulant therapy should be administered by the physician. Precaution should be taken when treating patients with previous stenting within 5 mm of target lesion IVL pulses may potentially interfere with certain implanted electrical devices (e.g., ventricular support systems). **Cautions—** Shockwave C2 and Shockwave C2+ should not be re-inserted once they are pulled out of the patient's body. Shockwave C2 Aero and Shockwave C2 Aero Fly may be re-inserted up to 3 times in the same patient when used in accordance with the IFU. **Potential adverse effects consistent with standard based cardiac interventions include–** Abrupt vessel closure – Allergic reaction to contrast medium, anticoagulant and/or antithrombotic therapy- Aneurysm-Arrhythmia-Arteriovenous fistula-Bleeding complications-Cardiac tamponade or pericardial effusion- Cardiopulmonary arrest-Cerebrovascular accident (CVA)- Coronary artery/vessel occlusion, perforation, rupture or dissection-Coronary artery spasm-Death-Emboli (air, tissue, thrombus or atherosclerotic emboli)-Emergency or non- emergency coronary artery bypass surgery-Emergency or non emergency percutaneous coronary intervention-Entry site complications-Fracture of the guide wire or failure/malfunction of any component of the device that may or may not lead to device embolism, dissection, serious injury or surgical intervention- Hematoma at the vascular access site(s)-Hemorrhage- Hypertension/Hypotension-Infection/sepsis/fever-Myocardial Infarction-Myocardial Ischemia or unstable angina-Pain-Peripheral Ischemia-Pseudoaneurysm-Renal failure/insufficiency-Restenosis of the treated coronary artery leading to revascularization-Shock/pulmonary edema-Slow flow, no reflow, or abrupt closure of coronary artery-Stroke-Thrombus- Vessel closure, abrupt-Vessel injury requiring surgical repair- Vessel dissection, perforation, rupture, or spasm. Risks identified as related to the device(s) and its use: Allergic/immunologic reaction to the catheter material(s) or coating-Device malfunction, failure, or balloon loss of pressure leading to device embolism, dissection, serious injury or surgical intervention-Atrial or ventricular extrasystole-Atrial or ventricular capture. **Prior to use, please reference the Instructions for Use for more information on indications, contraindications, warnings, precautions and adverse events. www.shockwavemedical.com/IFU.**

© 2026 Shockwave Medical, Inc. All Rights Reserved. SPL 80775 Rev C.

Johnson&Johnson MedTech