
VOLCANO

INSTRUCTIONS FOR USE
REFINITY ST
ROTATIONAL IVUS CATHETER

REF 89900 **ENGLISH**

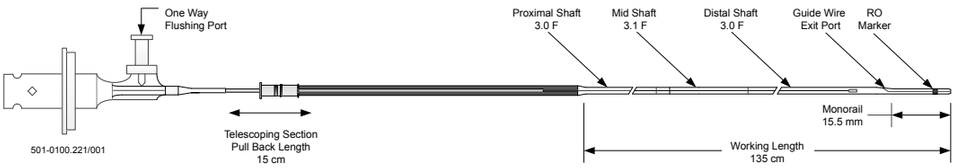

CAUTION:

1. **U.S. Federal Law restricts this device to sale by or on the order of a physician.**
2. **Prior to use, read this entire Instructions For Use.**

INDICATIONS FOR USE:

The REFINITY ST Rotational IVUS Imaging Catheter (REFINITY ST catheter) is intended for the intravascular ultrasound examination of coronary arteries. Intravascular ultrasound imaging is indicated in patients who are candidates for transluminal interventional procedures. REFINITY ST catheters are designed for use as an adjunct to conventional angiographic procedures to provide an image of the vessel lumen and wall structures.

DESCRIPTION:

The REFINITY ST catheter consists of two main assemblies: the imaging core and the catheter body. The catheter body is comprised of four sections: a distal section with a .014" compatible rapid exchange guide wire lumen and clear imaging window, a mid-shaft section, a braided proximal shaft, and a telescoping section.

The distal, mid, and proximal sections comprise the usable length or working length of the catheter. The telescoping section remains outside of the guiding catheter. The telescoping section allows the imaging core to be advanced and retracted for up to 15 cm of linear movement. The corresponding movement of the transducer occurs from the proximal end of the guidewire exit port to the proximal end of the window portion of the distal section.

The imaging core is composed of a hi-torque, flexible, rotating drive cable with a distal outward looking ultrasonic transducer. An electromechanical connector interface at the proximal end makes the connection to the patient interface module (PIM). The PIM–catheter interface consists of an integrated mechanical drive assembly and electrical connection.

A flushing port with a one-way valve is used to displace the air initially present within the catheter. The catheter must be flushed with sterile heparinized normal saline prior to use, as this provides the acoustic coupling media required for ultrasonic imaging. The one-way valve helps retain saline in the catheter during use.

The catheter body has a distal guide wire lumen with a proximal exit port located 15.5 mm from the distal end. One radiopaque (RO) marker band is embedded 0.5 cm from the tip. In addition, insertion depth indicators are located on the catheter body at 90 cm and 100 cm. The catheter is packaged with a sterile PIM cover, 3 cc and 10 cc syringes, and 13 in extension tubing with a 3-way stopcock.

Este catéter es para uso exclusivo con los sistemas IntraSight y de la series Volcano s5 y CORE. El catéter no funcionará si se conecta a cualquier otro sistema de adquisición de imágenes. Consulte el manual del usuario del sistema.

INCLUDED ACCESSORIES:

3cc syringe; One (1)

10cc syringe; One (1)

Extension tube; One (1)

3-way stopcock; One (1)

SpinVision Sterile Equipment cover; One (1)

CONTRAINDICATIONS:

THIS DEVICE IS NOT CURRENTLY INDICATED FOR USE IN CEREBRAL OR PERIPHERAL VESSELS. USE OF IVUS IMAGING CATHETERS IS CONTRAINDICATED WHERE INTRODUCTION OF ANY CATHETER WOULD CONSTITUTE A THREAT TO PATIENT SAFETY. CONTRAINDICATIONS INCLUDE: BACTEREMIA OR SEPSIS, MAJOR COAGULATION SYSTEM ABNORMALITIES, PATIENTS DISQUALIFIED FOR CABG SURGERY, PATIENTS DISQUALIFIED FOR PERCUTANEOUS CORONARY INTERVENTIONS, SEVERE HEMODYNAMIC INSTABILITY OR CARDIOGENIC SHOCK, PATIENTS DIAGNOSED WITH NITRATE-RESISTANT CORONARY ARTERY SPASM, SEVERE ARTERIAL CALCIFICATION OR SEVERE ARTERIAL TORTUOSITY AND CHRONIC TOTAL OCCLUSION.

ADVERSE EFFECTS:

Bleeding at the entry puncture site, injury to the vascular wall, thrombosis of the vessel, and peripheral embolization has occurred with the use of percutaneous intravascular catheter devices. Possible adverse effects include, but are not limited to, the following: death; myocardial infarction; occlusion; coronary vessel dissection; coronary artery spasm.

WARNINGS:

- Use of the REFINITY ST catheters is restricted to cardiovascular specialists who are familiar with, and have been trained to perform, the procedures for which this device is intended.
- Air entrapped in the catheter and flushing accessories can cause potential injury or death. Always verify that the catheter and flushing accessories have been properly cleared of air prior to inserting the catheter into the vasculature.
- DO NOT advance the catheter if resistance is encountered. The catheter should never be forcibly inserted into lumens narrower than the catheter body or forced through a tight stenosis.
- Exercise care when advancing the REFINITY ST catheter distal to a deployed stent. The short monorail segment can result in exposure of the guide wire to the stent struts.
- Care should be taken when advancing or re-advancing a guide wire or catheter through a deployed stent. A guide wire may exit between stent struts when crossing or re-crossing a stent that is not fully apposed to the vessel wall. When advancing or re-advancing the catheter over a guide wire and through a stented vessel, in the event that the stent is not fully apposed against the vessel wall, the guide wire / and or catheter may become entangled in the stent between the junction of the catheter and guide wire or within one or more stent struts. This may result in entrapment of the catheter/guide wire, catheter tip separation, and/or stent dislocation. Never use force to advance the catheter. Use caution when removing the catheter over the guide wire from a stented vessel to minimize patient risk.
- In instances where the device has crossed a deployed stent, care should be taken when retracting the device to ensure that entanglement does not occur. Fluoroscopy should be used to monitor guide wire position with respect to the imaging catheter and the stent; at no time should the imaging catheter be retracted if there is evidence of guide wire prolapse or if significant resistance to withdrawal is experienced. If either of these events occur, advance the imaging catheter distal of the stent and then carefully remove the whole system under the guidance of fluoroscopy.

PRECAUTIONS:

The REFINITY ST catheter is a delicate scientific instrument and should be treated as such. Always observe the following precautions:

- Contents are supplied STERILE using an EtO (ethylene oxide) process. Do not use if the sterile barrier is damaged.
- To maintain optimal patient safety, inspect the product prior to use. Do not use if saline leaks from any location other than the vent port located at the guide wire exit in the monorail section.
- **For single use only. Do not re-use, reprocess or re-sterilize. Re-use, reprocessing or re-sterilization may compromise the structural integrity of the device and/or lead to device failure which in turn may result in patient injury, illness or death.**
- The REFINITY ST catheter is designed for single use only. Volcano Corporation ("VOLCANO") makes no warranty, representation or condition of any kind, whether expressed or implied (including any warranty of merchantability, suitability or fitness for a particular purpose) respecting the re-use of the catheter.
- In addition, VOLCANO assumes no responsibility or liability for incidental or consequential damages which may result from such re-use. Re-use including resterilization of unused product may result in, but is not limited, to the following:
  - Potential critical harm to patient due to Device Separation, Material Deformation or Infection/Sepsis;
  - Failure to Image or other device malfunctions.
- The catheter has no user serviceable parts. Do not attempt to repair or to alter any component of the catheter assembly.
- Clean guide wire and flush catheter thoroughly with sterile heparinized normal saline before and after each insertion.
- Do not attempt to connect the catheter to electronic equipment other than the designated systems.
- Never attempt to attach or detach the catheter while the PIM motor is running. To do so may damage the connector.
- Avoid any sharp bends, pinching, or crushing of the catheter.
- Do not kink or sharply bend the catheter at any time. This can cause a drive cable failure. Do not insert the catheter into a guide catheter at an insertion angle greater than 45º. Do not use any catheter that has been kinked or sharply bent.
- Before withdrawing the catheter, ensure the PIM is not imaging or pulling back the catheter.
- When advancing or re-advancing the catheter over a guide wire and through a stented vessel, in the event that the stent is not fully apposed against the vessel wall, the guide wire / and or catheter may become entangled in the stent between the junction of the catheter and guide wire or within one or more stent struts. This may result in entrapment of catheter or guide wire, catheter tip separation, and/or stent dislocation. Never use force to advance the catheter.

INSTRUCTIONS FOR USE:

Inspection Prior to Use

Carefully inspect the package prior to use for any breach of the sterile barrier or damage to the contents. If the sterile barrier integrity is compromised or the contents damaged, contact your Volcano Corporation representative to return the damaged catheter. Open a new catheter and prepare it for use per this IFU.

Preparation For Use

- Refer to the operator's manual or user's guide for instrumentation and PIM Setup. Using sterile technique, remove the catheter from its sterile packaging. Do not open telescoping section when the catheter is within the protective Packaging Coil Housing. Remove the Packaging Coil protecting the catheter.
- Retract the movable Imaging Core completely to the proximal position via the telescope shaft.
- Fill both the 3 cc and 10 cc syringes with sterile heparinized normal saline. Connect both syringes to the 3-way stopcock, then connect the assembly to the extension tube, and flush the extension tube in order to expel all air from this assembly. Connect the extension tube to the one-way valve on the catheter hub. The 10 cc syringe is to be used as a reservoir for refilling the 3 cc flushing syringe.
- Flush the imaging catheter twice continuously using the 3 cc flushing syringe OR until all bubbles are expressed from the interior of the catheter within the clear distal shaft. DO NOT USE EXCESSIVE PRESSURE.
- Connect the imaging catheter to the PIM by inserting the proximal end of the connector through the opening in the sterile PIM cover, gently twisting the connector until it locks in place.
- Advance the imaging core so that it is at its fully distal position. Examine the imaging core within the clear distal shaft to ensure no air is in the system. If air is present, retract the imaging core and reflush. Advance the imaging core and recheck for air.
- Begin imaging by pressing the Image button on the PIM to ensure proper function of the catheter by observing a pattern of partial bright concentric rings on the monitor.
- Refill the 10 cc syringe as needed and reattach to the stopcock without introducing air into the line.
- An appropriate sized guide catheter (5F, I.D. ≥.056") and guide wire (max .014") should be placed according to local standard operating procedures prior to advancing the IVUS catheter.

Note: Guide wires that supply more stiffness near the distal tips are recommended.

Note: Always wipe down the guide wire with sterile heparinized normal saline prior to loading the catheter onto the guidewire.

CAUTION: Never advance the imaging catheter without guide wire support.

CAUTION: Never advance or withdraw the imaging catheter without the imaging core assembly in the most distal position.

CAUTION: Never advance or withdraw the imaging catheter without direct, fluoroscopic visualization.

CAUTION: Never advance the distal tip of the imaging catheter near the very floppy end of the guide wire. This part of the guide wire will not adequately support the catheter. A catheter advanced to this portion of the guide wire may not follow the guide wire when it is retracted and cause the guide wire to buckle into a loop. The catheter may then drag along the inside of the vessel and catch on the guide catheter tip. If this occurs, remove the catheter assembly, guide wire and the guide catheter together. If the catheter is advanced too near to the end of the guide wire, advance the guide wire while holding the imaging catheter steady. If this fails, withdraw the catheter and guide wire together. Continue to advance the imaging catheter into the guide catheter, up to the femoral or brachial marker. Tighten the hemostasis valve on the guide catheter's Y-adapter. Tighten only enough to prevent fluid/blood leakage.

Note: AN EXCESSIVELY TIGHTENED HEMOSTASIS VALVE MAY DISTORT THE IMAGE DUE TO BINDING OF THE ROTATING DRIVE CABLE.

Catheter Placement and Imaging

Note: All PIM functions can be executed either directly on the PIM using the console control pad or the Graphical User Interface (GUI) of the system.

- While the PIM is not imaging, and while using fluoroscopy, advance the imaging catheter over the guide wire until the distal marker crosses a minimum of 3 cm beyond the region of interest in the vessel/lesion.
- Keeping the catheter body and guide wire fixed press the IMAGE button on the PIM in order to begin imaging.
- Retract the imaging core either by automated or manual pullback.
  - For automated pullback, verify the desired pullback speed within the system menu. Press the RECORD (PULLBACK) button to begin the pullback and capture the videoloop.
  - For manual pullback, verify the manual mode is selected on the PIMr and press RECORD (PULLBACK) tocapture the videoloop and slowly pull back the telescoping section to retract the imaging core along its 15 cm length, imaging any region of interest.
- When finished, stop imaging by pressing the IMAGE button. Advance the imaging core to its most distal position. Maintain the position of the wire and remove the catheter.

Note: Always ensure that imaging is off before advancing the imaging core within the catheter.

Note: When the procedure is completed, remove and discard the catheter in accordance with local regulations.

Troubleshooting

If your system menu does not include "REFINITY ST Catheters", contact your Volcano Corporation representative before proceeding. If the image fades during use or shadowed areas are visible in situ, the distal lumen or catheter body may contain air bubbles. Remove the catheter and flush as indicated in the Preparation For Use section.

Refer to your specific Volcano system Operator's Manuals for instrumentation, setup, use and troubleshooting.

STORAGE AND HANDLING:

Products should be stored in a dry, dark, cool place in their original packaging.

PRODUCT SPECIFICATIONS:

Acoustic Output Parameter	B-Mode
ISPTA.3 (mW/cm^2)*	0.391
ISPPA.3 (W/cm^2)*	7.84
Pr.3 (MPa)	0.498
PD (µs)	0.0502
PRF (Hz)	1.54x10^4
Center Freq (MHz)	42.1
MI**	0.0826
TI**	1.25x10^{-3}

* Maximum overall uncertainty ± 27.1%

** As estimated in tissue

Model	REFINITY ST
Catalog number	89900
Maximum guide wire	0.014" (0.36 mm)
Minimum guide catheter I.D.	0.056" (1.42 mm)
Usable length	135 cm

TI: Thermal Index defined as $TI = \frac{W01x1f_C}{210}$

W01x1: Bounded-square Output (mW)

f_C: Center Frequency (MHz)

MI: Mechanical Index defined as MI= Pr.3/($f_C^{1/2}$)

$I_{SPPA.3}$: Derated Intensity, Spatial Peak Pulse Average (W/cm^2)

ISPTA.3: Derated Intensity, Spatial Peak Temporal Average (mW/cm^2)

Pr.3: Derated Peak Negative Pressure at a location of the maximum derated pulse intensity integral (MPa)

W_0: Total Power (mW)

PD: Pulse Duration (µs)

PRF: Pulse Repetition Frequency (Hz)

LIMITED WARRANTY:

Subject to the conditions and limitations on liability stated herein, Volcano Corporation ("VOLCANO") warrants that the REFINITY ST catheter (the "Catheter"), as so delivered, shall materially conform to VOLCANO'S then current specification for the Catheter upon receipt for a period of one year from the date of delivery. **ANY LIABILITY OF VOLCANO WITH RESPECT TO THE CATHETER OR THE PERFORMANCE THEREOF UNDER ANY WARRANTY, NEGLIGENCE, STRICT LIABILITY OR OTHER THEORY WILL BE LIMITED EXCLUSIVELY TO CATHETER REPLACEMENT OR, IF REPLACEMENT IS INADEQUATE AS A REMEDY OR, IN VOLCANO'S OPINION, IMPRACTICAL, TO A REFUND OF THE FEE PAID FOR THE CATHETER. EXCEPT FOR THE FOREGOING, THE CATHETER IS PROVIDED "AS IS" WITHOUT WARRANTY OF ANY KIND, EXPRESSED OR IMPLIED, INCLUDING WITHOUT LIMITATION, ANY WARRANTY OF FITNESS, MERCHANTABILITY, AND FITNESS FOR A PARTICULAR PURPOSE OR NONINFRINGEMENT. FURTHER, VOLCANO DOES NOT WARRANT, GUARANTEE, OR MAKE ANY REPRESENTATIONS REGARDING THE USE, OR THE RESULTS OF THE USE, OF THE CATHETER OR WRITTEN MATERIALS IN TERMS OF CORRECTNESS, ACCURACY, RELIABILITY, OR OTHERWISE.** Licensee understands that VOLCANO is not responsible for and will have no liability for any items or any services provided by any persons other than VOLCANO. VOLCANO shall have no liability for delays or failures beyond its reasonable control.

Additionally, this warranty does not apply if:

1. The Catheter is used in a manner other than described by VOLCANO in the Instructions For Use supplied with the Catheter.
2. The Catheter is used in a manner that is not in conformance with purchase specifications or specifications contained in the Instructions For Use.
3. The Catheter is re-used or re-sterilized.
4. The Catheter is repaired, altered, or modified by other than VOLCANO authorized personnel or without VOLCANO authorization.

If claims under this warranty become necessary, contact VOLCANO for instructions and issuance of a Return Material Authorization number if the Catheter is to be returned. Equipment will not be accepted for warranty purposes unless the return has been authorized by VOLCANO.

ADDITIONAL QUESTIONS REGARDING THIS PRODUCT SHOULD BE DIRECTED TO VOLCANO CORPORATION IN THE USA.

Legal Manufacturer:
Volcano Corporation
3721 Valley Centre Drive, Suite 500
San Diego, CA 92130 USA
(800) 228-4728
IGTD.CustomerInquiry@philips.com

USA & Canada:
(800) 228-4728
IGTD.CustomerInquiry@philips.com

International:
vecomplaints@philips.com or
IGTD.CustomerInquiry@philips.com

Authorized European Representative: EC REP
Volcano Europe SA/NV
Excelsiorlaan 41
B-1930 Zaventem, Bélgica
Teléfono: +32.2.679.1076
Fax: +32.2.679.1079

CE 2797

300004856942/B Revision Date: 09/2023

VOLCANO

LOT

ISO 15223-1 Batch code - Código de lote; Batchkod; Eräkoodi; Chargenbezeichnung; Codice del lotto; партиден код; Κωδικός παρτίδας; Numéro de lot; Batchcode; Batchkode; Sarzskód; lotnummer; код партии; Šifra serije; Código do lote; Parti kodu; Kód série; Codul lotului; kod partii; Broj serije

REF

ISO 15223-1 Catalog number - Número de catálogo; Katalognummer; Luettelonumero; Katalognummer; Numero di catalogo; каталожен номер; Αριθμός καταλόγου ; Numéro de référence; Catalogusnummer; Katalognummer; Katalógusszám; katalognummer; номер по каталогу; Kataloški broj; Número de catálogo; Katalog numarası; Katalogové číslo; Numărul de catalog; numer katalogowy; Kataloški broj

ISO 15223-1 Manufacturer - Fabricante; Tillverkare; Valmistaja; Hersteller; Fabbricante; производител; Κατασκευαστής; Fabricant; Fabrikant; Producent; Gyártó; produsent; производитель; Proizvođač; Fabricante; Üretici; Výrobce; Producător; producent; Proizvođač

ISO 15223-1 Do not use if package damaged - No utilizar si el envase está dañado; Använd inte om förpackningen är trasig; Ei saa käyttää, jos pakkaus on vahingoittunut; Bei beschädigter Verpackung nicht verwenden; Non utilizzare se la confezione è danneggiata; не използвайте при увредена опаковка; Να μην χρησιμοποιείται εάν η συσκευασία έχει υποστεί ζημιά; Ne pas utiliser si l'emballage est endommagé; Niet gebruiken als de verpakking beschadigd is; Må ikke anvendes, hvis emballagen er ødelagt; Ne használja fel, ha a csomagolás sérült; må ikke brukes hvis pakningen er skadet; не использовать, если упаковка повреждена; Ne koristite ako je pakiranje oštećeno; Não utilizar se a embalagem estiver danificada; Paket hasarlıysa kullanmayın; Nepoužívejte, je-li obal poškozen; A nu se utiliza dacă ambalajul este avariat; nie używać, jeśli opakowanie jest uszkodzone; Nemojte koristiti ako je pakovanje polomljeno

STERILE EO

ISO 15223-1 - Sterilized using ethylene oxide - Esterilizado con óxido de etileno; Steriliserad med etylenoxid; Steriloitu etyleenioksidilla; Mit Ethylenoxid sterilisiert; Sterilizzato ad ossido di etilene; стерилизирано с етиленов оксид; Αποστειρωμένο με χρήση αιθυλενοξειδίου; Stérilisé à l'oxyde d'éthylène; Gesteriliseerd met ethyleenoxide; Steriliseret med ethylenoxid; Etilénoxiddal sterilizálva; sterilisert med etylenoksid; стерилизовано этиленоксидом; Sterilizirano etilen-oksidom; Esterilizado com óxido de etileno; Etilen oksit kullanılarak sterilize edilmiştir; Sterilizováno etylenoxidem; Sterilizat cu oxid de etilenă; wysterylizowano tlenkiem etylenu; Sterilisano korišćenjem etilen-oksida

ISO 15223-1 - Store in a dry, dark, cool place - Guardar en un sitio fresco, oscuro y seco; Förvaras svalt, mörkt och torrt; Säilytä kuivassa, pimeässä ja viileässä.; An einem trockenen, dunklen, kühlen Ort lagern; Conservare in luogo fresco, asciutto e al riparo dalla luce; Съхранявайте на сухо, тъмно и хладно място; Να φυλάσσεται σε ξηρό, σκοτεινό και δροσερό χώρο; Conserver dans un endroit sec et frais à l'abri de la lumière; Op een droge, donkere en koele plaats bewaren; Opbevares tørt, mørkt og køligt.; Száraz, fénytől védett és hűvös helyen tárolandó; Oppbevares på et tørt, mørkt og kjølig sted; Хранить в сухом, темном и прохладном месте; Čuvati na suhom, tamnom i hladnom mjestu; Armazenar em local fresco, seco e escuro; Serin ve kuru bir yerde saklayın; Skladujte v suchu, temnu a chladu; Depozitaţi într-un loc uscat, întunecat şi răcoros; Przechowywać w suchym, ciemnym i chłodnym miejscu; Čuvati na suvom, mračnom, hladnom mestu

ISO 15223-1 - Do not re-use - No reutilizar; Återanvänd inte; Ei saa käyttää uudelleen; Nicht wiederverwenden; Non riutilizzare; не използвайте повторно; Να μην επαναχρησιμοποιείται; Ne pas réutiliser; Niet hergebruiken; Må ikke genbruges; Ne használja fel újra; må ikke brukes på nytt; не использовать повторно; Nemojte ponovo upotrebljavati; Não reutilizar; Yeniden kullanmayın; Nepoužívejte znovu; A nu se reutiliza; nie używać ponownie; Nemojte ponovo da koristite

ISO 15223-1 - Do not resterilize - No volver a esterilizar; Omsterilisera inte; Ei saa steriloida uudelleen; Nicht resterilisieren; Non risterilizzare; не стерилизирайте повторно; Να μην επαναποστειρώνεται; Ne pas restériliser; Niet opnieuw steriliseren; Må ikke resteriliseres; Ne sterilizálja újra; må ikke steriliseres på nytt; не стерилизовать повторно; Nemojte ponovo sterilizirati; Não reesterilizar; Yeniden sterilize etmeyin; Nesterilizujte znovu; A nu se resteriliza; nie sterylizować ponownie; Nemojte sterilizovati

ISO 15223-1 - Non-pyrogenic - Apirógeno; Icke-pyrogen; Pyrogeeniton; Nicht-pyrogen; Apirogeno; непирогенно; Μη πυρογενές; Apyrogène; Pyrogeenvrij; Uden pyrogener; Nem pirogén; ikke-pyrogen; апирогенно; Nepirogeno; Não pirogénico; Pirojenik değildir; Nepyrogenní; Apirogen; wyrób niepirogenny; Nepirogeni

EC REP

ISO 15223-1 - Authorized representative in the European community - Representante autorizado en la Comunidad Europea; Auktoriserad representant i Europeiska gemenskapen; Valtuutettu edustaja Euroopan yhteisössä; Autorisierte EU-Vertretung; Rappresentante autorizzato nella Comunità europea; упълномощен представител в Европейската общност; Εξουσιοδοτημένος αντιπρόσωπος στην Ευρωπαϊκή κοινότητα; Représentant autorisé pour la Communauté européenne; Erkende vertegenwoordiger in de Europese gemeenschap; Autoriseret repræsentant i EU; Hivatalos képviselő az Európai Közösségben; autorisert EU-representant; уполномоченный представитель в Европейском сообществе; Ovlašteni zastupnik za Europsku zajednicu; Representante autorizado na Comunidade Europeia; Avrupa topluluğu yetkili temsilcisi; Autorizovaný zástupce v Evropském společenství; Reprezentant autorizat în Comunitatea Europeană; autoryzowany przedstawiciel na terenie Unii Europejskiej; Ovlašćeni predstavnik za Evropsku zajednicu

IEC 60878 2794 – Use by date - Fecha de caducidad; Sista förbrukningsdag; Viimeinen käyttöpäivä; Verfallsdatum; Utilizzare entro; срок на годност; Τελική ημερομηνία ανάλωσης; Date limite d'utilisation; Uiterste gebruiksdatum; Sidste anvendelsesdato; Lejárati dátum; utløpsdato; използвать до; Upotrijebiti do; Data de validade; Son kullanma tarihi; Datum použitelnosti; A se utiliza până la data de; termin ważności; Rok trajanja

1

IEC 60878 2794 - Packaging unit - Unidad de embalaje; Förpackningsenhet; Pakkausyksikkö; Verpackungseinheit; Unità di imballaggio; опаковъчна единица; Μονάδα συσκευασίας; Unité de conditionnement; Verpakking; Emballageenhed; Csomagolási egység; emballasjeenhet; упаковочная единица; Pakiranje; Unidade de embalagem; Paket ünitesi; Balicí jednotka; Unitate ambalare; jednostka opakowania; Jedinica pakovanja

INCLUDED ACCESSORIES: 3cc syringe; One (1) 10cc syringe; One (1) Extension tube; One (1) 3-way stopcock; One (1) SpinVision Sterile Equipment cover; One (1)	ВКЛЮЧЕНИ АКСЕСОАРИ: 3 cc спринцовка; Един (1) брой 10 cc спринцовка; Един (1) брой Удължителна тръба; Един (1) брой 3-пътно спирателно кранче; Един (1) брой Стерилна покривка за оборудване SpinVision; Един (1) брой	PRILOŽENI PRIBOR: štrcaljka od 3 cc; jedna (1) štrcaljka od 10 cc jedna (1) produžna cijev; jedna (1) trosmjerna zaporna skretnica; jedna (1) sterilni pokrov za opremu SpinVision; jedan (1)	DODÁVANÉ PŘÍSLUŠENSTVÍ: Injekční stříkačka o objemu 3 ccm, Jedna (1) Injekční stříkačka o objemu 10 ccm, Jedna (1) Prodlužovací hadička, Jeden (1) Trojcestný kohout, Jeden (1) Kryt sterilního zařízení SpinVision, Jeden (1)
MEDFØLGENDE TILBEHØR: 3 ml sprøjte; Én (1) 10 ml sprøjte; Én (1) Forlængerslange; Én (1) 3-vejs stophane; Én (1) SpinVision sterilt overtræk til udstyr; Ét (1)	MEEGELEVERDE ACCESSOIRES: Spuit van 3 cc; Een (1) Spuit van 10 cc; Een (1) Verlengslang; Een (1) 3-wegafsluitkraan; Een (1) SpinVision steriele apparatuurafdekking; Een (1)	KAASASOLEVAD TARVIKUD 3 cc süstal: üks (1) 10 cc süstal: üks (1) Pikenduspuoolik: üks (1) 3-suunaline sulgekraan: üks (1) SpinVisioni steriilne seadmekate: üks (1)	MUKANA TOIMITETTAVAT LISÄVARUSTEET: 3 ml:n ruisku; Yksi (1) 10 ml:n ruisku; Yksi (1) Jatkoletku; Yksi (1) 3-tiesulkuhana; Yksi (1) Steriili SpinVision-laitesuoja; Yksi (1)
ACCESSOIRES INCLUS : Seringue 3 cc ; une (1) Seringue 10 cc ; une (1) Tube d'extension ; un (1) Robinet à 3 voies ; un (1) Housse d'équipement stérile SpinVision ; une (1)	ENTHALTENES ZUBEHÖR: 3-ml-Spritze; ein Stück (1) 10-ml-Spritze; ein Stück (1) Verlängerungsschlauch; ein Stück (1) Dreiwegehahn; ein Stück (1) SpinVision sterile Gerateabdeckung; ein Stück (1)	ΠΑΡΕΑΚΟΜΕΝΑ ΠΟΥ ΣΥΜΠΕΡΙΛΑΜΒΑΝΟΝΤΑΙ: σύριγγα 3cc, Ένα (1) σύριγγα 10cc, Ένα (1) Σωλήνας επέκτασης, Ένα (1) 3-οδη στρόφιγγα, Ένα (1) Στείρο κάλυμμα εξοπλισμού SpinVision, Ένα (1)	MELLÉKELT TARTOZÉKOK: 3 cm3-es fecskendő; Egy (1) 10 cm3-es fecskendő; Egy (1) Hosszabbító cső; Egy (1) Háromállású csap; Egy (1) SpinVision steril védőhuzat; Egy (1)
ACCESSORI INCLUSI: Siringa da 3 cc; uno (1) Siringa da 10 cc; uno (1) Tubo di estensione; uno (1) Rubinetto a tre vie; uno (1) Protezione sterile per apparecchiatura SpinVision; uno (1)	INKLUDERT TILBEHØR: 3 cc sprøyte; Én (1) 10 cc sprøyte; Én (1) Forlengelsesslange; Én (1) Treveis stoppekran; Én (1) SpinVision sterilt utstyrsdeksel; Én (1)	DOŁĄCZONE AKCESORIA: Strzykawka 3 cm3; jedna (1) sztuka Strzykawka 10 cm3; jedna (1) sztuka Przewód przedłużający; jedna (1) sztuka Zawór 3-drożny; jedna (1) sztuka Osłona SpinVision Sterile Equipment; jedna (1) sztuka	ACCESORII INCLUSE: Seringă de 3 cc; Una (1) Seringă de 10 cc; Una (1) Tub de extensie; Unul (1) Robinet de oprire cu trei căi; Unul (1) Husă echipament steril SpinVision; Una (1)
MEDFÖLJANDE TILLBEHÖR: Spruta på 3 cc: En (1) Spruta på 10 cc: En (1) Förlängningsrör: Ett (1) 3-vägs avstängningskran: En (1) SpinVision – hölje för steril utrustning: Ett (1)	ACESSÓRIOS INCLUÍDOS: Seringa de 3cc; Uma (1) seringa de 10cc; Um (1) Tubo de extensão; Uma (1) Torneira de 3 vias; Uma (1) Tampa para equipamento estéril SpinVision; Uma (1)	DAHİL OLAN AKSESUARLAR: 3 cc şırınga; Bir (1) 10 cc şırınga; Bir (1) Uzatma hortumu; Bir (1) 3 yönlü vana; Bir (1) SpinVision Steril Ekipman kılıfı; Bir (1)	В КОМПЛЕКТ ВХОДЯТ СЛЕДУЮЩИЕ ПРИНАДЛЕЖНОСТИ: Шприц объемом 3 куб. см; одна (1) шт. Шприц объемом 10 куб. см; одна (1) шт. Удлинительная трубка; одна (1) шт. 3-ходовой запорный кран; одна (1) шт. Стерильный чехол для оборудования SpinVision; одна (1) шт.
UKLJUČENI DODACI: Špric od 3 CC; Jedan (1) Špric od 10 CC; Jedan (1) Produžna cev; Jedna (1) 3-smerni sigurnosni ventil; Jedan (1) Sterilna navlaka za opremu SpinVision; Jedna (1)			

Rx ONLY

FDA final rule - Prescription only - Norma final de la FDA: Solo con prescripción médica; Slutlig FDA-regel – endast på ordination; FDA:n lopullinen sääntö – Vain lääkärin määräyksestä; Endgültige FDA-Entscheidung – Rezeptpflichtig; Norma definitiva FDA - Solo su prescrizione; Последно правило на FDA – само по предписание; Τελικός κανόνας FDA - Μόνο κατόπιν ιατρικής συνταγής; Règlement final de la FDA – Sur prescription uniquement; Oordeel FDA - Alleen op recept; FDA endelig beslutning - Kun på recept; FDA végső szabály – Csak rendelvényre; Endelig avgjørelse fra Food and Drug Administration (FDA) – selges kun på resept; окончательное правило FDA — только по предписанию; Konačna odluka agencije FDA – samo na recept; Regra final da FDA – Apenas com receita médica; Nihai FDA kuralı - Yalnızca reçete ile satılır; Konečné pravidlo FDA – Pouze na předpis; Regulament final FDA - Doar pe bază de prescripţie; Przepis końcowy FDA – tylko na zlecenie lekarza; Konačno pravilo agencije FDA - Samo po nalogu zdravstvenog radnika

LATEX

Not made with natural rubber latex - No está fabricado con látex de caucho natural; Inte framställd med naturgummilatex; Valmistuksessa ei ole käytetty luonnonkumia/lateksia; Nicht mit Naturlatex hergestellt; Non realizzato in lattice di gomma naturale; Не е произведено с естествен каучуков латекс; Δεν κατασκευάζεται με λάτεξ από φυσικό καουτσούκ; Fabriqué sans latex de caoutchouc naturel; Niet gemaakt met natuurlijke rubberlatex; Ikke fremstillet med naturgummilatex; Természetes gumilatexet nem tartalmaz; Inneholder ikke naturgummilateks; изготовлено без применения натурального каучукового латекса; Nije izrađeno od prirodnoga gumenog lateksa; Fabricado sem látex de borracha natural; Doğal kauçuk lateksten üretilmemiştir; Není vyrobeno za použití přírodního latexu; Nu este fabricat cu latex din cauciuc natural; Wyprodukowano bez dodatku naturalnej gumy lateksowej; Ne sadrži prirodni gumeni lateks

PN

Part number - Número de referencia; Artikelnummer; Osanumero; Teilenummer; Numero di parte; Каталожен номер; Αριθμός προϊόντος; Référence; Onderdeelnummer; Reservedelsnummer; Cikkszám; Delenr.; номер по каталогу; Broj dijela; Referência; Parça numarası; Číslo; Numărul de catalog; Numer wyrobu; Broj dela