



Subject-level mean calibration gap (red = FDR-rejected at $\alpha=0.05$)


GPT-4o-mini

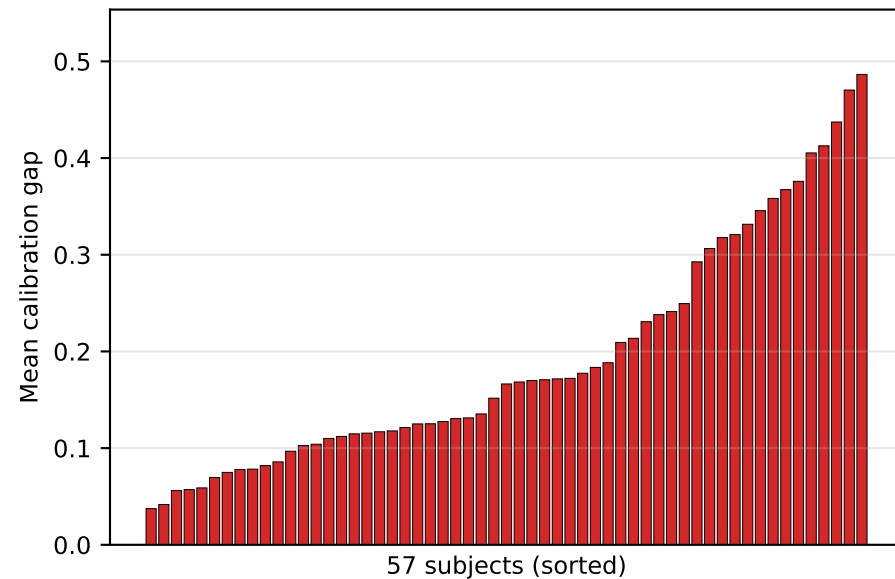


Llama-3-8B

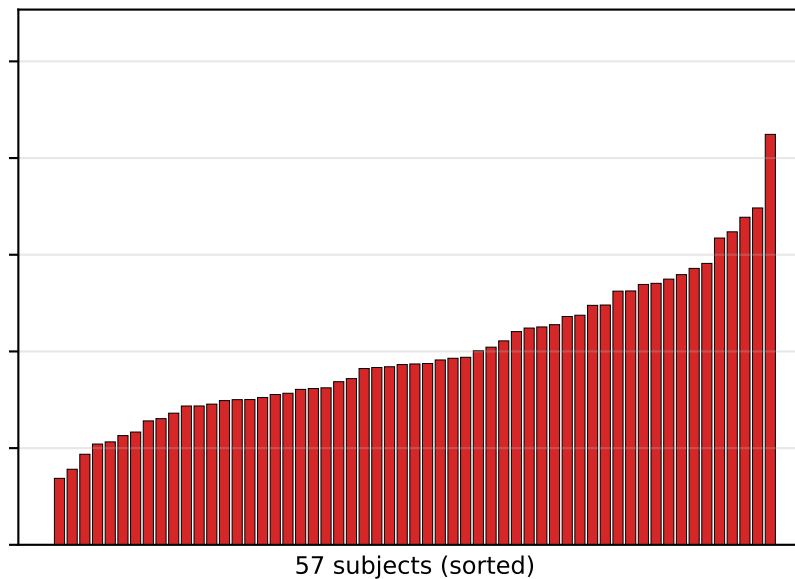


Qwen-0.5B

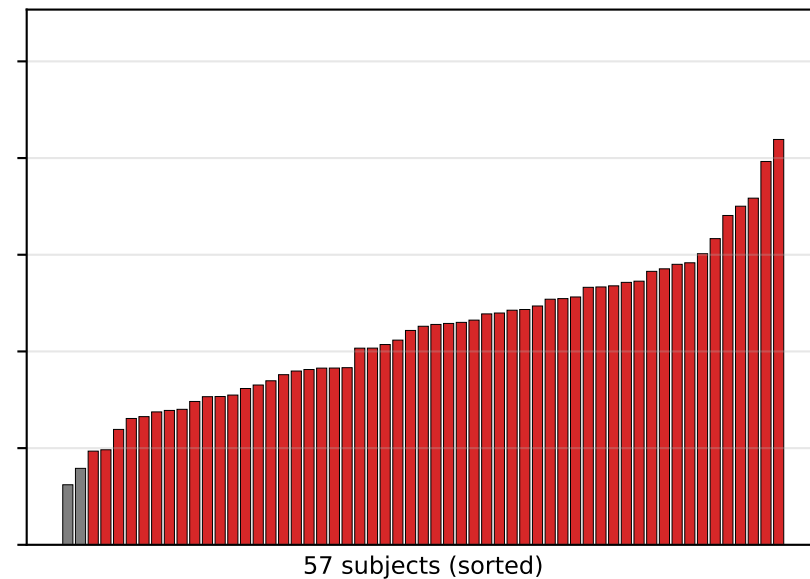

Qwen-1.5B

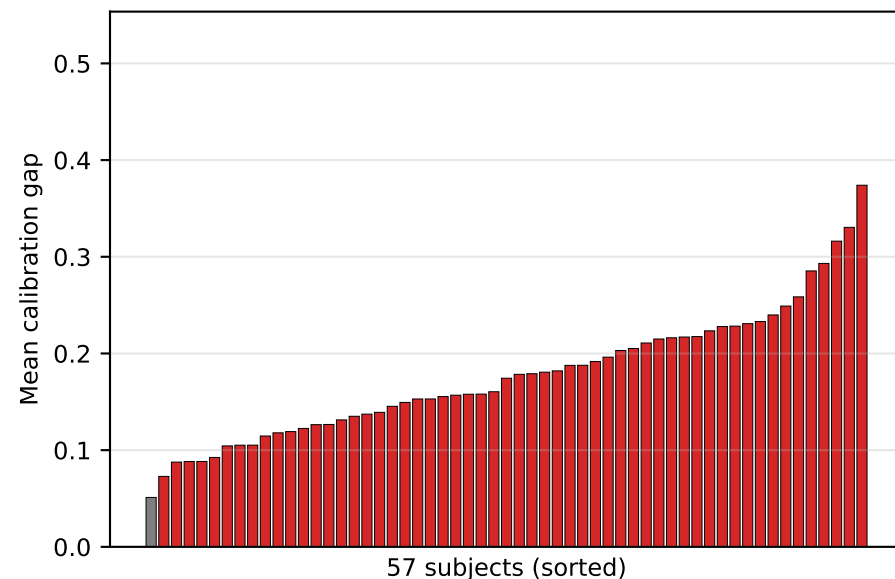

Qwen-7B

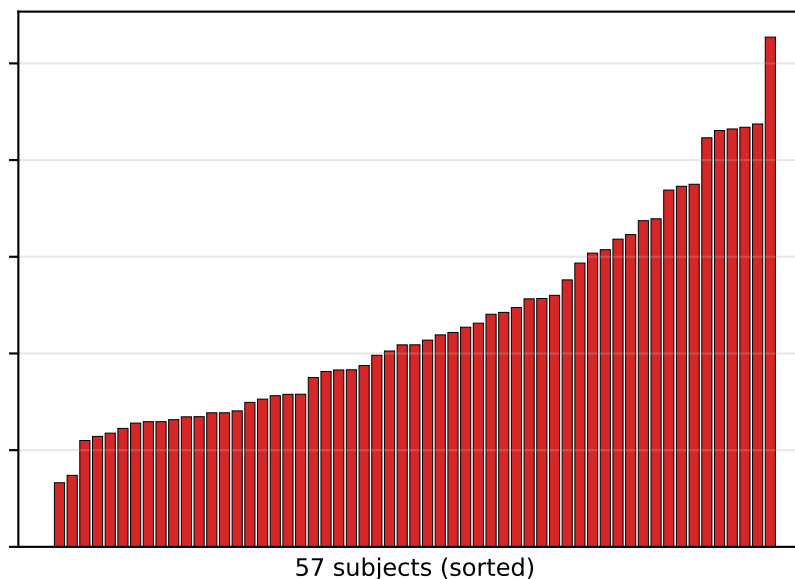

Qwen-14B

