



STF-09-MR-187187: Pressure Oscillations in Slow-filling


Raw LV Pressure Trace

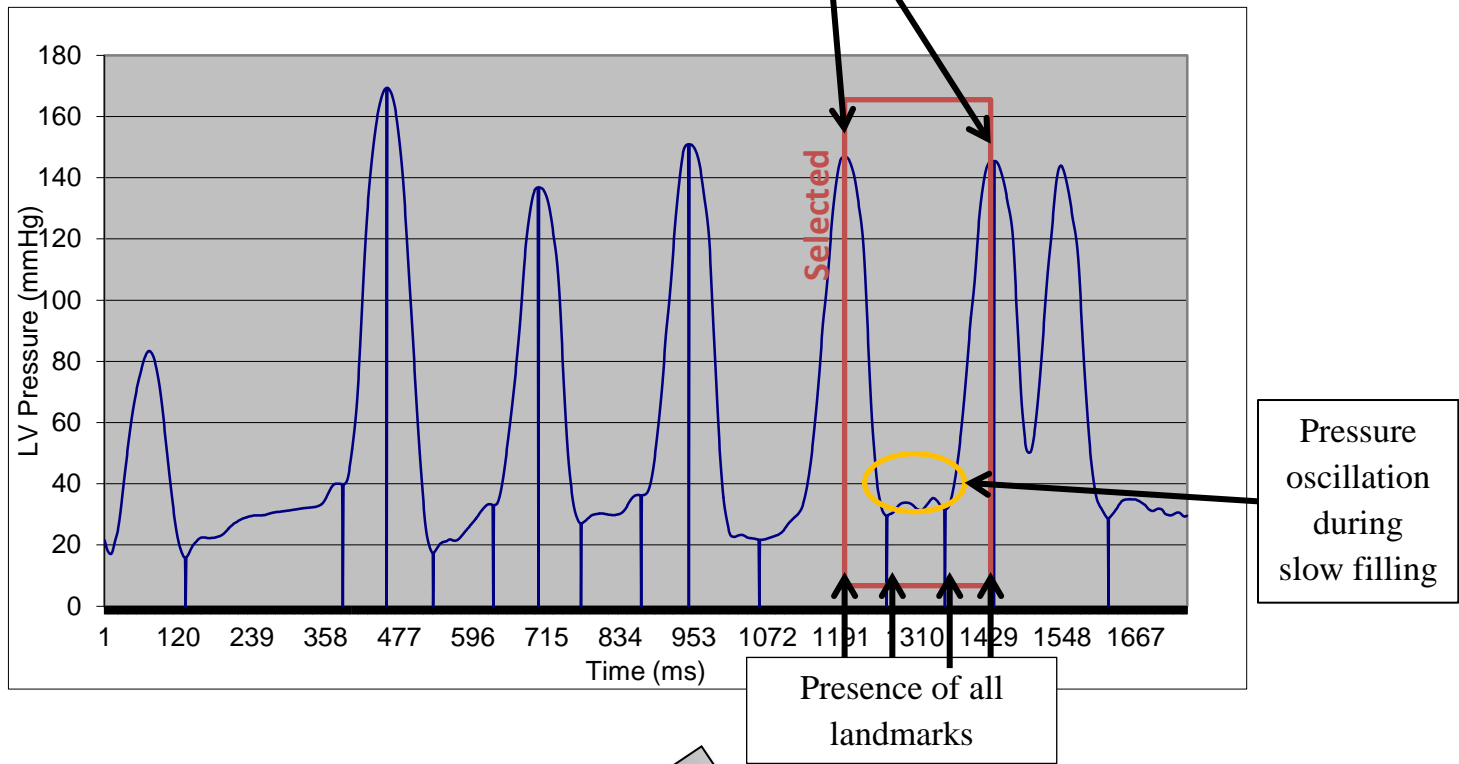

Raw Aortic Pressure Trace

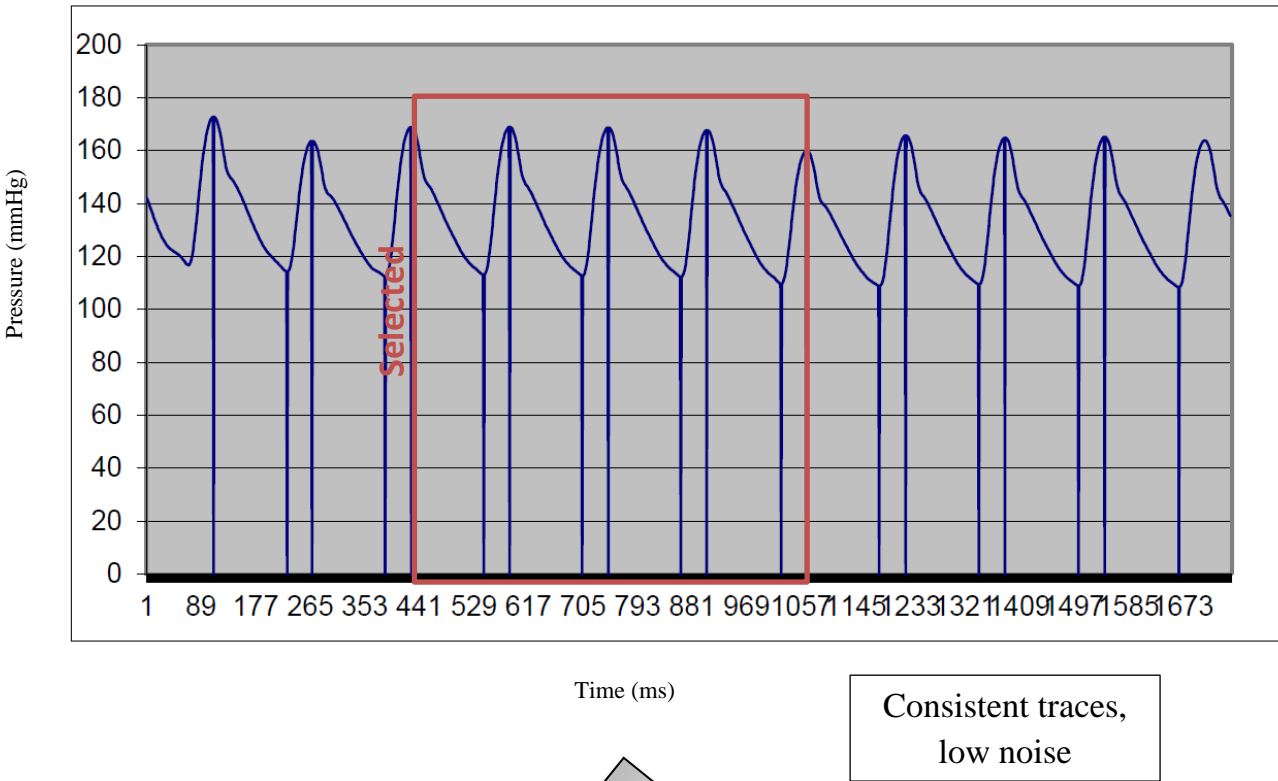


Alignment of Timing

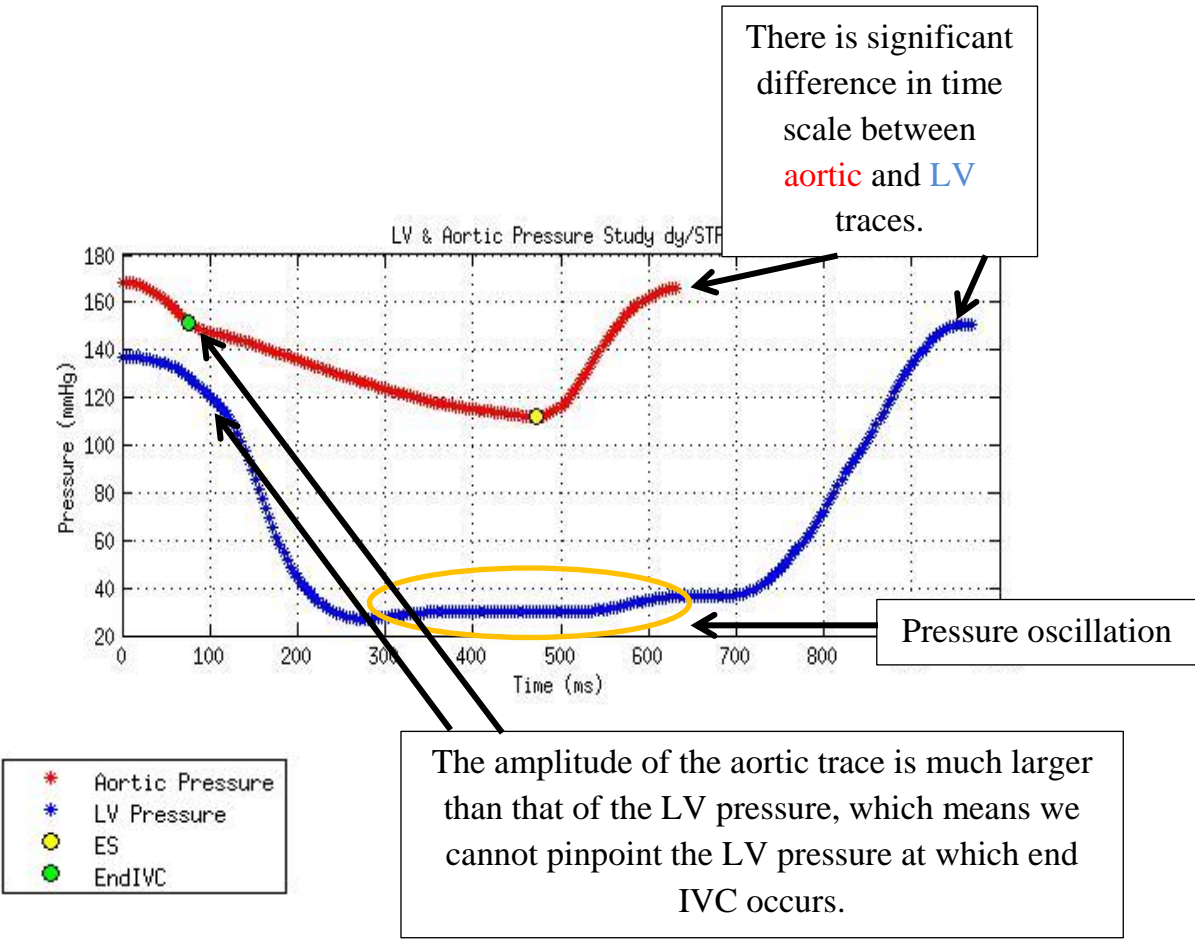


STF-11-MR-152152: Noisy Pressure trace & alternans (?)


Raw LV Pressure Trace

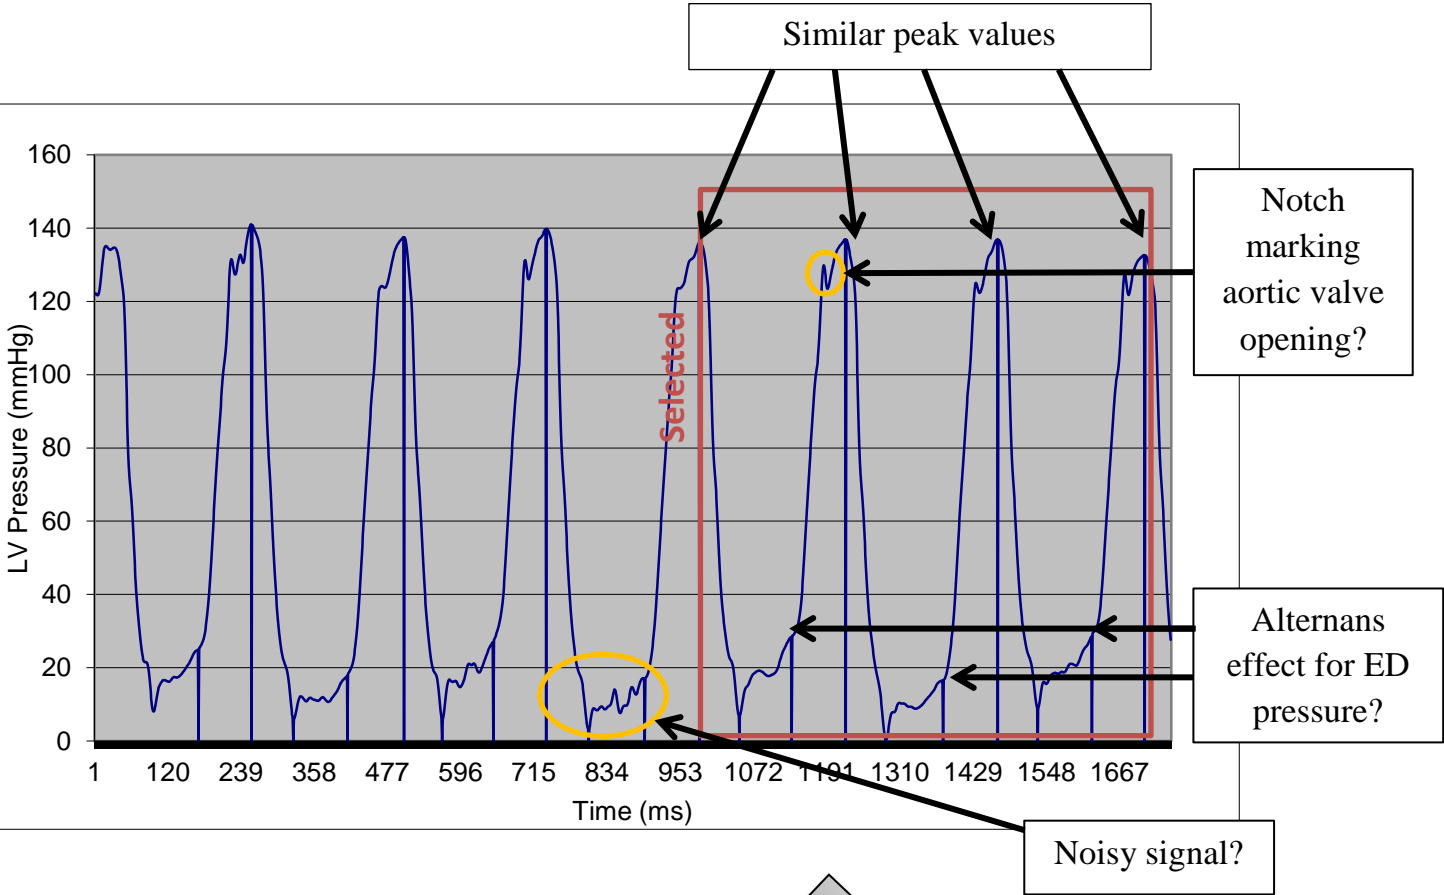

Raw Aortic Pressure Trace

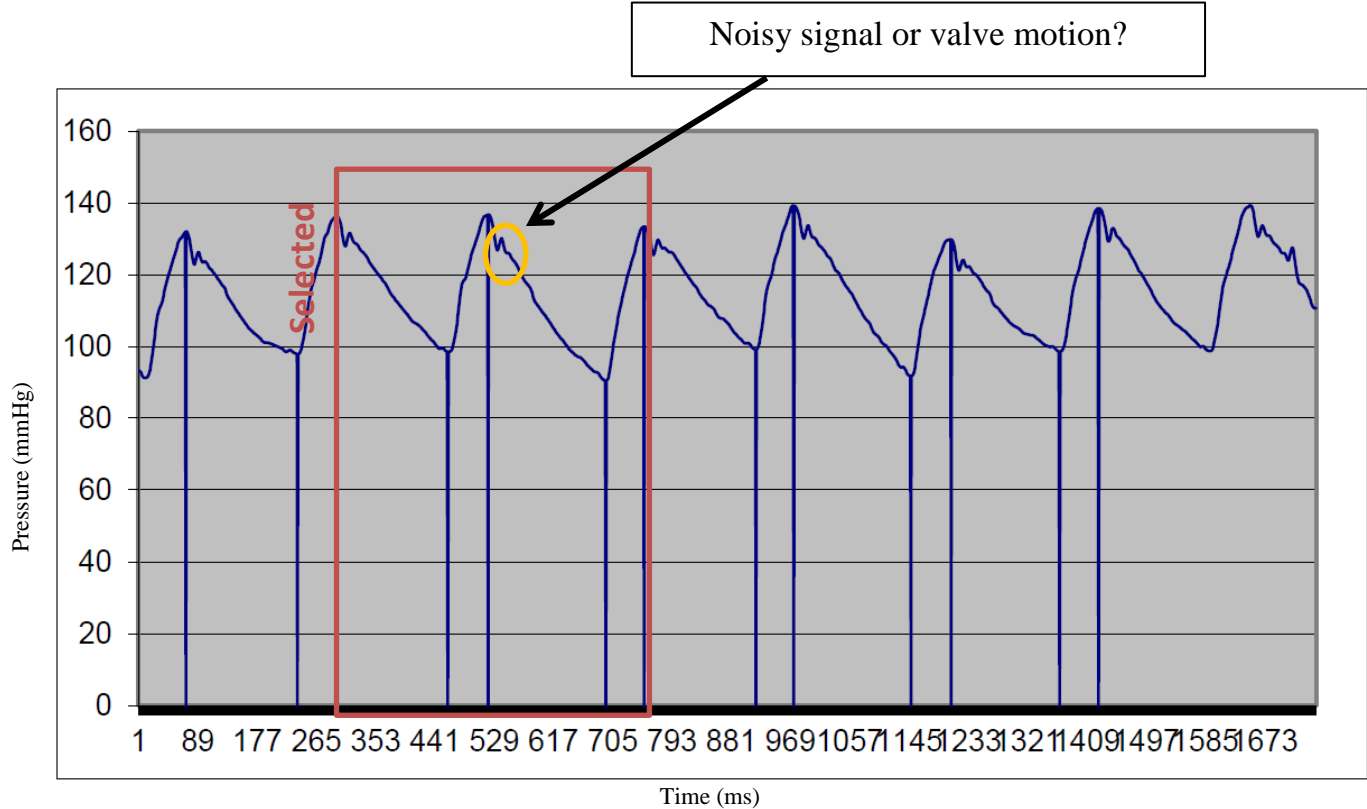


Alignment of Timing

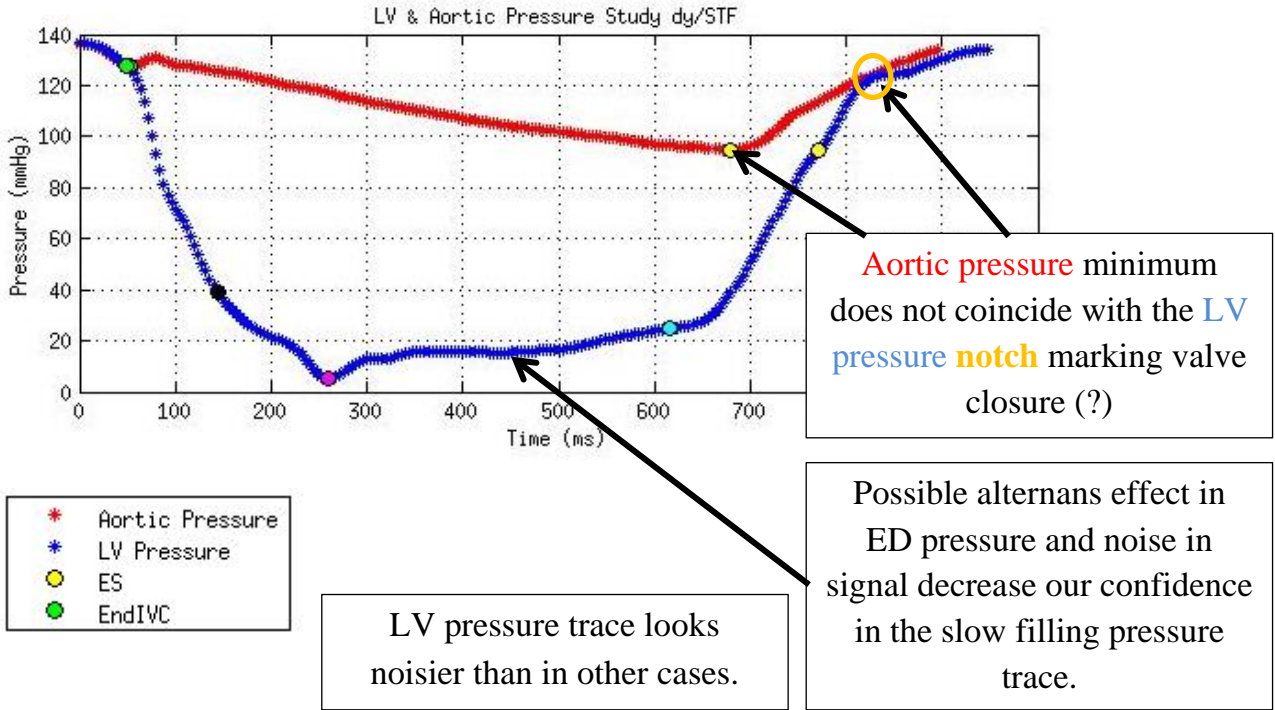


STF-13-MR-273273: Alternans -> pressure peak discontinuity


Raw LV Pressure Trace

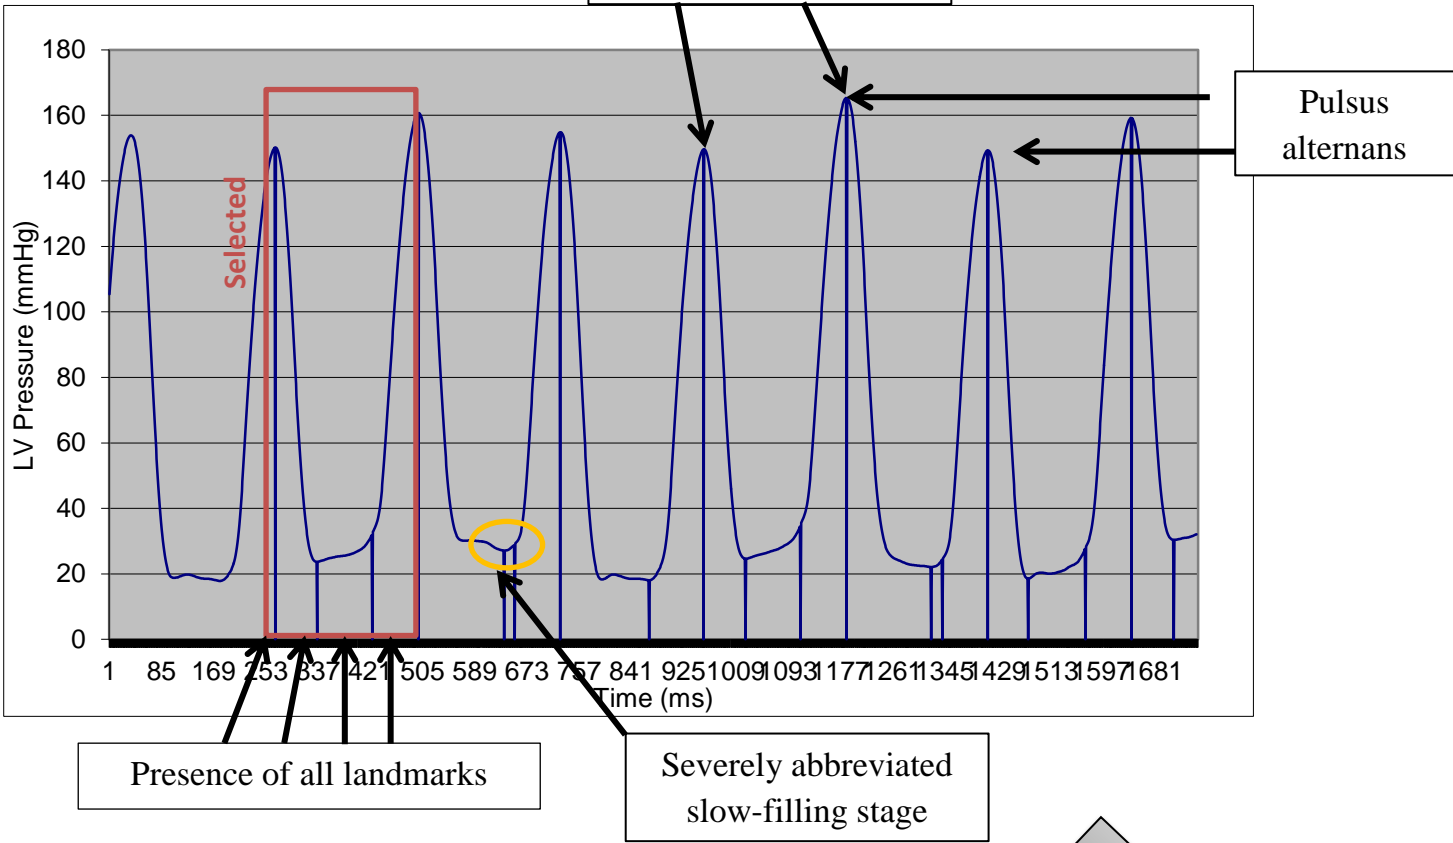

Raw Aortic Pressure Trace

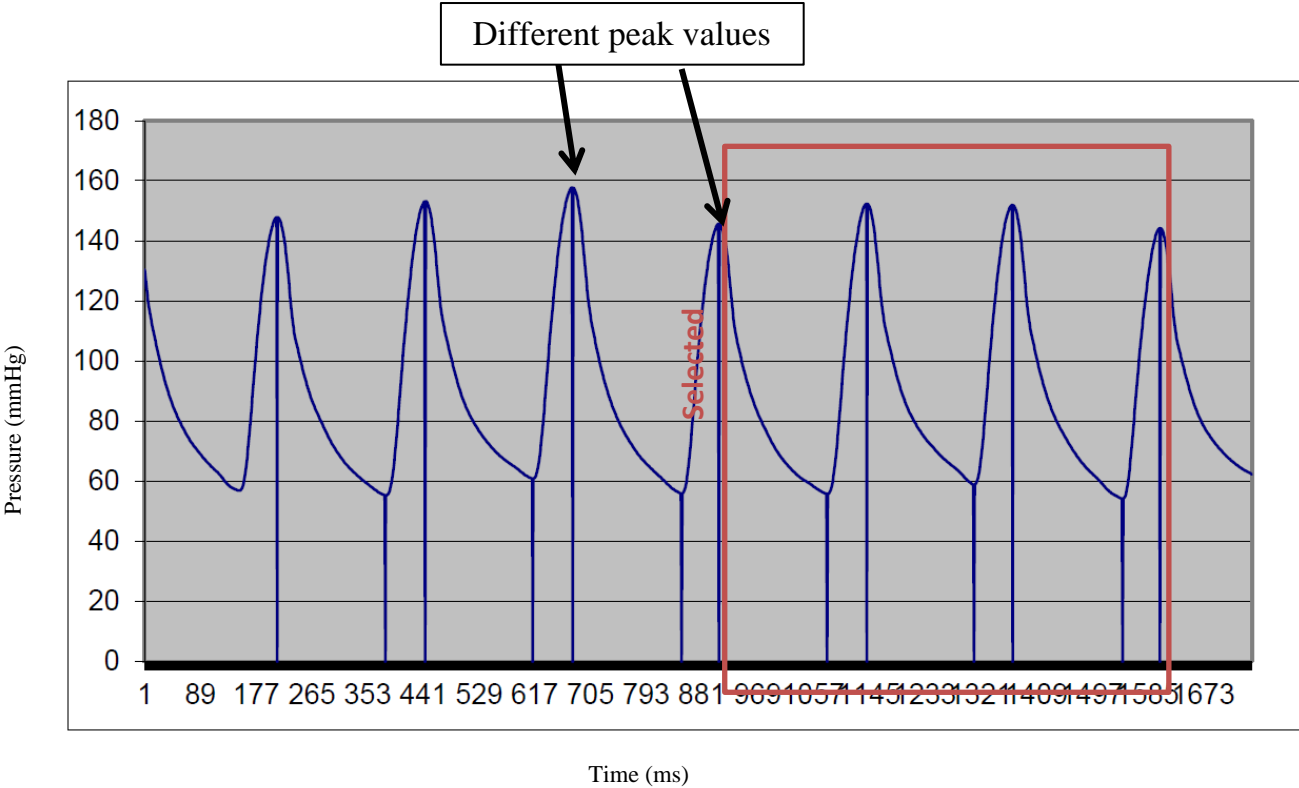


Alignment of Timing

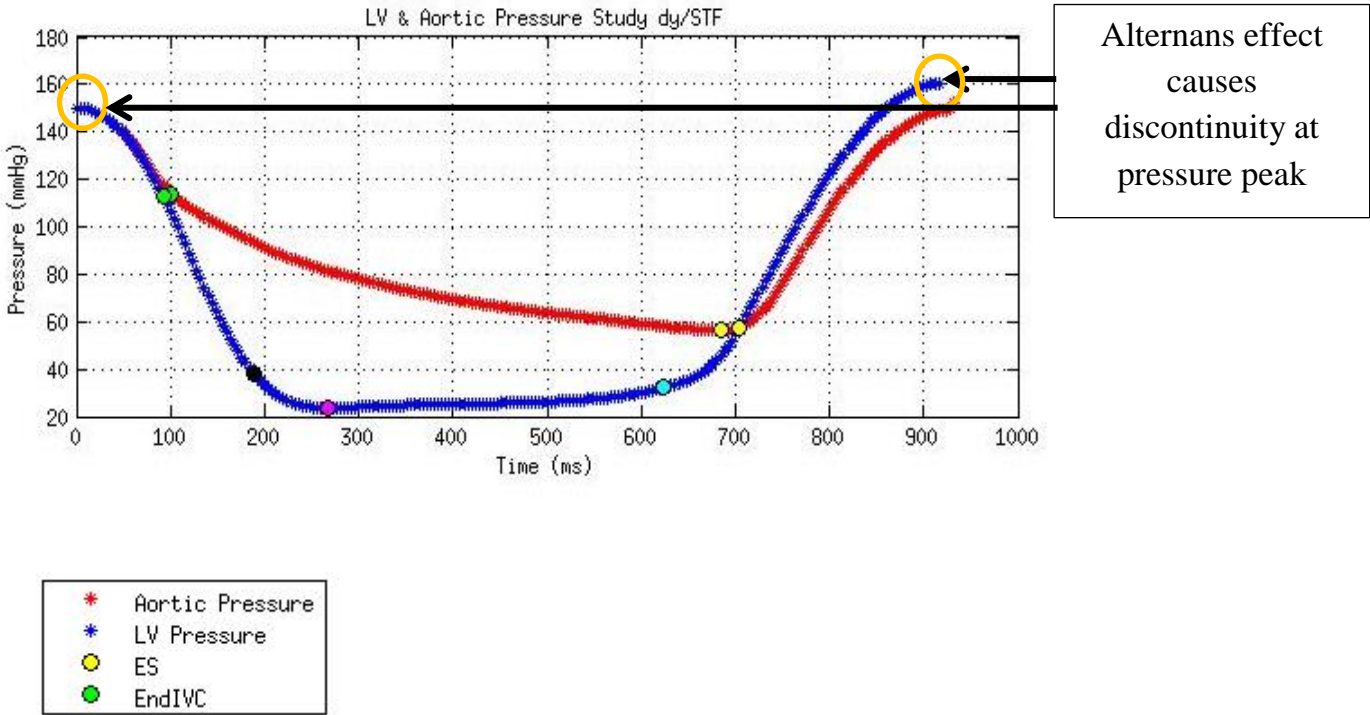

STF-10-MR-220220: Relatively good


Raw LV Pressure Trace

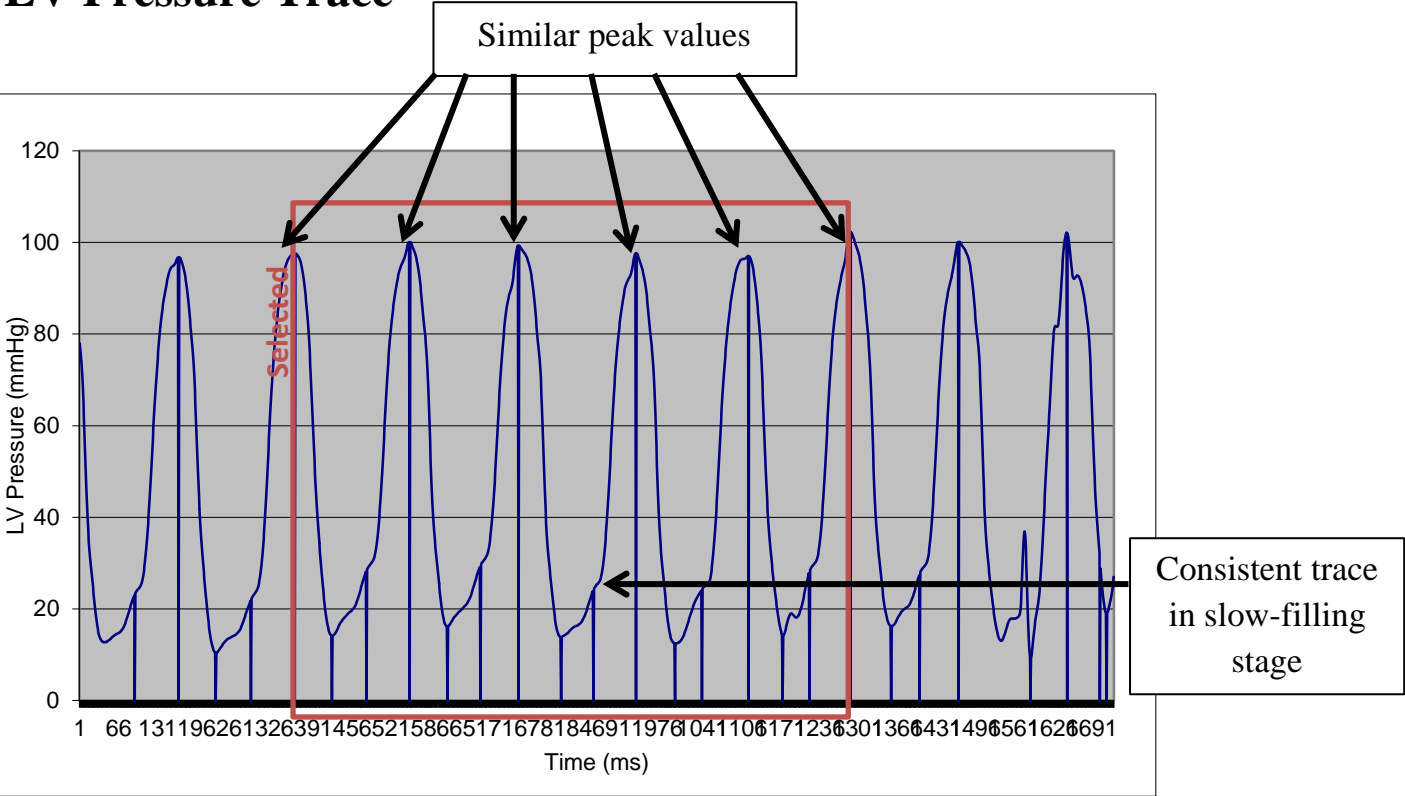

No pressure oscillations during slow-filling

Minimal noise


Raw Aortic Pressure Trace

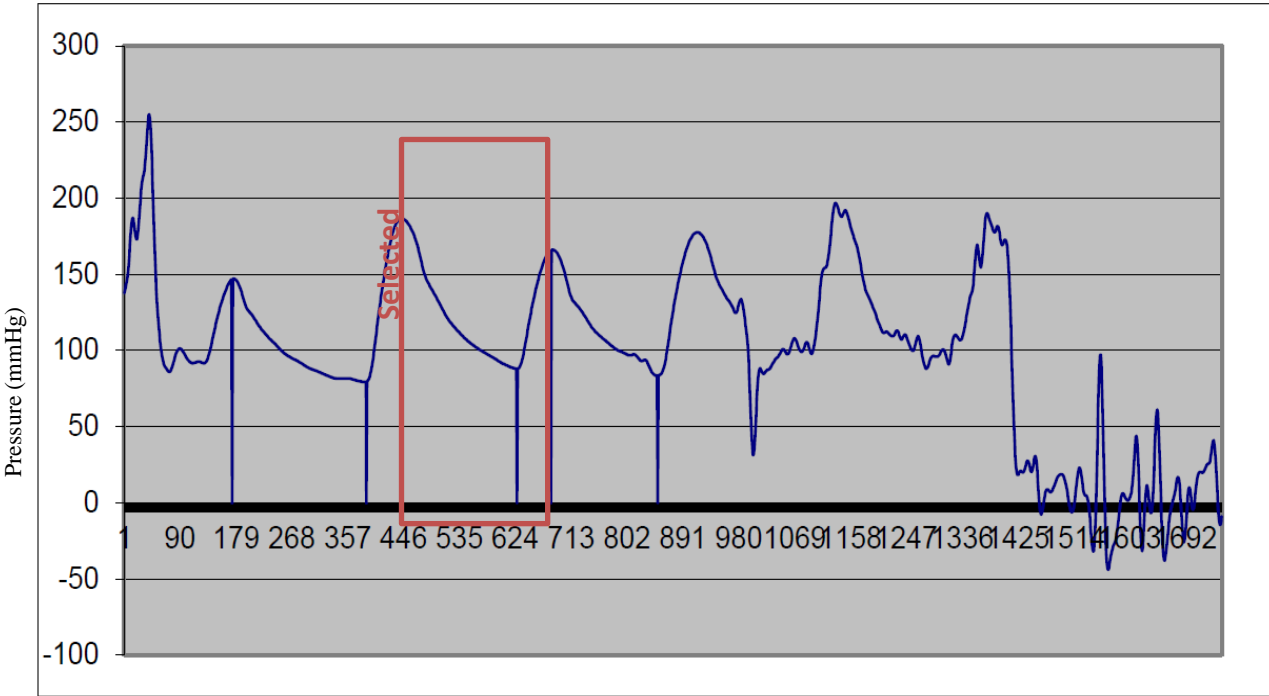

Only one usable cycle

Peak values vary greatly


Alignment of Timing

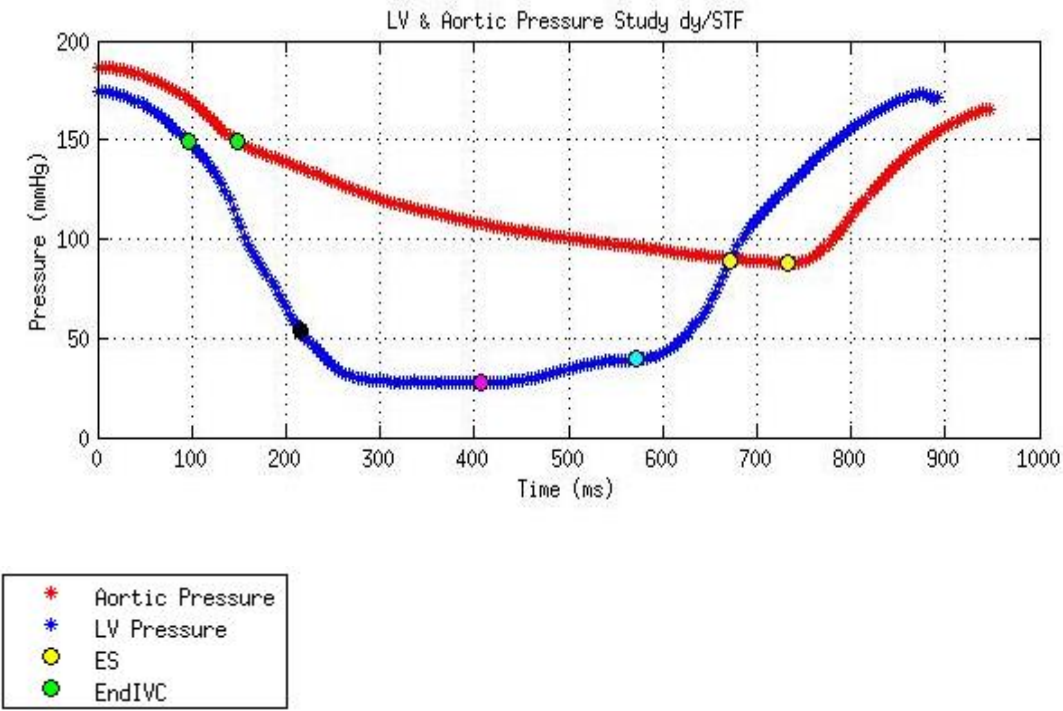




STF-01-MR-TE: Good

Raw Pressure Trace

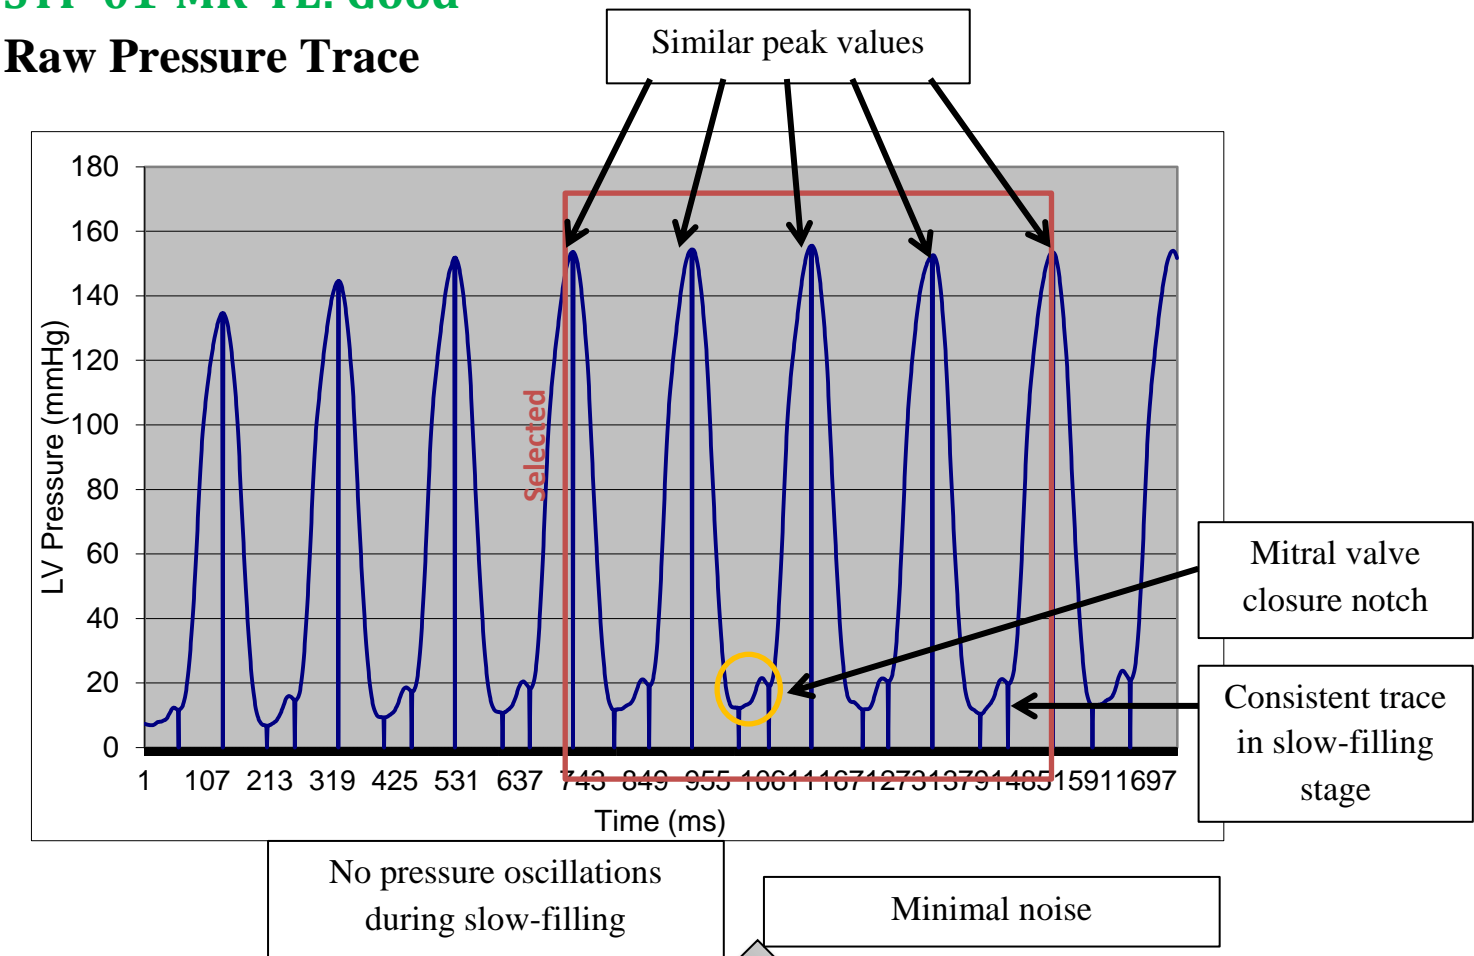

Raw Aortic Pressure Trace

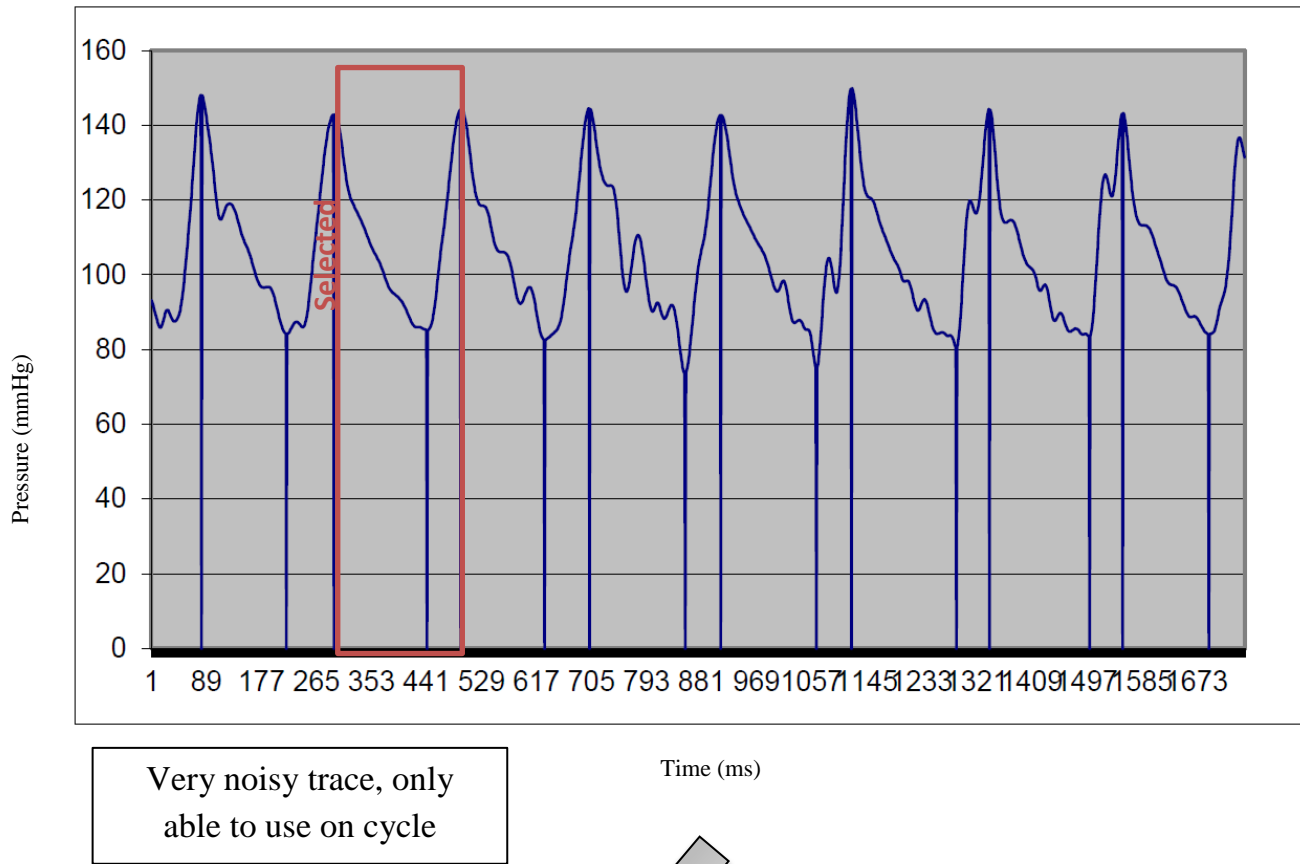

Alignment of Timing

