


Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13804685_2026-03-29_16-04-48.xad

Created: 3/29/2026 4:04:48 PM
Modified: 3/29/2026 5:12:37 PM

Electrophoresis File Run Summary

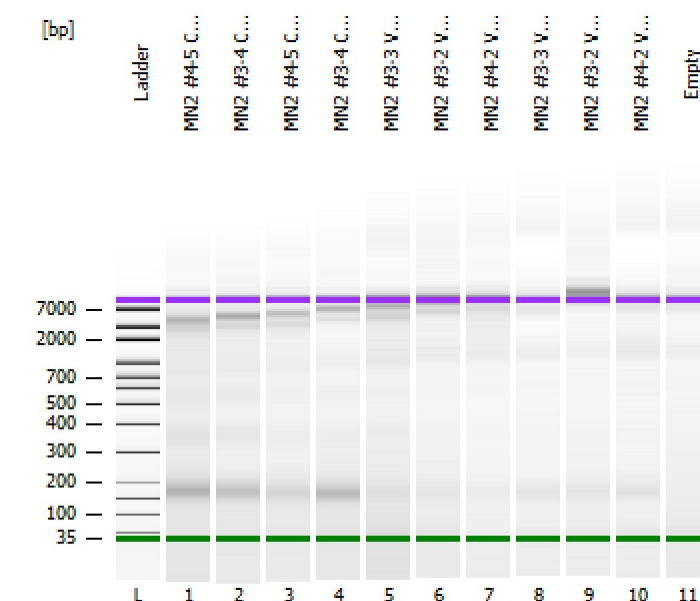

Instrument Information:

Instrument Name: DE13804685
Serial#: DE13804685
Firmware: C.01.069
Type: G2939A


Assay Information:

Assay Origin Path: C:\Program Files (x86)\Agilent\2100 bioanalyzer\2100 expert\assays\dsDNA\High Sensitivity DNA.xsy
Assay Class: High Sensitivity DNA Assay
Version: 1.03
Assay Comments: Copyright © 2003-2010 Agilent Technologies


Chip Information:

Chip Lot #:
Reagent Kit Lot #:
Chip Comments:


MN2 #4-5 Combo (2/12/2026)

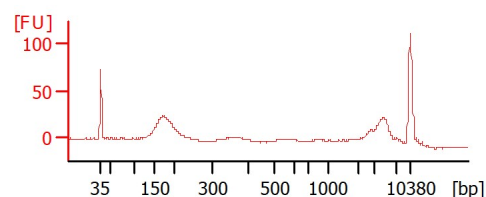


MN2 #3-4 Combo (2/12/2026)

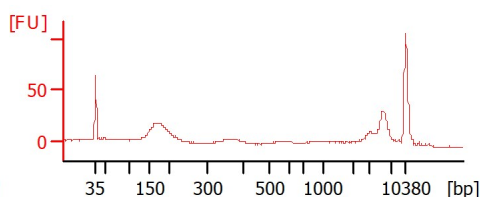


MN2 #4-5 Combo (2/19/2026)

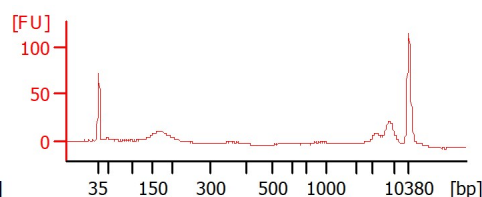


MN2 #3-4 Combo (2/19/2026)

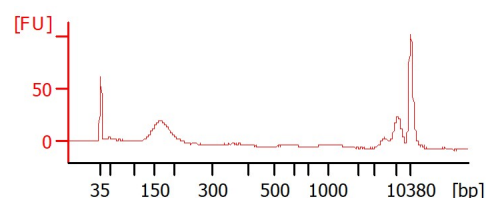


MN2 #3-3 Veh (2/12/2026)

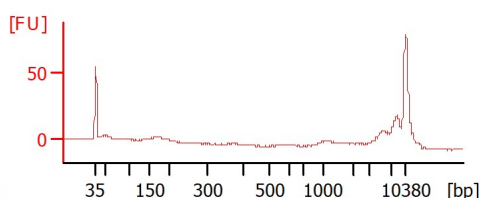


MN2 #3-2 Veh (2/12/2026)

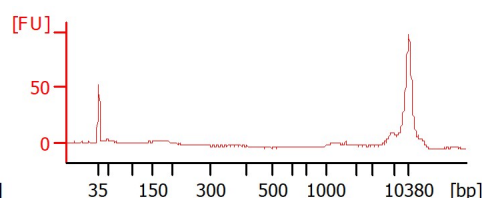


MN2 #4-2 Veh (2/12/2026)

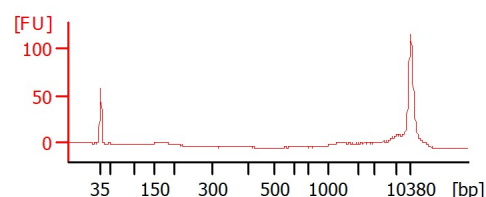


MN2 #3-3 Veh (2/19/2026)

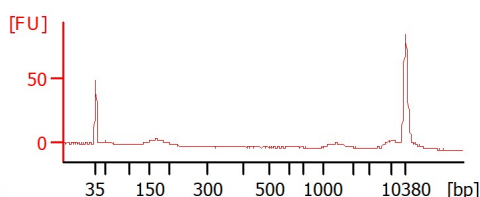


MN2 #3-2 Veh (2/19/2026)

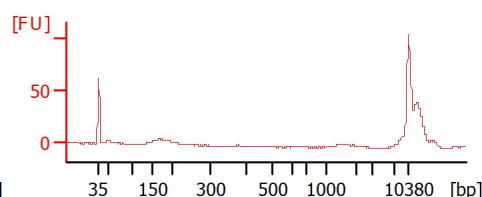

MN2 #4-2 Veh (2/19/2026)

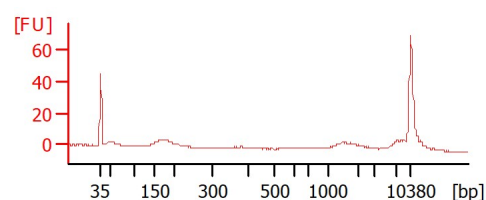

Empty

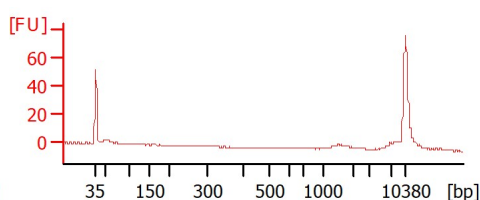

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13804685_2026-03-29_16-04-48.xad

Created: 3/29/2026 4:04:48 PM
Modified: 3/29/2026 5:12:37 PM

Electrophoresis File Run Summary (Chip Summary)

Sample Name	Sample Comment	Rest. Digest	Status	Observation	Result Label	Result Color
MN2 #4-5 Combo (2/12/2026)		☐	✓			
MN2 #3-4 Combo (2/12/2026)		☐	✓			
MN2 #4-5 Combo (2/19/2026)		☐	✓			
MN2 #3-4 Combo (2/19/2026)		☐	✓			
MN2 #3-3 Veh (2/12/2026)		☐	✓			
MN2 #3-2 Veh (2/12/2026)		☐	✓			
MN2 #4-2 Veh (2/12/2026)		☐	✓			
MN2 #3-3 Veh (2/19/2026)		☐	✓			
MN2 #3-2 Veh (2/19/2026)		☐	✓			
MN2 #4-2 Veh (2/19/2026)		☐	✓			
Empty		☐	✓			
Ladder		☐	✓			
Chip Lot #			Reagent Kit Lot #			

Chip Comments :

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13804685_2026-03-29_16-04-48.xad

Created: 3/29/2026 4:04:48 PM
Modified: 3/29/2026 5:12:37 PM

Electrophoresis Assay Details

General Analysis Settings

Number of Available Sample and Ladder Wells (Max.) : 12
Minimum Visible Range [s] : 32
Maximum Visible Range [s] : 138
Start Analysis Time Range [s] : 33
End Analysis Time Range [s] : 137.5
Ladder Concentration [pg/μl] : 1950
Uses Standard Area for Ladder Fragments
Lower Marker Concentration [pg/μl] : 125
Upper Marker Concentration [pg/μl] : 75
Used Upper Marker for Quantitation
Standard Curve Fit is Point to Point
Show Data Aligned to Lower and Upper Marker

Integrator Settings

Integration Start Time [s] : 33.05
Integration End Time [s] : 137
Slope Threshold : 0.8
Height Threshold [FU] : 5
Area Threshold : 0.1
Width Threshold [s] : 0.6
Baseline Plateau [s] : 0.5

Filter Settings

Filter Width [s] : 0.5
Polynomial Order : 4


Ladder

Ladder Peak	Size	Area
1	35	160
2	50	210
3	100	208
4	150	221
5	200	242
6	300	270
7	400	305
8	500	306
9	600	336
10	700	321
11	1000	366
12	2000	413
13	3000	411
14	7000	400
15	10380	214

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13804685_2026-03-29_16-04-48.xad

Created: 3/29/2026 4:04:48 PM
 Modified: 3/29/2026 5:12:37 PM

Electropherogram Summary

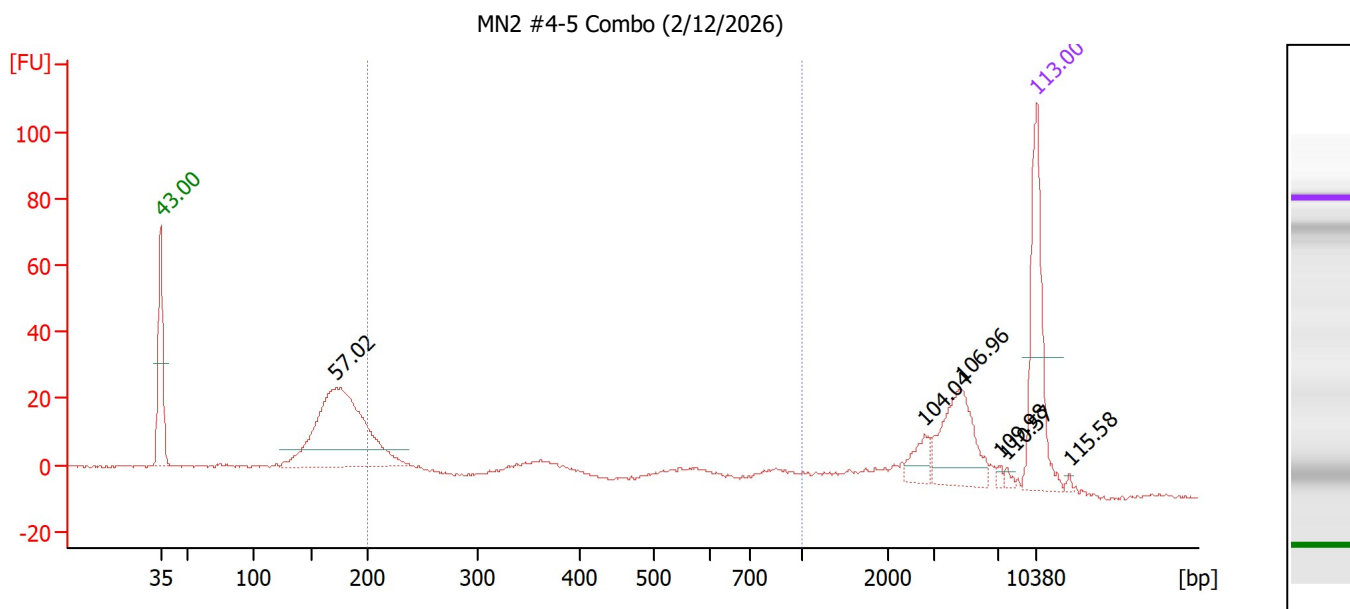

Overall Results for sample 1 : MN2 #4-5 Combo (2/12/2026)

Number of peaks found: 6 Corr. Area 1: 198.4
 Noise: 0.5

Peak table for sample 1 : MN2 #4-5 Combo (2/12/2026)

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	172	251.43	2,214.3	
3	2,817	15.91	8.6	Upper Marker
4	4,746	59.63	19.0	
5	7,122	2.74	0.6	
6	7,753	2.61	0.5	
7	10,380	75.00	10.9	
8	13,165	0.00	0.0	

Region table for sample 1 : MN2 #4-5 Combo (2/12/2026)


From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	198.4	30	456	47.1	209.73	953.2	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13804685_2026-03-29_16-04-48.xad

Created: 3/29/2026 4:04:48 PM
 Modified: 3/29/2026 5:12:37 PM

Electropherogram Summary Continued ...

MN2 #3-4 Combo (2/12/2026)

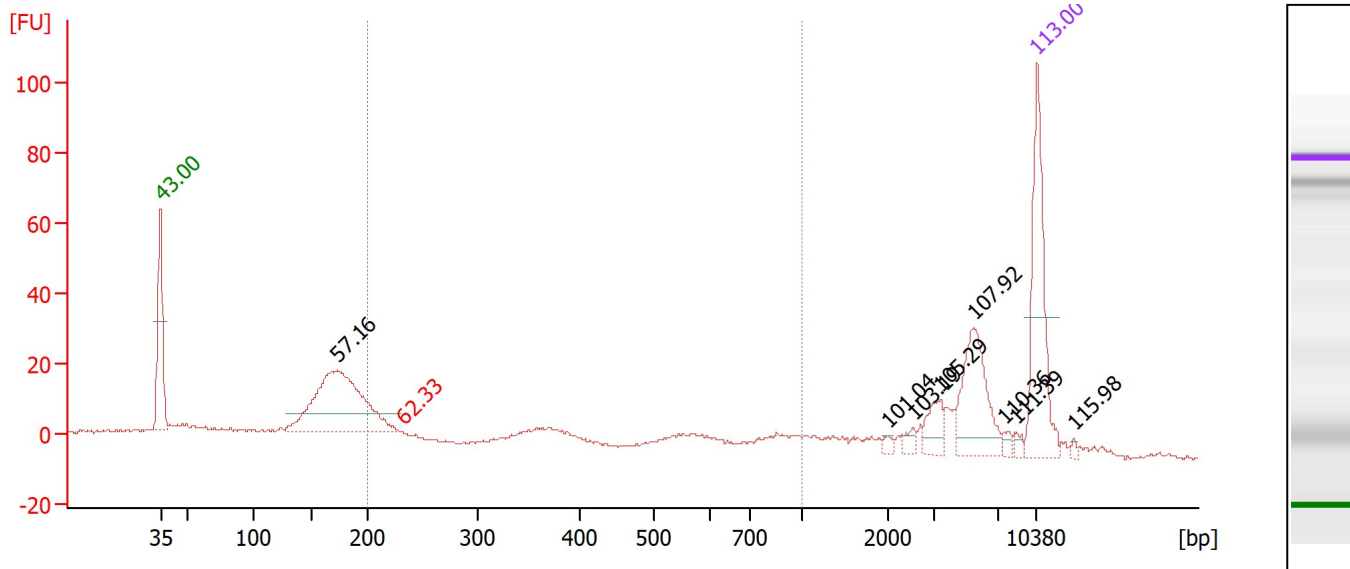

Overall Results for sample 2 : MN2 #3-4 Combo (2/12/2026)

Number of peaks found: 8 Corr. Area 1: 143.4
 Noise: 0.4

Peak table for sample 2 : MN2 #3-4 Combo (2/12/2026)


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	174	183.58	1,602.5	
3	232	0.06	0.4	excluded peak
4	1,998	3.25	2.5	
5	2,583	5.01	2.9	
6	3,445	16.68	7.3	
7	5,491	57.02	15.7	
8	7,535	4.12	0.8	
9	8,641	3.55	0.6	
10	10,380	75.00	10.9	Upper Marker
11	13,594	0.00	0.0	

Region table for sample 2 : MN2 #3-4 Combo (2/12/2026)

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	143.4	24	468	47.2	152.34	682.6	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13804685_2026-03-29_16-04-48.xad

Created: 3/29/2026 4:04:48 PM
 Modified: 3/29/2026 5:12:37 PM

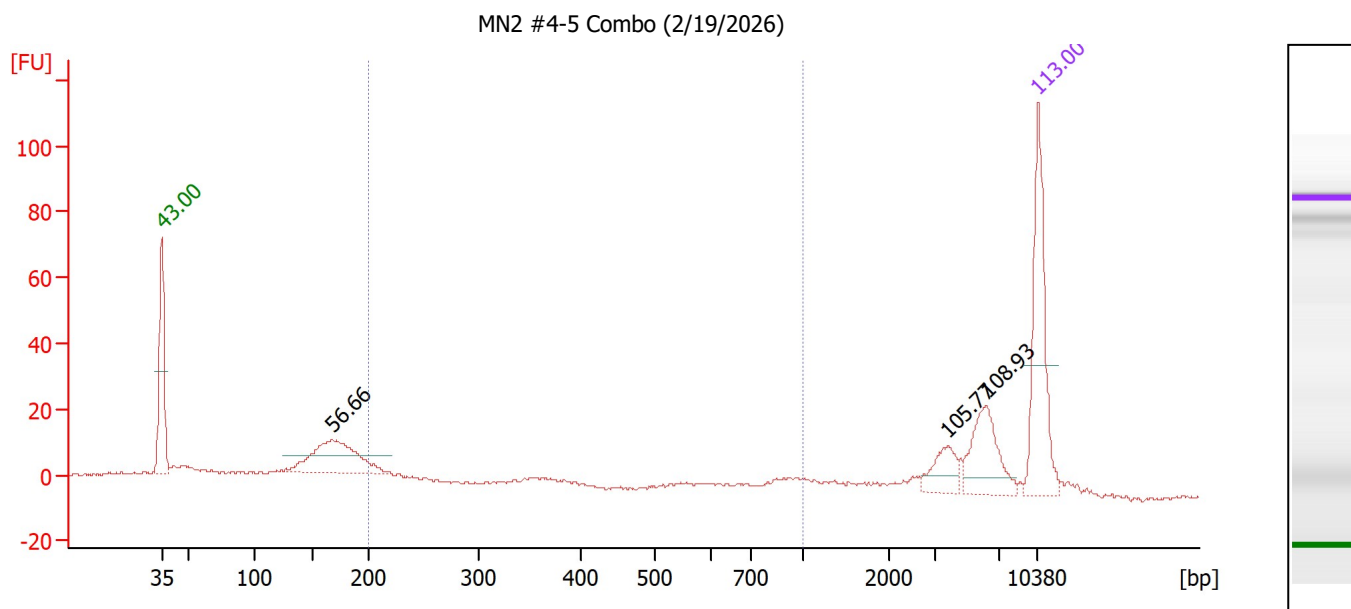Electropherogram Summary Continued ...**Overall Results for sample 3 : MN2 #4-5 Combo (2/19/2026)**

Number of peaks found: 3 Corr. Area 1: 99.8
 Noise: 0.5

Peak table for sample 3 : MN2 #4-5 Combo (2/19/2026)

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	168	95.63	862.4	
3	3,819	20.49	8.1	
4	6,274	43.75	10.6	
5	10,380	75.00	10.9	Upper Marker

Region table for sample 3 : MN2 #4-5 Combo (2/19/2026)


From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	99.8	22	487	49.3	100.95	447.1	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13804685_2026-03-29_16-04-48.xad

Created: 3/29/2026 4:04:48 PM
 Modified: 3/29/2026 5:12:37 PM

Electropherogram Summary Continued ...

MN2 #3-4 Combo (2/19/2026)

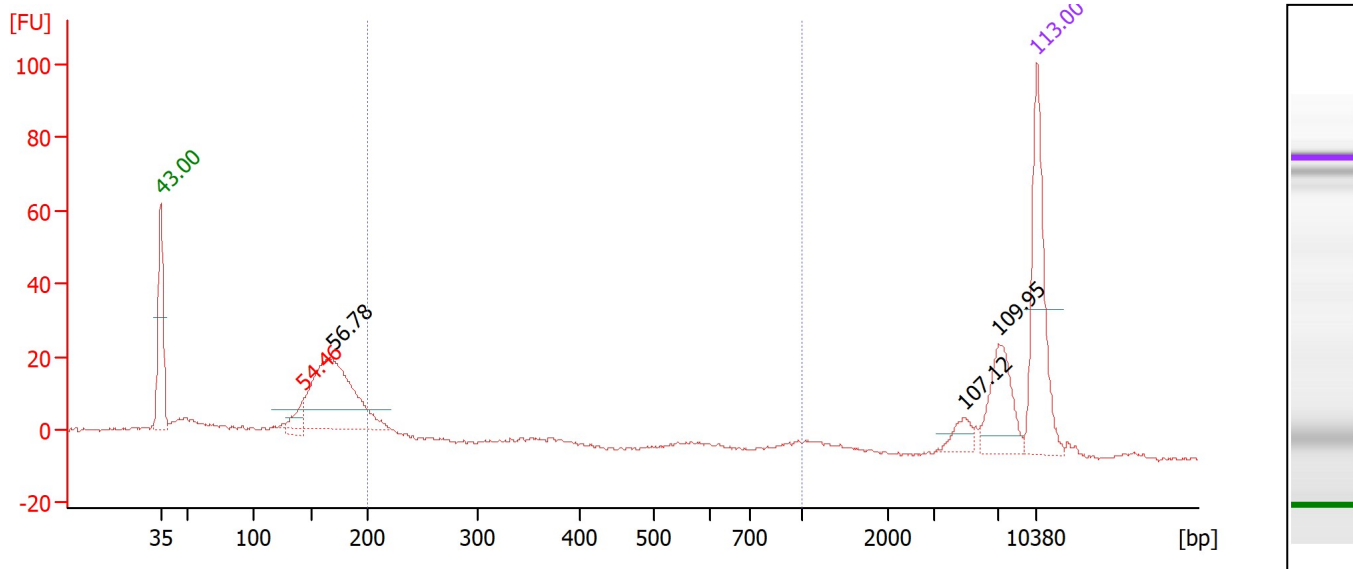**Overall Results for sample 4 : MN2 #3-4 Combo (2/19/2026)**

Number of peaks found: 3 Corr. Area 1: 45.2
 Noise: 0.4

Peak table for sample 4 : MN2 #3-4 Combo (2/19/2026)

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	169	176.57	1,579.2	
3	144	21.95	231.6	excluded peak
4	4,863	10.90	3.4	
5	7,093	41.87	8.9	
6	10,380	75.00	10.9	Upper Marker

Region table for sample 4 : MN2 #3-4 Combo (2/19/2026)


From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	45.2	12	409	60.1	49.59	270.5	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13804685_2026-03-29_16-04-48.xad

Created: 3/29/2026 4:04:48 PM
 Modified: 3/29/2026 5:12:37 PM

Electropherogram Summary Continued ...

MN2 #3-3 Veh (2/12/2026)

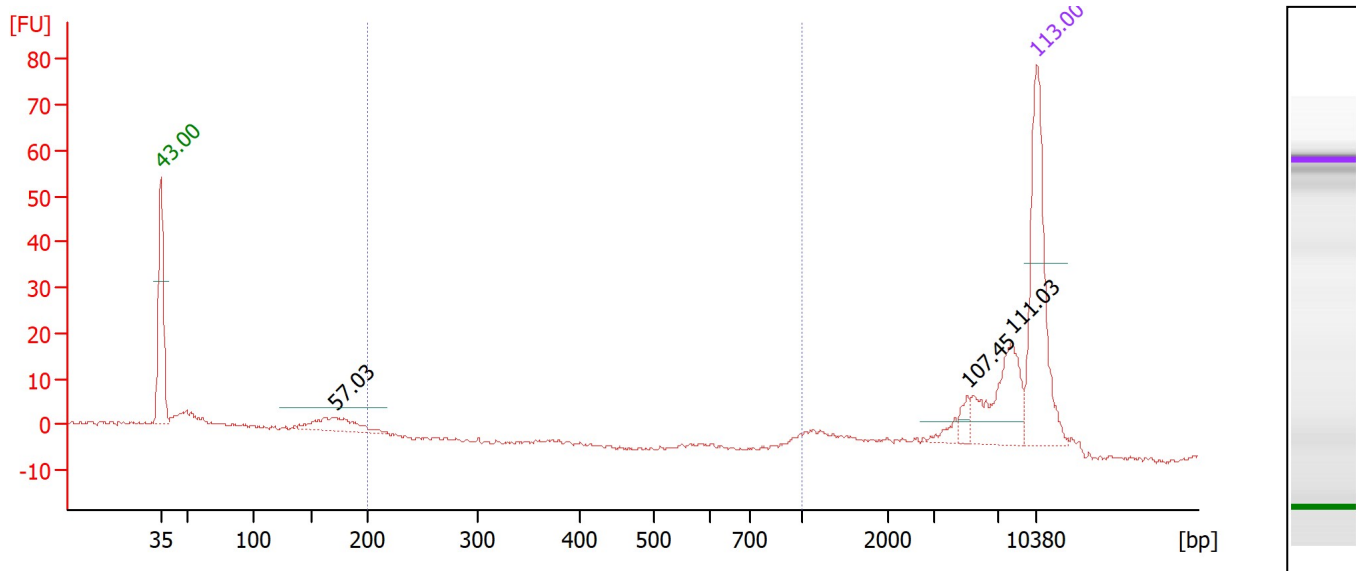**Overall Results for sample 5 : MN2 #3-3 Veh (2/12/2026)**

Number of peaks found: 3 Corr. Area 1: 8.4
 Noise: 0.4

Peak table for sample 5 : MN2 #3-3 Veh (2/12/2026)

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	172	30.23	266.0	
3	8,249	53.87	9.9	
4	5,124	6.86	2.0	Upper Marker
5	10,380	75.00	10.9	

Region table for sample 5 : MN2 #3-3 Veh (2/12/2026)


From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	8.4	4	642	52.7	9.63	44.9	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13804685_2026-03-29_16-04-48.xad

Created: 3/29/2026 4:04:48 PM
 Modified: 3/29/2026 5:12:37 PM

Electropherogram Summary Continued ...

MN2 #3-2 Veh (2/12/2026)

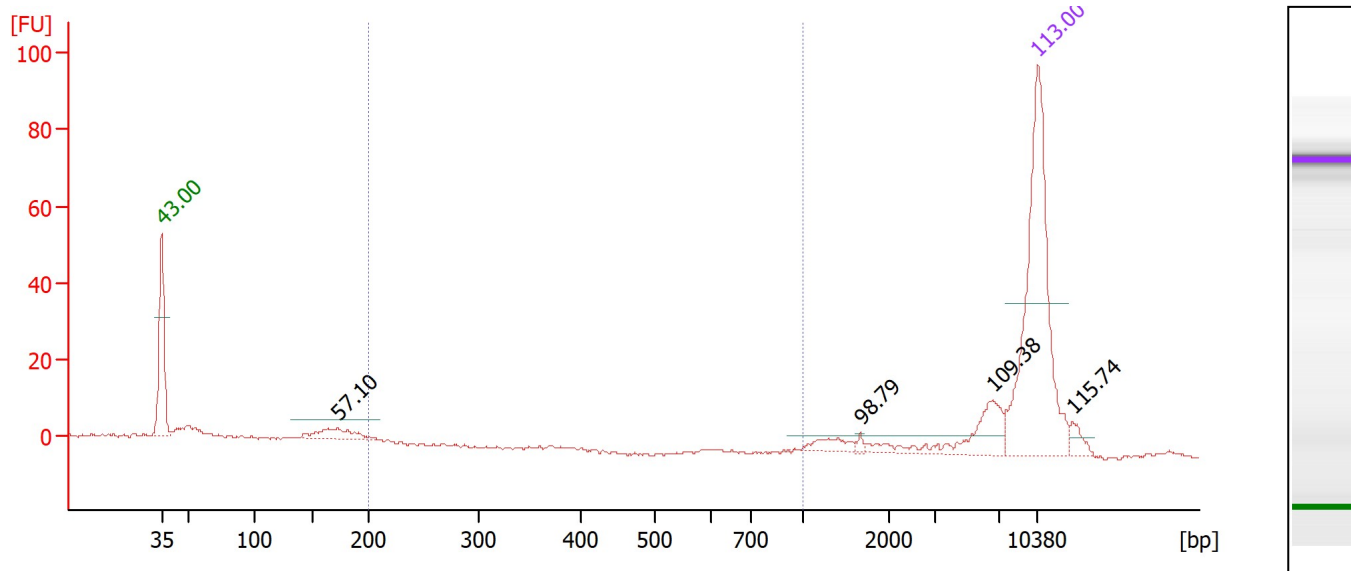**Overall Results for sample 6 : MN2 #3-2 Veh (2/12/2026)**

Number of peaks found: 4 Corr. Area 1: 6.2
 Noise: 0.4

Peak table for sample 6 : MN2 #3-2 Veh (2/12/2026)


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	173	14.61	128.0	
3	6,620	25.30	5.8	
4	1,670	1.37	1.2	
5	10,380	75.00	10.9	Upper Marker
6	13,341	0.00	0.0	

Region table for sample 6 : MN2 #3-2 Veh (2/12/2026)

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	6.2	4	461	68.1	4.30	24.6	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13804685_2026-03-29_16-04-48.xad

Created: 3/29/2026 4:04:48 PM
 Modified: 3/29/2026 5:12:37 PM

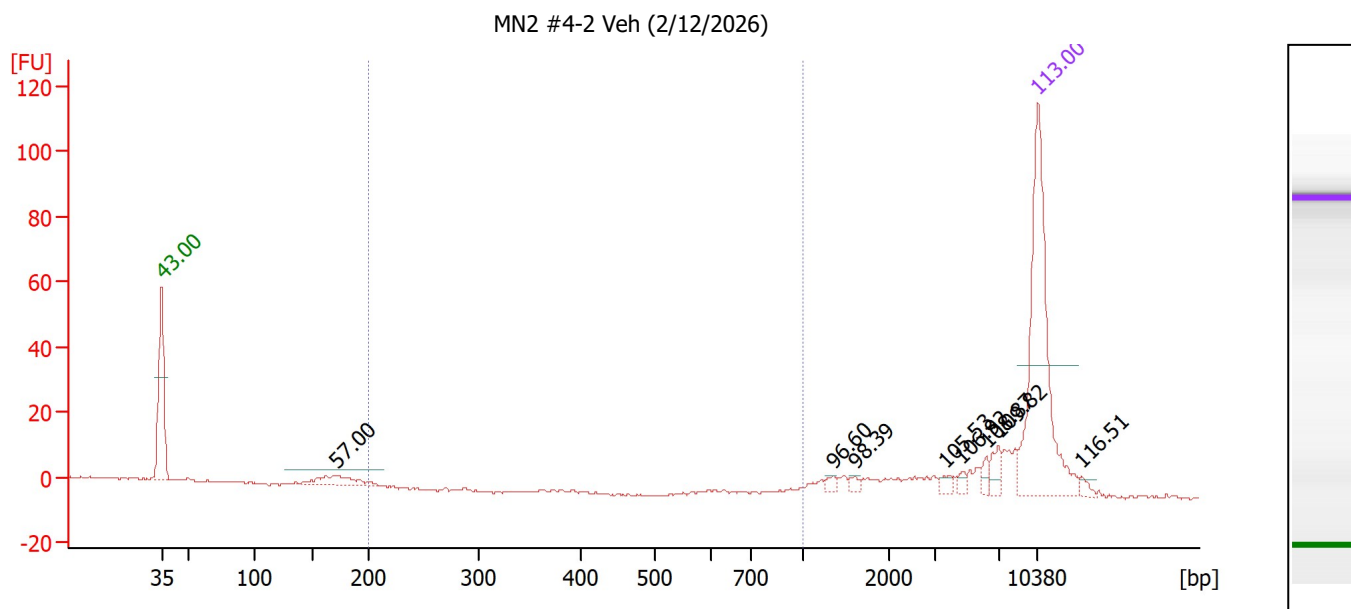Electropherogram Summary Continued ...**Overall Results for sample 7 : MN2 #4-2 Veh (2/12/2026)**

Number of peaks found: 8 Corr. Area 1: 3.0
 Noise: 0.4

Peak table for sample 7 : MN2 #4-2 Veh (2/12/2026)


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	172	15.87	140.0	
3	1,349	2.42	2.7	Upper Marker
4	1,610	1.93	1.8	
5	3,630	2.90	1.2	
6	4,712	2.27	0.7	
7	6,227	3.36	0.8	
8	6,963	5.93	1.3	
9	10,380	75.00	10.9	
10	14,173	0.00	0.0	

Region table for sample 7 : MN2 #4-2 Veh (2/12/2026)

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	3.0	2	813	28.2	1.84	5.2	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13804685_2026-03-29_16-04-48.xad

Created: 3/29/2026 4:04:48 PM
 Modified: 3/29/2026 5:12:37 PM

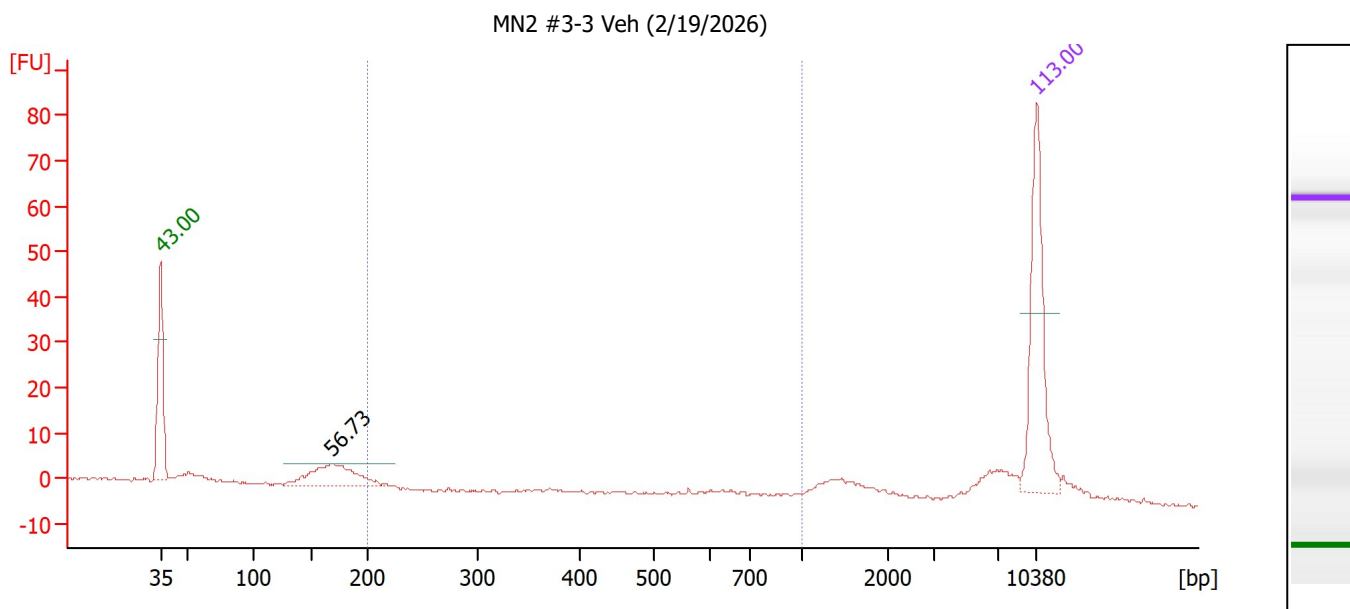Electropherogram Summary Continued ...**Overall Results for sample 8 : MN2 #3-3 Veh (2/19/2026)**

Number of peaks found: 1 Corr. Area 1: 2.3
 Noise: 0.4

Peak table for sample 8 : MN2 #3-3 Veh (2/19/2026)

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	169	56.75	509.5	
3	10,380	75.00	10.9	Upper Marker


Region table for sample 8 : MN2 #3-3 Veh (2/19/2026)

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	2.3	2	313	59.0	3.50	23.2	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13804685_2026-03-29_16-04-48.xad

Created: 3/29/2026 4:04:48 PM
 Modified: 3/29/2026 5:12:37 PM

Electropherogram Summary Continued ...

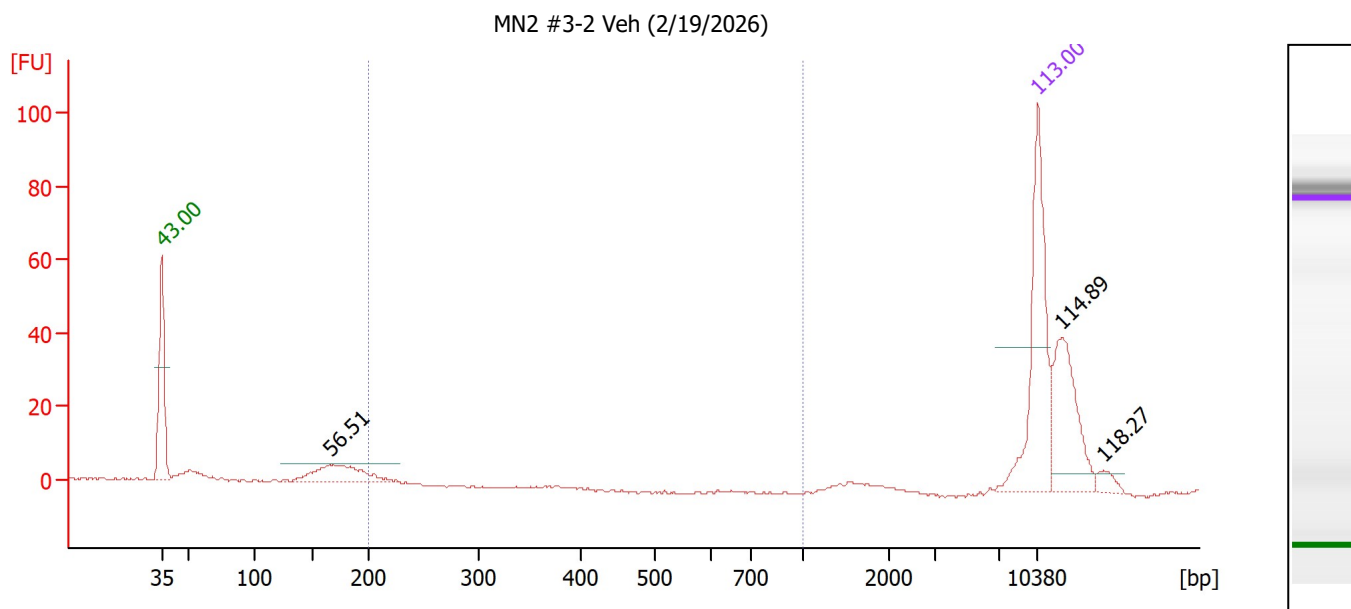

Overall Results for sample 9 : MN2 #3-2 Veh (2/19/2026)

Number of peaks found: 3 Corr. Area 1: 12.5
 Noise: 0.4

Peak table for sample 9 : MN2 #3-2 Veh (2/19/2026)


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	166	43.62	397.4	
3	10,380	75.00	10.9	Upper Marker
4	12,419	0.00	0.0	
5	16,064	0.00	0.0	

Region table for sample 9 : MN2 #3-2 Veh (2/19/2026)

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	12.5	6	272	40.5	13.33	84.2	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13804685_2026-03-29_16-04-48.xad

Created: 3/29/2026 4:04:48 PM
 Modified: 3/29/2026 5:12:37 PM

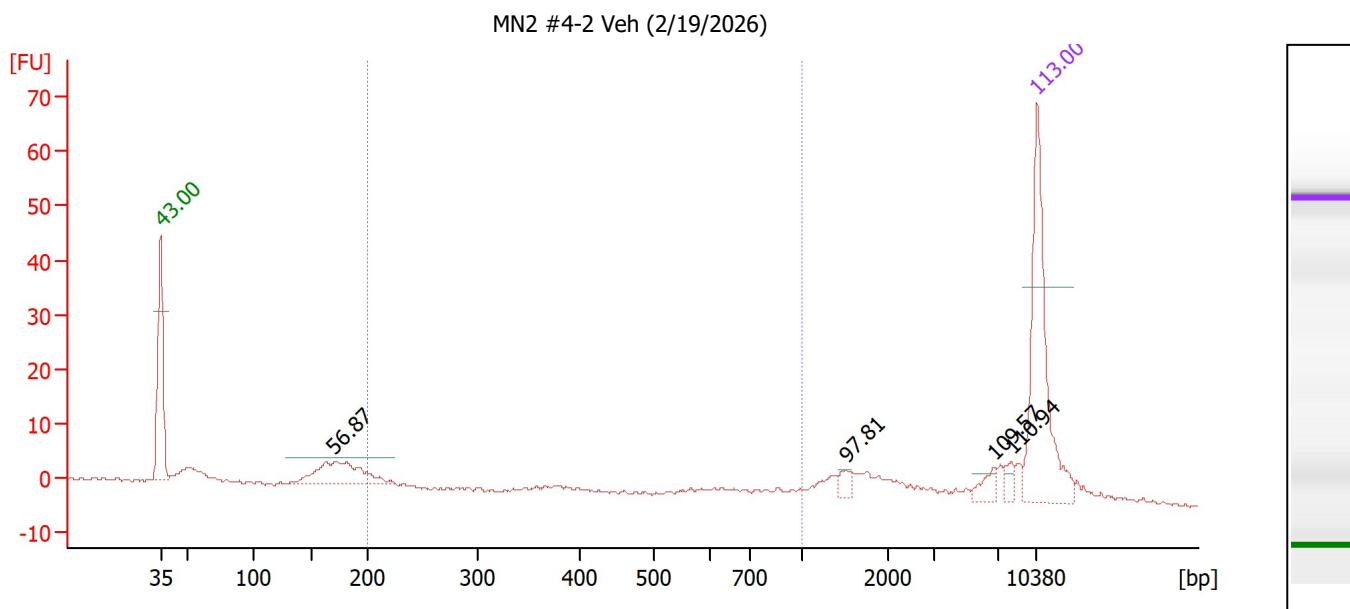Electropherogram Summary Continued ...**Overall Results for sample 10 : MN2 #4-2 Veh (2/19/2026)**

Number of peaks found: 4 Corr. Area 1: 7.8
 Noise: 0.3

Peak table for sample 10 : MN2 #4-2 Veh (2/19/2026)


Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	170	52.59	467.6	
3	1,526	5.45	5.4	
4	6,772	6.96	1.6	
5	8,161	4.70	0.9	Upper Marker
6	10,380	75.00	10.9	

Region table for sample 10 : MN2 #4-2 Veh (2/19/2026)

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	7.8	7	459	59.3	11.21	61.2	Blue

Assay Class: High Sensitivity DNA Assay
 Data Path: C:\...gh Sensitivity DNA Assay_DE13804685_2026-03-29_16-04-48.xad

Created: 3/29/2026 4:04:48 PM
 Modified: 3/29/2026 5:12:37 PM

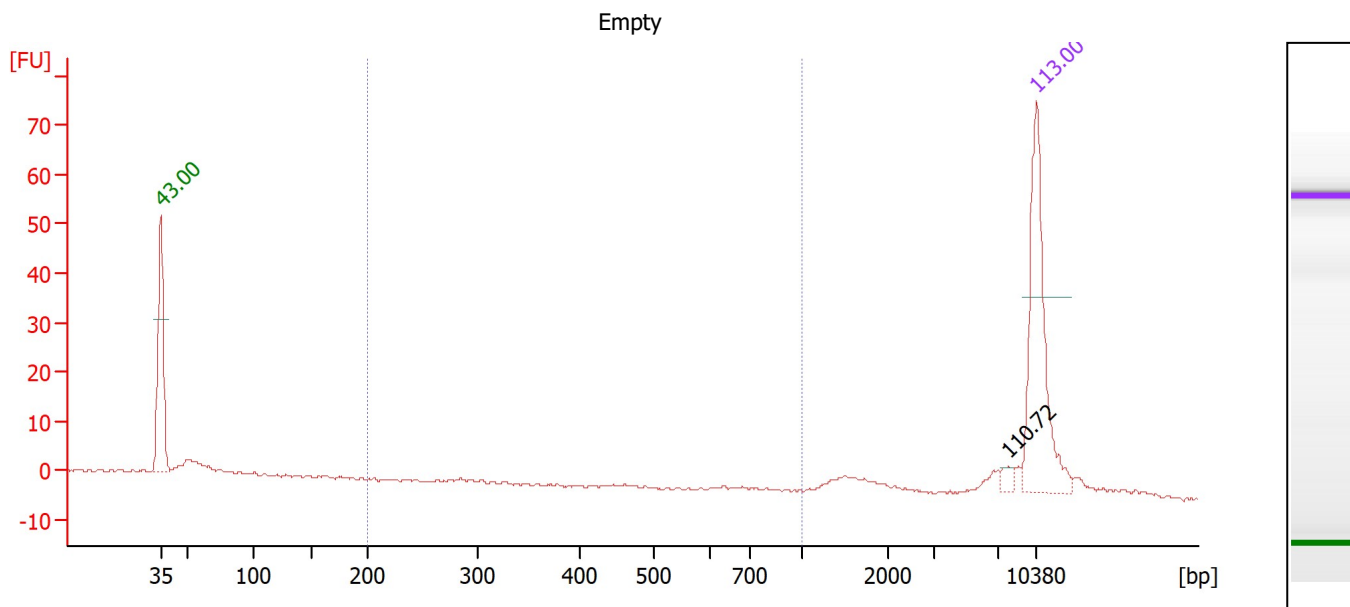Electropherogram Summary Continued ...**Overall Results for sample 11 : Empty**

Number of peaks found: 1 Corr. Area 1: 0.1
 Noise: 0.3

Peak table for sample 11 : Empty

Peak	Size [bp]	Conc. [pg/μl]	Molarity [pmol/l]	Observations
1	35	125.00	5,411.3	Lower Marker
2	7,923	3.83	0.7	
3	10,380	75.00	10.9	Upper Marker

Region table for sample 11 : Empty

From [bp]	To [bp]	Corr. Area	% of Total	Average Size [bp]	Size distribution in CV [%]	Conc. [pg/μl]	Molarity [pmol/l]	Color
200	1,000	0.1	0	284	0.3	0.08	0.4	Blue

Assay Class: High Sensitivity DNA Assay
Data Path: C:\...gh Sensitivity DNA Assay_DE13804685_2026-03-29_16-04-48.xad

Created: 3/29/2026 4:04:48 PM
Modified: 3/29/2026 5:12:37 PM

Gel Image