


LOO-SFE leakage sensitivity on matched 114 samples

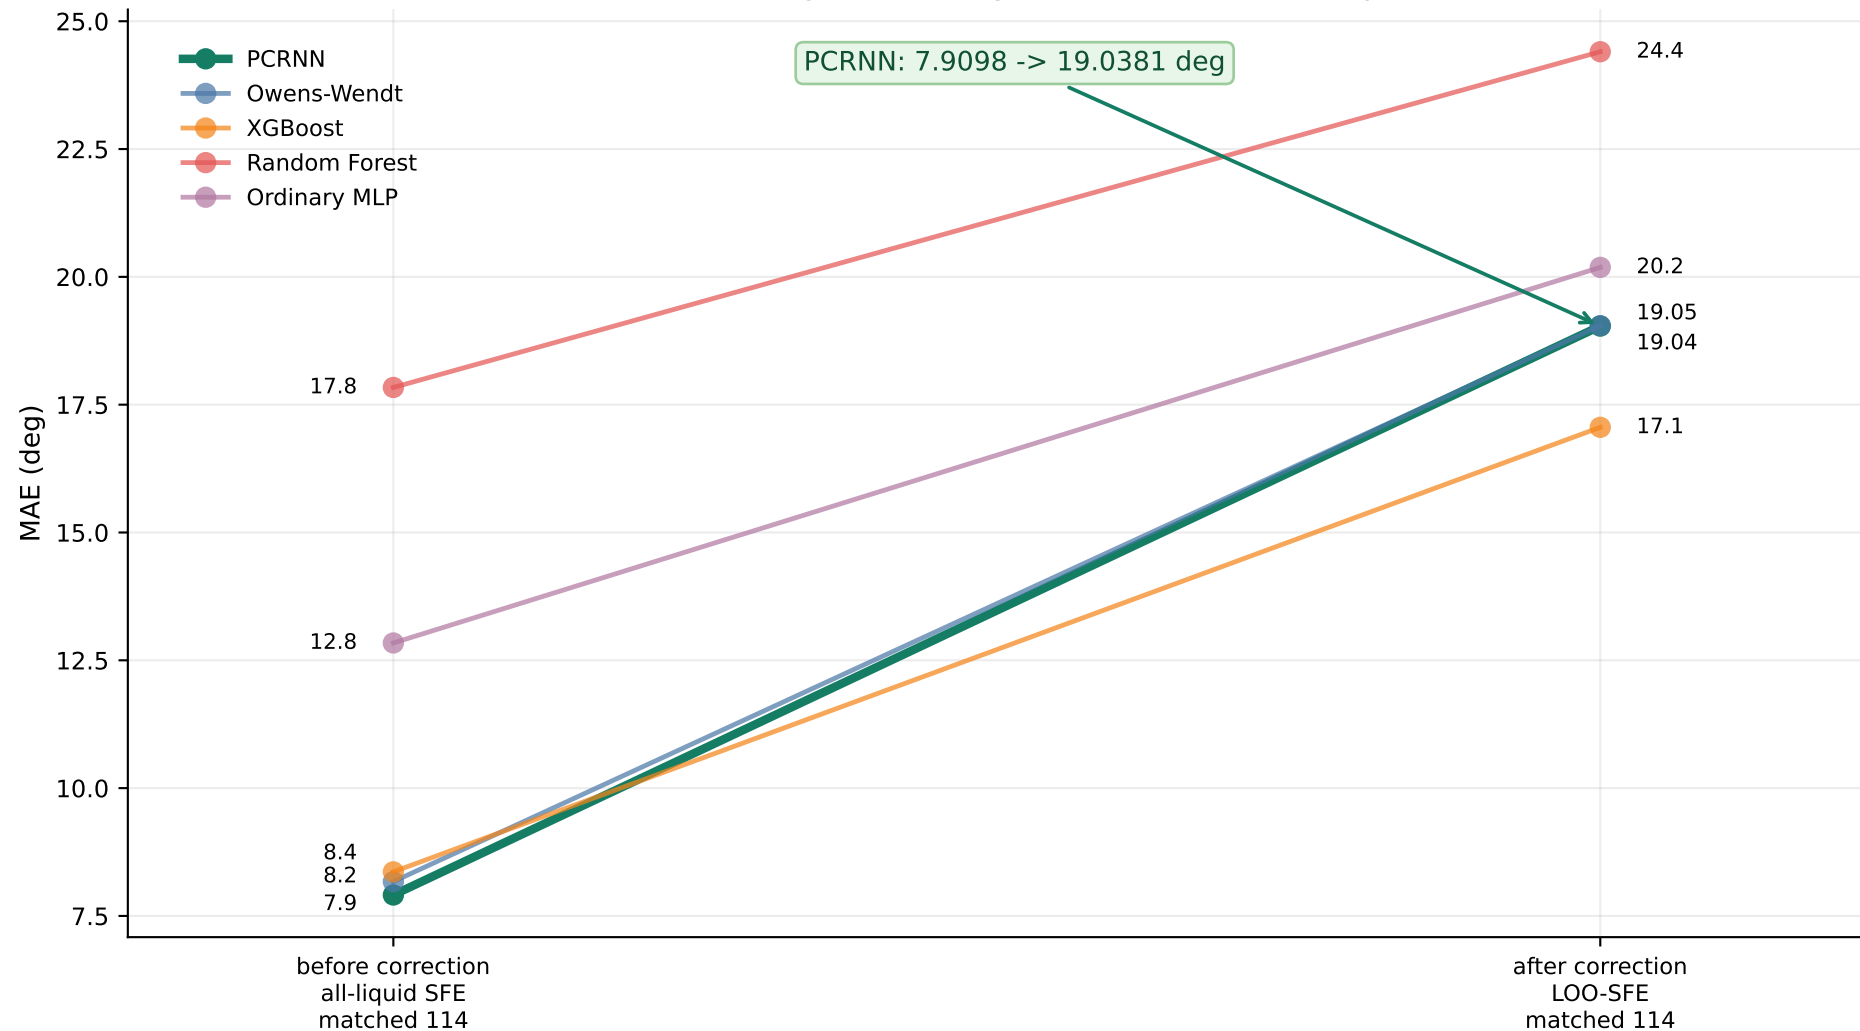

This sensitivity panel explains leakage risk; the after-correction LOO-SFE 114 cohort is the primary clean external result.