

Countess™ 3 Report

1/12/23 3:12pm

Summary

Sample name: exars_2022_21_1
Count ID: 1043



Results

Trypan Blue corrected

	Concentration	
Total		4.26 x 10 ⁶ /mL
Live	45%	1.90 x 10 ⁶ /mL
Dead	55%	2.35 x 10 ⁶ /mL

Settings

	Live	Dead	
Acquisition			
Intensity	36	36	
Focus	67	67	
Gating			
Protocol			
Size	0, 70	0, 70	
Brightness	0, 255	0, 255	
Circularity	0, 100	0, 100	

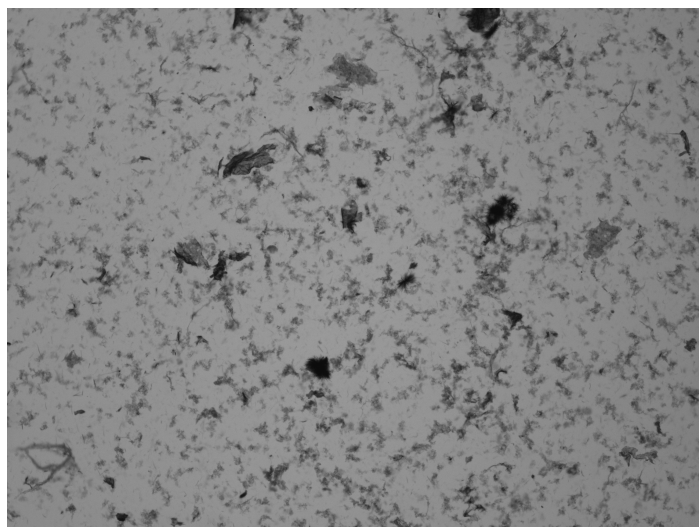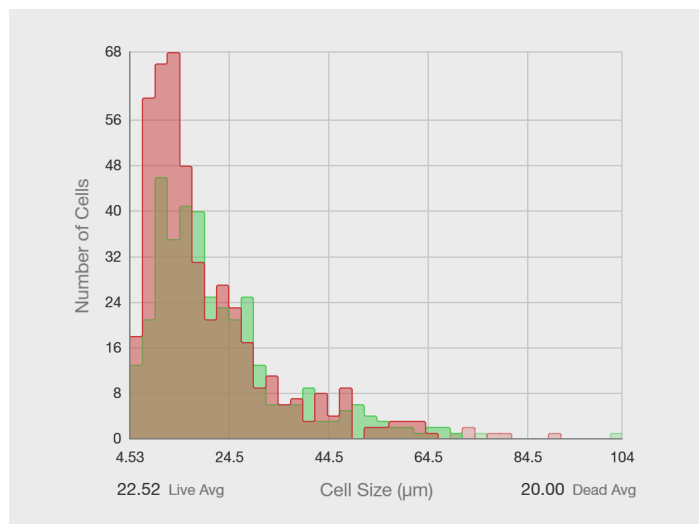

Countess™ 3 FL
Automated Cell Counter

invitrogen
by Thermo Fisher Scientific