



**Czech
Technical
University
in Prague**

F3

**Faculty of Electrical Engineering
Department of measurement**

Manual for STM32 diagnostic logic probe

Milan Jiříček

**Supervisor: doc. Ing. Jan Fischer, CSc.
Study programme: Open Informatics
Specialization:
2025**

Contents

1 Build	2
1.1 STM32G030 SOP8	2
1.2 STM32G030 TSSOP20	2
2 Local mode	3
2.0.1 Activation	3
2.1 Logic probe mode	3
2.2 Generating periodic pulses	4
2.3 Rise edge detection	4
2.4 Falling edge detection	4
3 Terminal mode	6
3.1 Universal keys	6
3.2 How to enable	6
3.3 PINOUT	7
3.4 MENU	7
3.5 Basic Mode	8
3.5.1 Voltmeter/Ohmmeter	8
3.5.2 Signal detect	9
3.5.3 Signal generator	11
3.6 Advanced Mode	11
3.6.1 SHIFT Register	11
3.6.2 NEOPIXEL	12
3.6.3 UART	13
3.6.4 I2C	14
3.6.5 SPI	15

Section 1

Build

1.1 STM32G030 SOP8

TODO: doplnit podrobnosti

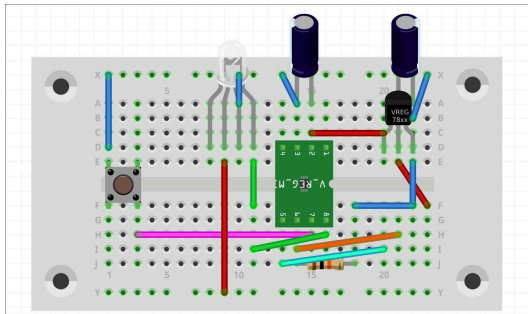


Figure 1: Diagram SOP8 ve Fritzingu

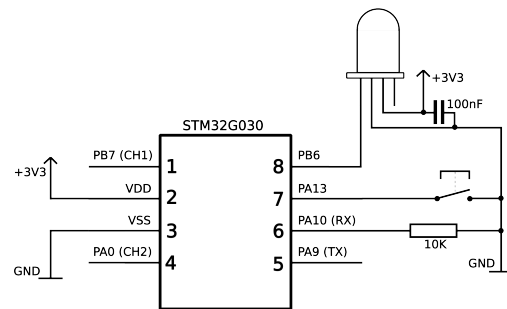


Figure 2: Diagram SOP8

1.2 STM32G030 TSSOP20

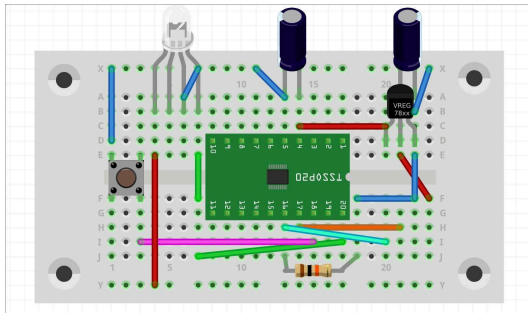


Figure 3: Diagram TSSOP20 ve Fritzingu

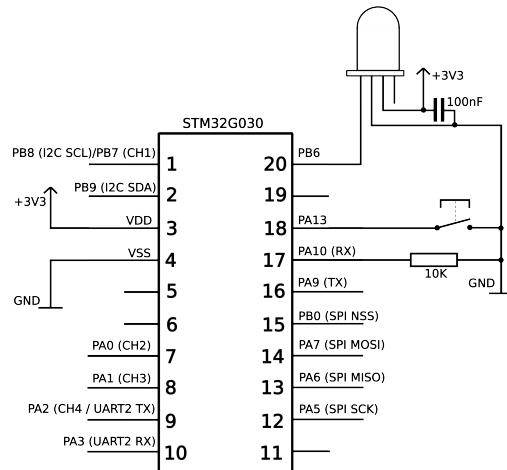


Figure 4: Diagram TSSOP20

Section 2

Local mode

This mode enables quick circuit diagnostics without requiring a computer connection. It offers the following features:

- **Logic Probe:** Instant visualization of signal states (HIGH/LOW) on connected channels.
- **Edge Detection:** Recognition of both rising edge and falling edge signal transitions.
- **Pulse Generation:** Continuous pulsing
- **Manual Logic Level Control:** Set fixed HIGH/LOW levels on selected channels.

To switch between modes, hold the button for approximately 500 ms. The RGB LEDs indicate the active mode by displaying its assigned color when the button is released.

2.0.1 Activation

Local mode is enabled when the device is powered without UART computer connection. To activate it:

1. Connect only the power supply to the assembled circuit (no data/USB connection).
2. Upon startup, the device detects a logic LOW (0) on the receive (RX) pin, which is reserved for computer communication.
 - *Note:* When connected to a computer, the RX pin defaults to logic HIGH (1), disabling Local mode.
3. A startup RGB LED color sequence (e.g., alternating green-blue-red) will play to visually confirm Local mode is active.

2.1 Logic probe mode

This mode is designed for diagnosing logic circuits. It enables real-time monitoring of logic states (HIGH/LOW) across two independent channels via color-coded LED indicators. The channels are assigned to pins PB7 (Channel 1) and PA0 (Channel 2). Ideal for quick signal verification.

LED Behavior:

- Mode indicator: AQUA

Channel Selection:

- Toggle Channel 1 and Channel 2 by *pressing* the button.
- Selected channel is confirmed by the LED color:
 - Channel 1: PURPLE
 - Channel 2: YELLOW

State Detection:

- HIGH (Logic 1): GREEN
- LOW (Logic 0): RED
- Floating/Intermediate State: LED turns OFF

PIN Assignments:

- **Channel 1:** PB7
 - *SOP8* package: Pin 1
 - *TSSOP20* package: Pin 1
- **Channel 2:** PA0
 - *SOP8* package: Pin 4
 - *TSSOP20* package: Pin 7

■ 2.2 Generating periodic pulses

This mode produces periodic pulses with button-controlled activation. Output state visualized through persistent LED feedback.

LED Behavior:

- Mode indicator: WHITE
- Active state: Maintains WHITE continuously

Operation:

- Press button to toggle between:
 - ON: Signal generation active
 - OFF: Output disabled

PIN Assignment:

- Signal output: PA0
 - *SOP8* package: Pin 4
 - *TSSOP20* package: Pin 7

■ 2.3 Rise edge detection

This mode detects raising edge on input pin. Time-limited visual confirmation provided upon detection.

LED Behavior:

- Mode indicator: BLUE
- Detection confirmation: GREEN (1 second)

Operation:

- Continuous monitoring of PA0 pin for raise edge
- When pulse detected, GREEN LED color is on for 1 second

PIN Assignment:

- Signal input: PA0
 - *SOP8* package: Pin 4
 - *TSSOP20* package: Pin 7

■ 2.4 Falling edge detection

This mode detects falling edge on input pin. Time-limited visual confirmation provided upon detection.

LED Behavior:

- Mode indicator: PURPLE
- Detection confirmation: GREEN (1 second)

Operation:

- Continuous monitoring of PA0 pin for raise edge
- When pulse detected, GREEN LED color is on for 1 second

PIN Assignment:

- Signal input: PA0
 - SOP8 package: Pin 4
 - TSSOP20 package: Pin 7

Section 3

Terminal mode

This mode is used for deeper identification of the problem.

3.1 Universal keys

- [R] - reload page to fix broken ansi sequences
- [Q] - return to menu

3.2 How to enable

Terminal mode is enabled by connecting device through converter. After connecting device to USB, open terminal which supports ANSI sequences. Recommended application is **PUTTY**.

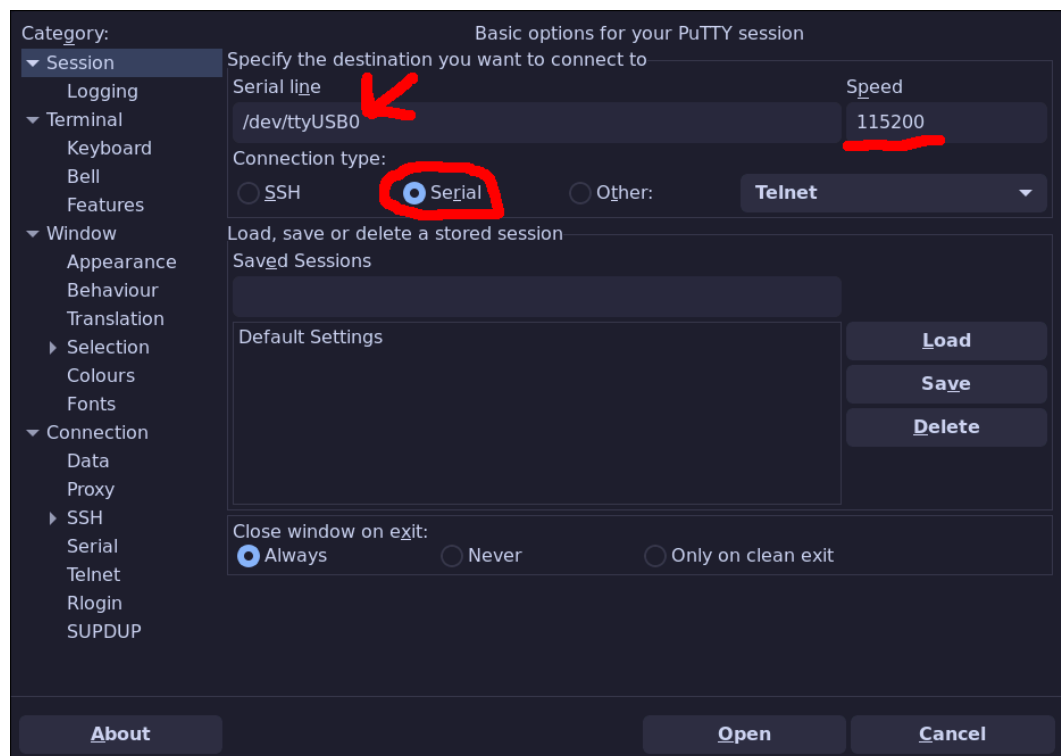


Figure 5: Putty settings

Select Serial as connection type. Enter **115200** as Speed of the serial communication and enter correct type of serial line. Usually on linux `/dev/ttyUSB0`.

After connection, press letter R on keyboard and menu appear.

3.3 PINOUT

Colors of wires show location of connect devices. If some text is colored, like **PA0**, that is pin 4(SOP8)/pin 7(TSSOP20).

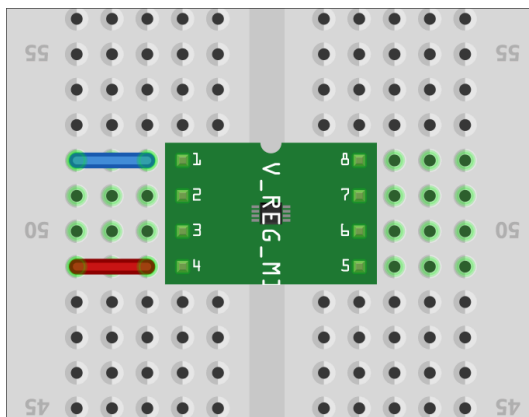


Figure 6: Voltage channels SOP8

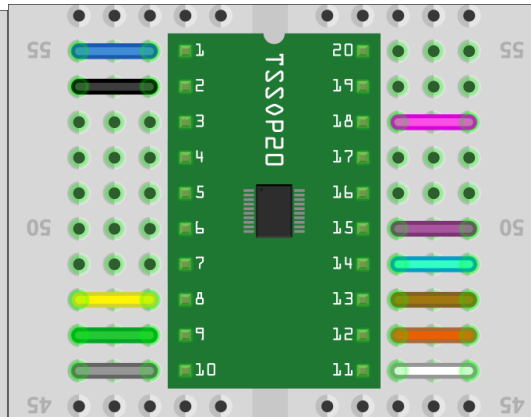


Figure 7: Voltage channels TSSOP20

3.4 MENU

The menu is divided into basic functions and advanced functions. In the **SOP8** version only the basic function is available. By pressing letter on keyboard written next to name, function can be selected.

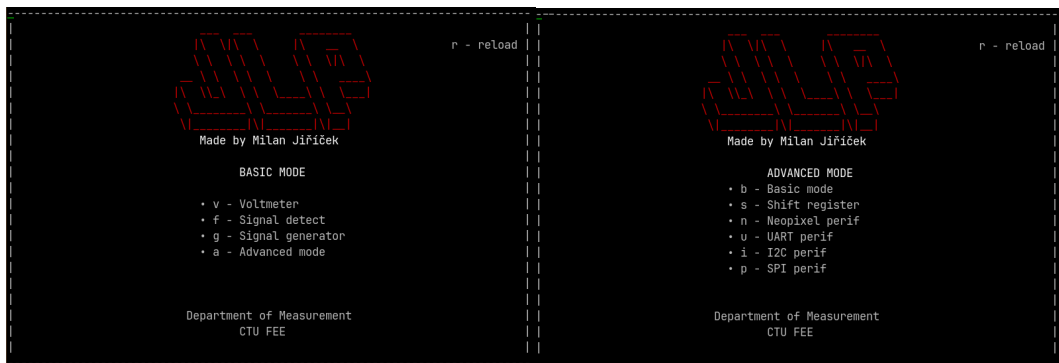


Figure 8: Basic menu



Figure 9: Advanced menu

■ 3.5 Basic Mode

3.5.1 Voltmeter/Ohmmeter

Voltmeter

Voltmeter shows different channels. Versions differs in the number of channels. Page shows **Reference voltage**, which is used for calibrating channel voltage.

- In parantheses is shown which pin is used as channel.
- **[1-4]** - Toggle channel on or off
- **[S]** - Apply settings of toggling channels
- **[M]** - switch between Voltmeter and ohmmeter

Red arrow points to the logic level of voltage.

- If shows **H**, channel is in high level
- If shows **L**, channel is in low level
- If shows **?**, channel is in interstate

If channel has **x** instead of value, it is turned off. To turn off or turn on the channel, it is necessary to press key of the number.

Example: For turn off the channel 1 press **1** on the keyboard and then **S** for saving the value.

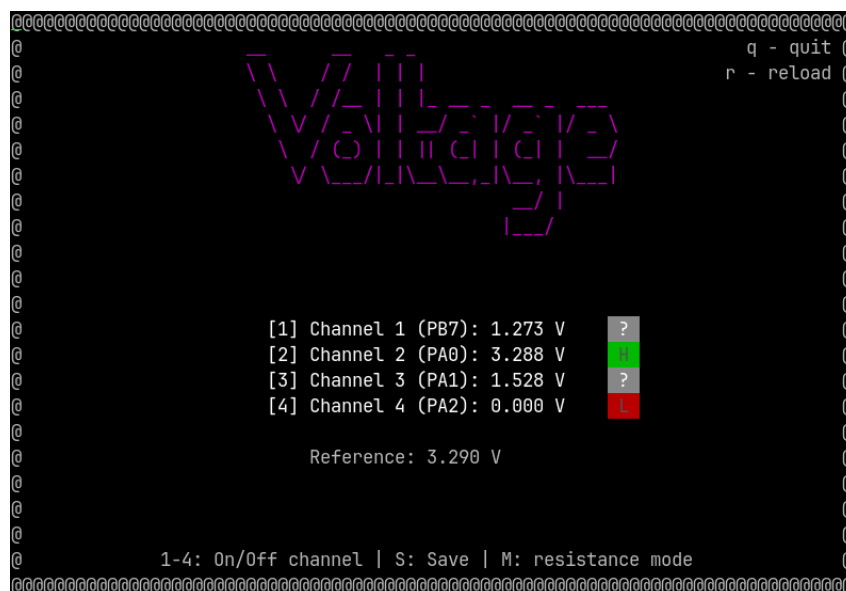


Figure 10: Voltmeter page

Figure 6 and Figure 7 shows, which pins are used for channels. SOP8 has **channel 1(PB7)** and **channel 2(PA0)**, but TSSOP20 has also **channel 3(PA1)** and **channel 4(PA2)**.



Pulse

Pressing **M** will change mode to pulse up or down mode. Pulse up will catch rising edge and pulse down will catch falling edge. If edge is catched, Flag will be changed to TRUE. To delete flag, press **D**. Pulse is catched on **PA0**.

- **[D]** - delete flag of caught signal
- **[M]** - change mode

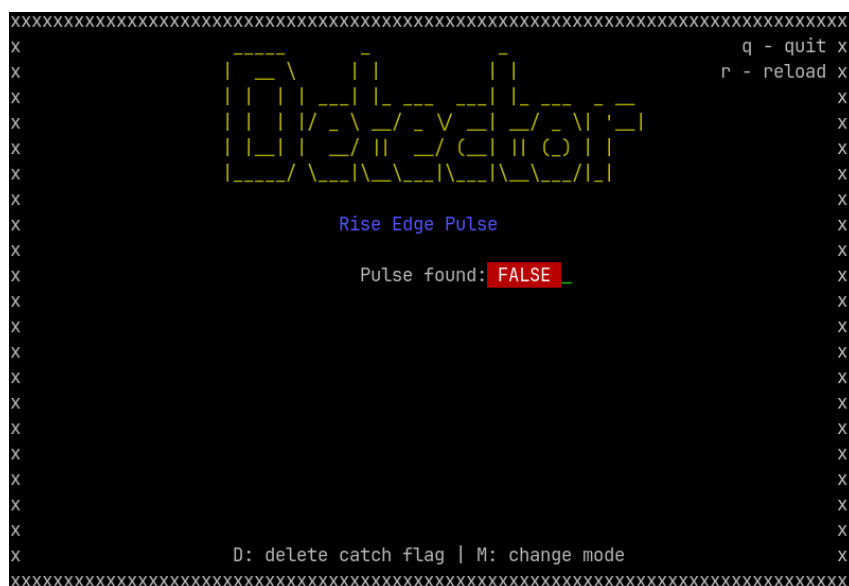


Figure 13: Pulse page

3.5.3 Signal generator

- **[E]** - edit pulse width or end edit mode
- **[Y]** - edit repeat count or end edit mode
- **[T]** - toggle mode from pulse up to pulse down
- **[S]** - send signal
- **[1-9]** - change pulse width
- **[X]** - delete pulse width number

On **PA0** pin can be send signal with specific pulse width. Width can be edited by **E**. There are two modes. When pulse up is choosed, default pin setup is **LOW LEVEL**. When signal is sent **HIGH LEVEL** is set for specified time. When pulse down is choosed, default pin setup is **HIGH LEVEL** and when signal is sent **LOW LEVEL** is set for specific time. By changing repeat counter, user can generate signal x times.



Figure 14: Generate signal page

■ 3.6 Advanced Mode

This function is only on **TSSOP20**!

3.6.1 SHIFT Register

Pin **PA0** is used for send data and pin **PB7** is used as clock signal. In case of **74HC595** pin **PA1** is used as Output enable.

User can change sequence for shift register which will be sent.

- [1-8] - Toggle 1 or 0 on specified position
- [S] - send sequence

```

*****
*                                     q - quit *
*                                     r - reload *
*
*          SHIFT REGISTER
*        PB7/1-CLOCK | PA0/7-DATA | PA1/8-RCLK
*
*      | 1 || 1 || 0 || 1 || 1 || 0 || 0 || 1 |
*
*
*
*
*
*
*
*
*
*
*
*
*
*
*
*
*
*
*
*
*1-8: Toggle bit | S: send | D: send one bit | F: reset counter | G: send RCLK*
*****

```

Figure 15: Neopixel page

■ 3.6.2 NEOPIXEL

Neopixel perif, can be read or wrote. Modes can be changed by pressing **M**. Neopixel is read on pin **PA0**. When signal is detected. Value is showed on the display. Data can be send to Neopixel by pin **PA13**.

On write, user can choose color from 0 to 255 for every color element. By pressing **S** selected signal will be sent.

- **[0-9]** - Change value
- **[X]** - Delete value
- **[M]** - Change mode
- **[K]** - Edit values
- **[L]** - Move cursor
- **[S]** - Send neopixel data


```

q - quit ;
r - reload ;

UART WRITE (PIN PA2)

WORDLEN: 8 | PARITY: N | STOPBITS: 1 | SEND BYTES: 1
BAUDRATE 115200

| 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 | 0 |

T: edit settings | K: edit vals | S: send | M: change mode_

```

Figure 17: UART page

3.6.4 I2C

I2C peripheral can be read and write. Modes can be changed by pressing **M**. **SCL** use PB8 and **SDA** use PB9.

First mode is address scan, where probe shows, which address on I2C is active. Second mode is slave mode, where probe is behaving as slave. User can set I2C address of the slave. Third mode is master mode, where probe is behaving as master. To selected adress, probe send entered data by user. Fourth mode is testing **SSD1306** display, where after pressing **S**, display set all pixels active.

- **[0-F]** - Change hex value
- **[X]** - Delete value
- **[M]** - Change mode
- **[K]** - Edit values
- **[L]** - Move cursor
- **[S]** - Send data
- **[T]** - Edit settings
- **[Y]** - Change bytes to send
- **[U]** - Switch read write



Figure 18: I2C Scan address page

Figure 19: I2C Slave page

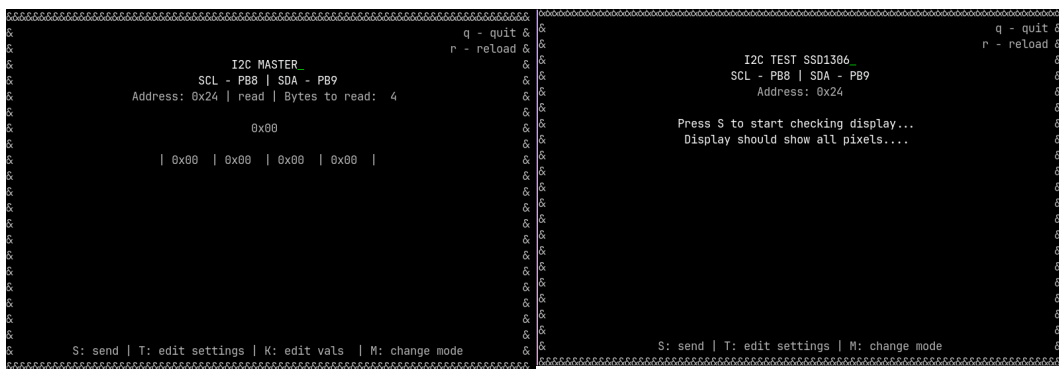


Figure 20: I2C Master page

Figure 21: I2C display testing page

3.6.5 SPI

SPI peripheral can be read and write. Modes can be changed by pressing **M**. **SCK** use PA5, **MISO** use PA6, **MOSI** use PA7 a **NSS** use PB0.

First mode is slave mode, where probe is behaving as slave. second mode is master mode, where probe is behaving as master. Fourth mode is testing **SSD1306** display, where after pressing **S**, display set all pixels active.

- **[0-F]** - Change hex value
- **[X]** - Delete value
- **[M]** - Change mode
- **[K]** - Edit values
- **[L]** - Move cursor
- **[S]** - Send data
- **[T]** - Edit settings
- **[Y]** - Switch Phase
- **[U]** - switch Polarity
- **[P]** - read/write
- **[I]** - Change bytes to send

Figure 23: SPI Display test page

Figure 24: SPI Master page