Anaerobic Workstation

Model No.: A-300



Make: BIOXIA

BiOxia

www.bioxia.co.in

Anaerobic A300

Construction: Durable, Non-Corrosive, Opaque Sheet of Acrylic Resin of 6mm or 8mm thickness for entire body, except front panel of acrylic resin but transparent sheet, for better visibility and insulation

Material used are durable & non corrosive & all joints are smooth finished.

Size: External: 670 X 800 X 705 mm – Length x Height x Depth

Main Workstation Capacity:

a) Up to 350 plates of 90mm X 15mm



Safety Features:

Excess pressure relief valve

Temperature overshoot controller.

Condensate controller technology should be inbuilt in the workstation.

Pressure relief valve for releasing excess pressure inside chamber, shall be provided.

Heating element along with controller shall be provided to maintain the temperature inside chamber within ambient to 45 °C, with Temperature Uniformity ± 1° C at 37°C.

LCD Display with touch screen Controlled: continuously show

Chamber pressure


Humidity

Temperature

Fluorescent Light

LCD display should continuously indicate Positive pressure (0.15 KPA/0.0015 bar) of the main chamber.

LCD Display with Touch Screen Controller:

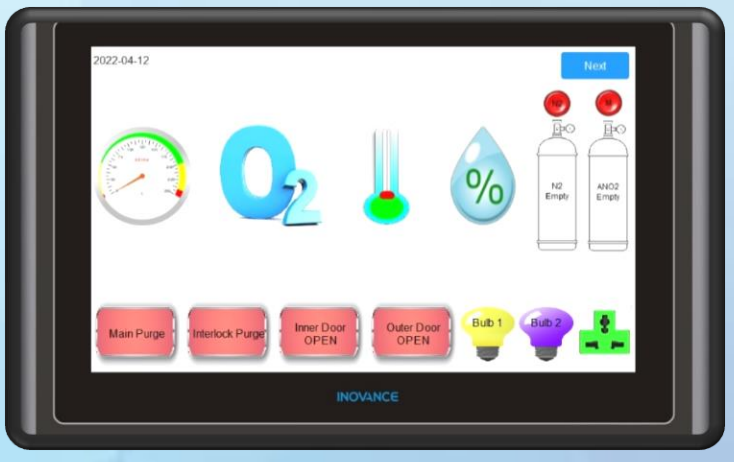

Touch Screen LCD Display

Fitted with one additional connection for attaching gas jar, so that jars can be attached, side by side simultaneously

Touch screen operating panel and in-built vacuum pump

Able to generate any mixed gas atmosphere (other than hazardous and inflammable) in transparent jars, by programming of required O2 (atmospheric), N2 and CO2 & H2 (from cylinders of mix gases & pure gases) percentage.

All controlled conditions like Capnophilic, anaerobic & Micro-aerophilic be created within 60 seconds, reproducible and stay within 0.5% of the desired value.

Minimum 30 programs to be customized as per user requirements

System to identity defective jars, catalysts and non-availability of gases, before incubation

Intake air filters facility to prevent air microbial contamination

It would be keeping its jar atmosphere with appropriate humidity to prevent drying and cross contaminations

It would be able to work with standard transparent anaerobic jars of any make

The equipment would be supplied with two sets of all necessary accessories including gas cylinders and pressure regulators (One set to be in-use and one set to be kept reserve) and catalyst to be provided

Provide both sets of required gas cylinders filled with gases at the time of installation

Four spare jars of twelve plates capacity with dedicated controller have been supplied along with machine

Accurate temperature control: ambient +5 – 45 deg C with automatic humidity control without dry spot

Power Supply :

- Power Input : 220 V-240V AC,50 Hz fitted with plug
- Resettable Over current breaker fitted for protection

ISO 9001 : 2015 Certified

CE Marked : CE marked product

GMP Certified

NSIC Certified Company


EN 12469:2000

ISO 13485:2016


European Conformity CE Certificate

Applicable Standards : EN ISO 14971:2012, EN ISO 13485 : 2012, EN 980:2008, EN 1041 : 2008, EN 61010-1:2010, EN 61326-1:2013, EN 12469:2000


Touch Screen Display

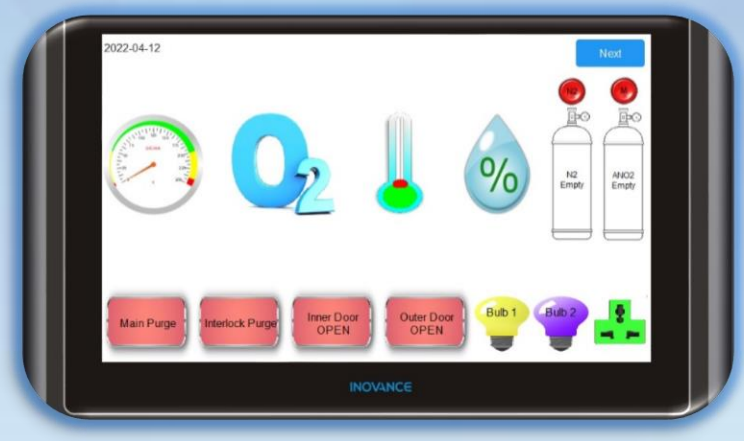

Catalyst & Detox Pouch

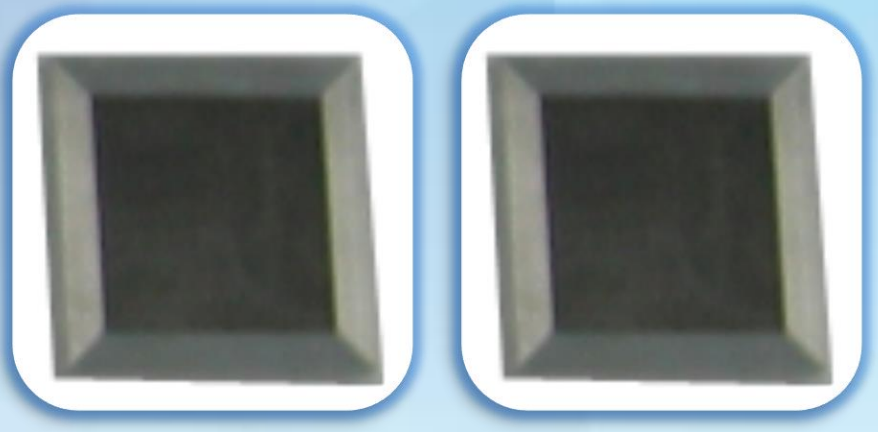

Calibration of Oxygen

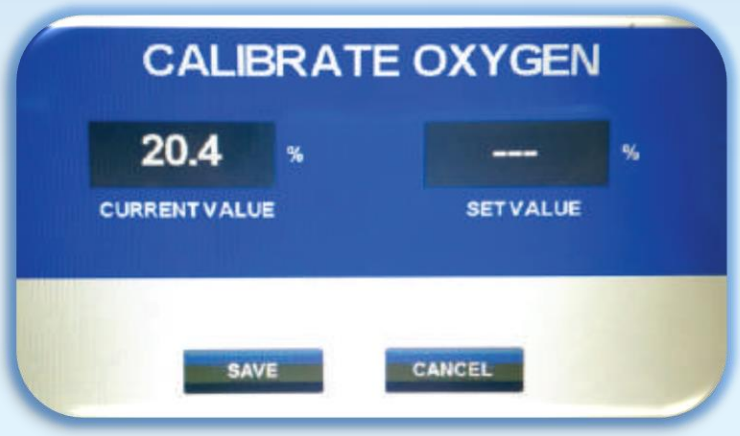



Condensing Cooling Plate



PRODUCT SUMMARY

PRODUCT SUMMARY OF WORKSTATION

MODEL	A300
Max Plate Capacity	350
Cabinet Mode of Construction	Solvent bonded Acrylic / Stainless Steel 304
Max Incubation Temperature	45° C
Gas Supply	Mixed Gas 5% H2 + 5% Co2 + 90% N2 & 100% N2 gas
Humidity control	√
Condensate Control	√
Positive Pressure Display	√
Safety Excess Pressure Relief Valve	√
Low Gas Alarm	√
Fluorescent Illumination	√
Palladium Catalyst	√
Activated Carbon Particles	√
Oxygen Sensor with Display	√
Internal Power Supply	√
LCD Display with control	√
Fan Unit	√
Anaerobic Indicator	√
Pair of Gloves	√
Petri Dish Holder	√

Work Address: H-7, Rajalaxmi Commercial Complex, Ground Floor, Kalher, Tal-Bhiwandi, Dist- Thane 421302
Email: bioxia.in@gmail.com | Website: www.bioxia.co.in