
HYPOXIA WORKSTATION

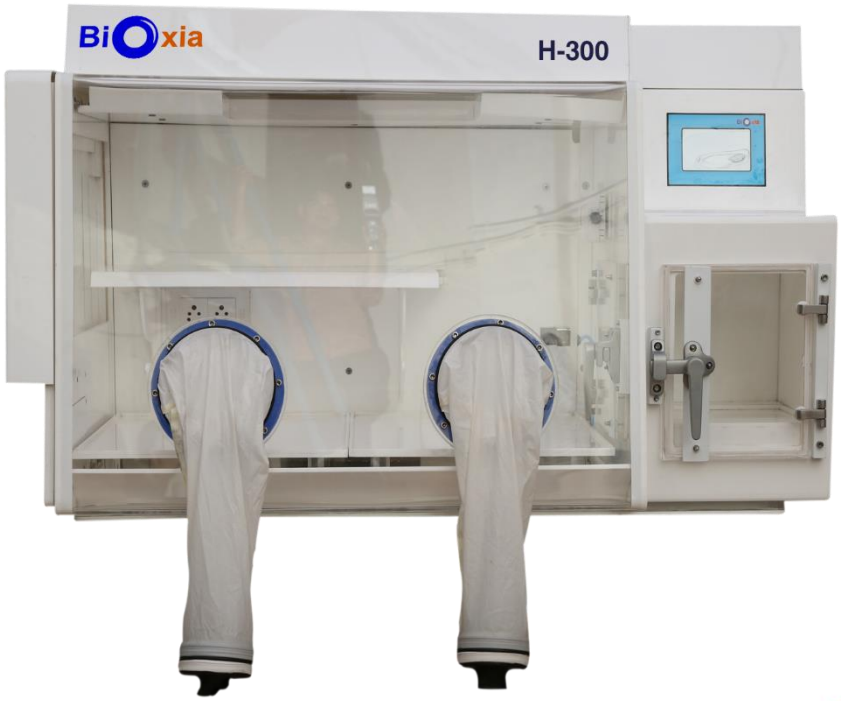

Model: H300

BiOxia

www.bioxia.co.in

Hypoxia Workstation H-300

Construction:

Durable, Non-Corrosive, Opaque sheet of Acrylic Resin of 6 mm or 8 mm thickness for entire body, except front panel of acrylic resin but transparent sheet, for better visibility and insulation.

The equipment comprises of a gas (air) controlling unit and a chamber to keep the tissue culture flasks/ 6 well plates/ Petri plates.

The workstation itself work as an incubator (no extra outside incubator needed) Digitally Controlled with digital temperature indicator cum controller ambient +5 Deg. C to 50 Deg. C ± 1 Deg. C.

Dimensions : L X H X D (approx.)

External : 900 X 740 X 660
Main Chamber : 650 X 500 X 500
Inter lock : 250 X 300 X 300

Main Workstation Capacity:

a) Up to 350 Petri plates
b) Additional inoculation space for regular working
c) One supply port inside the chamber

Interlock Capacity :

a) Interlock transfer Up to 25 petri plates of 90mm X 15mm
b) Auto Inter lock cycle
c) Interlock Cycle Time: 25 S

Safety Features :

Excess pressure relief valve.

Temperature overshoot controller.

Condensate controller technology inbuilt in the workstation

To make the chamber-controlled oxygen, automatic forced purging system for Main Chamber, with adjustable purging period.

To achieve the chamber oxygen faster rate, additional facility to condition the workstation atmosphere using proper direction of internal air, should be provided.

Pressure relief valve for releasing excess pressure inside chamber, will be provided

All the connecting tubes between the cylinder and the chamber durable and of good quality that not crack or be difficult to negotiate curves/ bends. one single tube connecting the controller in the chamber.

LCD Display with touch screen Controlled:

Chamber pressure & Gas Cylinder Pressure

Temperature & Humidity

Oxygen & Co2

Fluorescent Light 1 & Light 2.

LCD display continuously indicate percentage of oxygen in the chamber

Internal Socket indication continuously present on the screen

Chamber accurately maintains and controls **temperature, humidity, oxygen & Carbon dioxide** concentration to be able to provide hypoxic conditions for cell culture.

The controller displays the temperature of the environment in which the cell culture chamber is present.

The controller provides variable hypoxic concentration cycles of variable duration within one set of protocol.

Said Touch Screen display continuously indicate & controls:

(I) Controls O2 from 0.1% to 20.9%in 0.1% increments and accuracy of 0.1% of the set concentration
(II) Controls CO2 from 0.1 % to 30.0%in 0.1% increments accuracy of + 0.1% of the set concentration.

LCD Display with touch screen Controlled :

1) LCD display continuously indicate Positive pressure (0.15 KPA/0.0015 bar) of the main chamber.
2) Audio & Visual alarm for low or excess oxygen & Carbon dioxide level.
3) Audio & Visual alarm for gas cylinder pressures, chamber pressure and temperature.

Said Touch screen simplifies the calibration process:

(I) Automatically calibrates O2 sensor through one touch screen control.

(II) Provides rapid equalization.

(III) Facilitates the download of data.

(IV) Provides Faculty Recognition

Said Touch Screen display allows Hypoxic cycling:

Facilitating up to 4 different O2

Concentrations through a user-defined sequence of time

Oxygen sensor shall be present out of main working chamber

Auto excess pressure control system

The front 10% slope viewing panel

Heater for dehumidification

Heating element along with controller shall be provided to maintain the temperature inside chamber within ambient to 50°C, with Temperature Uniformity ± 1° C at 37°C

Temperature ambient to 50 deg. C.

Inbuilt Trim-point for temperature calibration.

Additional, Utility port with “flexible hose” for manual purging by Nitrogen, inside the chamber

Proper valve for purging, both for main chamber & Interlock chamber.

Workstation will be operated by foot switch outside chamber

Foot switch outside chamber for Purging & Spot lamp operation.

Activated Detox to absorb smell.

Inspection Spot-lamp

Inlet options for Two separate cylinders: N2 & O2

The hypoxic environment of the cell culture chamber maintainable without compromising the hypoxia conditions.

Store dialogs for 6 months. One set of data stored per minute. Each data set comprising of time, date, oxygen and CO2 (set and actual).

Power Supply :

Power Input : 220 V-240V AC,50 Hz fitted with plug

Resettable Over current breaker fitted for protection

Certification:

NSIC Certified Company	ISO 9001: 2015 Certified	GMP Certified
CE Marked: CE marked product	EN 12469:2000	IS0 13485:2016
European CE conformity Compliance Certificate		

----------Calibration Oxygen----------






Touch Screen Display




Hypoxic Cycle

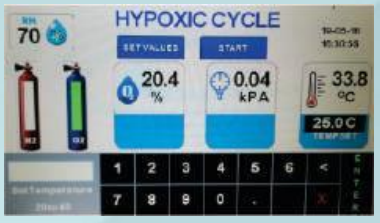

----------Data Logging Facility----------





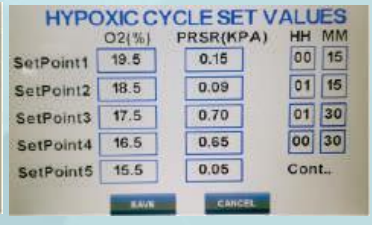

Co2 Controller




Flexible Hose



Interlock Transfer



Condensation Cooling Plate



Foot Switch



Hypoxia Workstation H-300

MODEL	H300
Max Plate Capacity	350
Interlock Plate capacity	25
Interlock Cycle Time	25s
Cabinet Mode of Construction	Solvent bonded Acrylic / Stainless Steel 304
Max Incubation Temperature	50° C
Gas Supply	Dual Gas (O2:100%, Co2: 100% & Nitrogen: 100%)
Humidity control	√
Condensate Control	√
Positive Pressure Display	√
Safety Excess Pressure Relief Valve	√
Low Gas Alarm	√
Inspection Spot Lamp	√
Fluorescent Illumination	√
Palladium Catalyst	√
Activated Carbon Particles	√
Oxygen Sensor with Display	√
Oxygen Controlled with Display 0.0% to 22%	√
Co2 Controlled with Display 0.0% to 30.0%	√
Ultra Violet (UV) Light	O
Bare Hand Facility	√
Foot Switch Operation	√
Removable Front	O
Internal Power Supply	√
Utility nozzle Connection	√
LCD Display with control	√
Fan Unit	√
Adjustable Shelf	O
Anaerobic Chamber	√
Cabinet Stand	O
Regulator for Cylinder	O
Gloves	√
Vacuum Line Port	√
Cable Gland Port	√
Petri Dish Holder	√

√ - Available O - Optional N/A - Not Available

BIOXIA- H-7, Rajalaxmi Commercial Complex, Ground Floor, Kalher, Tal- Bhiwandi, Dist- Thane 421302
Email: bioxia.in@gmail.com | Tel. No.: 8655003624