
Anaerobic Cum Microaerophilic Chamber

Model: M-800

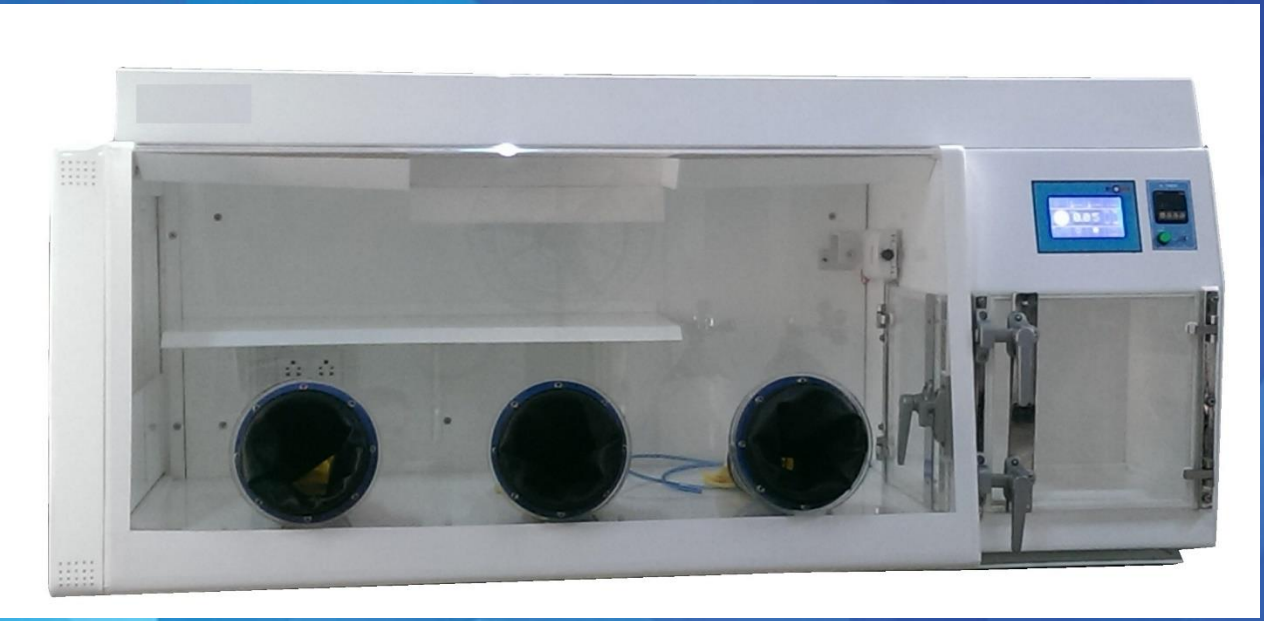

Make: BIOXIA

BiOxia

www.bioxia.co.in

Anaerobic Cum Microaerophilic Chamber M 800

Body Construction: Body Construction: Durable, Non-Corrosive, Opaque sheet of Acrylic Resin of 6mm or 8mm thickness for the entire body, except the front panel of acrylic resin but transparent sheet, for better visibility and insulation.

These workstations allow us to isolate cells in a chamber that accurately maintains and controls temperature, humidity, oxygen & Carbon dioxide. With this workstation we will studied the most complex cell interactions under perfect hypoxic or anoxic conditions.

Main Workstation Capacity:

Up to 950 plates of 90mm X 15mm

Inoculation working space: 40 % of Total volume in addition to above space

Single Chamber

Size: L X H X D (approx.)

External : 1500 X 740 X 800 mm

Internal : 900 X 600 X 600 mm

Interlock : 400 X 400 X 300 mm

Internal Working Space : 650 Litres or more

Separate Transfer Chamber: Air Lock/ Isolated/Interlock chamber, for inserting at least 66 plates at a time, with Proper leakproof door and handle

Interlock Cycle Time: 45 S

Transfer System: Separate Transfer Chamber



Incubation: Integrated

Inlet operation for four separate gases – Premixed anaerobic gas (H2: Co2: N2)10% : 10 % : 80 %), N2, Co2 and Air or Oxygen

To make the chamber oxygen-free, automatic forced purging system for the Main Chamber as well as interlock chamber, with adjustable purging period will be provided

Gloveless Technology

Airlock / Pass box System: Minimum Time to reach Anaerobic Conditions (Less than 2 mins)

All controlled conditions like Anaerobic Micro-aerophilic, Hypoxic, Capnophilic be created.

Oxygen Level: < 0.1 % (1,000 ppm) or less adjustable catalyst removal, real time monitoring

Gas Control: Automated Gas Mixing, Precise control of N2, H2, Co2

Oxygen Controlled with Display 0.0 % to 25 %

To achieve the chamber oxygen faster rate, additional facility to condition the workstation atmosphere using Palladium catalyst and adjust the internal air flow will be provided

Condensate controller technology inbuilt in the workstation.

Workstation controlled & continuously show positive pressure of the chamber.

Positive pressure (0.15 KPA / 0.0015 bar) of anaerobic environment, continuously maintained inside the incubation chamber.

Workstation controlled temperature, Fluorescent Light & blower.

Safety Features: Excess Pressure relief valve for releasing excess pressure inside chamber.

Temperature Overshoot controller for safety purpose.

Heating element along with controller provided to maintain the temperature inside chamber within 25°C to 48°C, with Temperature Uniformity ± 2° C at 37°C, ± 0.5 ° C accuracy.

Humidity Control: 50 % to 90 % relative humidity, stable environment with a built humidity system.

Temperature Control: Programmable 25° C to 48 ° C, ± 0.5 ° C accuracy

Digital LCD Display with Touch Screen Controller:



Touch Screen LCD Display

I. Touch Screen LCD Display for Monitoring as well as control: of Chamber pressure, Temperature, Humidity, gas cylinder pressure, Light 1 & Light 2

II. Said Touch Screen display should continuously indicate & control:

a. Controls O2 from 0.0 % to 25.0 % in 0.1% increments

b. Controls CO2 from 1.0 % to 30.0%in 0.1% increments

c. Controls Pressure from 0.15 to 0.30 KPA increments

d. Control of Temperature from ambient to 48 ° C

e. Control of Humidity from ambient to 85 % Rh

III. Said LCD display simplifies the calibration process

a. Automatically calibrates O2 sensor through one touch screen control.

b. Provides rapid equalization.

c. Facilitates the download of data.

IV. Said Touch Screen display allows hypoxic cycling:

a. Facilitating up to 4 different O2 and Co2

b. Concentrations through a user-defined sequence of time

c. Oxygen sensor and Co2 sensor shall be present in the main working Chamber

V. Workstation shall be supplied with Gas Control Software

USB communications port, 60 days continuous storage of event log data of Temperature, Pressure, O2, Co2 One touches calibration (O2), On-screen fault assistance, Cycle programming

Data Logging : Real Time Monitoring, Data Logging,

Alarms for Breaches, Fully Automated with 60 day data logging available

VI. Digital Display with in build Sleep Mode Operation: Automatically save energy as well as help to maintain sterile work area during workstation is not in operation

There should be utility port with “flexible hose” for manual purging by nitrogen, inside the chamber, through Foot Switch

Condensate controller technology should be inbuilt in the workstation

Workstation shall be controlled & continuously show positive pressure of the chamber. Positive pressure (0.15 KPA / 0.0015 bar) of inner environment, shall be continuously maintained inside the incubation chamber

Atmosphere monitoring : O2, Co2, H2, Temperature and Humidity Sensors

Visual alarm for low or excess oxygen & Co2 level shall be provided

Visual alarm for gas cylinder pressures, chamber pressure and temperature shall be provided

Safety Features: Excess Pressure relief valve for releasing excess pressure inside chamber, shall be provided.

Overshoot Temperature Control System - Temperature Overshoot controller for safety purpose shall be provided

Inbuilt Trim-point for temperature calibration shall be provided.

Workstation shall be front 10% slope viewing panel.

Workstation shall be operated by foot switch, for operation of gas nozzle ports & spot lamp inside chamber and Nitrogen purging

Foot-operated high intensity halogen inspection spot lamp for close sample analysis shall be provided

Humidity Control: To give precise environmental control. Ambient to 85 % shall be provided

Temperature Control: Incubation control from Ambient + 5 °C to 48 °C

Temperature overshoot controller for safety purpose shall be provided.

Gloveless technology for direct hand access into workstation shall be provided

5/15-amp, Electrical power socket within the work area shall be provided

Trolley with castor wheel to keep the machine

Additional Accessories:

Nitrogen gas cylinder with regulator	1 No.	Mix gas cylinder with regulator	1 No.
Air Cylinder / Oxygen Cylinder with Regulator – 1 No.		Co2 gas Cylinder with regulator – 1 No.	
Catalyst pouch (400 gms)	1 No.	Neoprene Gloves	1 pair.
Bare Hand Gloves Facility for access inside the chamber & easy And comfortable handling	2 Nos.	Anaerobic indicator media / Stripes with terable & Sealed cover Petriplate Holder	5 Nos

Tropicalization:

- Operating Temp 25°C to 48°C
- Storage Temp up to 48 °C
- Relative Humidity : Up to 90 % No condensing

Power Supply :

- Power Input : 220 V-240V AC,50 Hz fitted with plug
- Resettable over current breaker fitted with protection


23. Standards &Safety :

- CE Marked product
- ISO 9001 : 2015
- GMP Certified


Warranty : 3 years comprehensive, onsite warranty Included

Applicable Standards : EN ISO 14971:2012, EN ISO 13485 : 2012 , EN 980:2008 , EN 1041 : 2008 , EN 61010-1:2010, EN 61326-1:2013, EN 12469:2000


Touch Screen Display

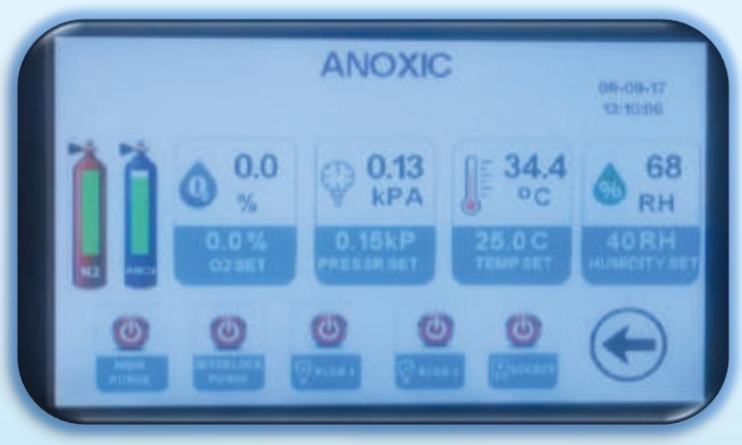

Data Logging Facility

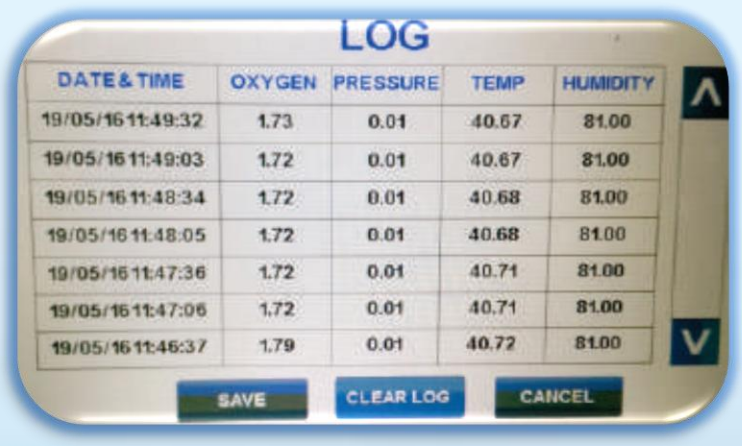


Calibration of Oxygen

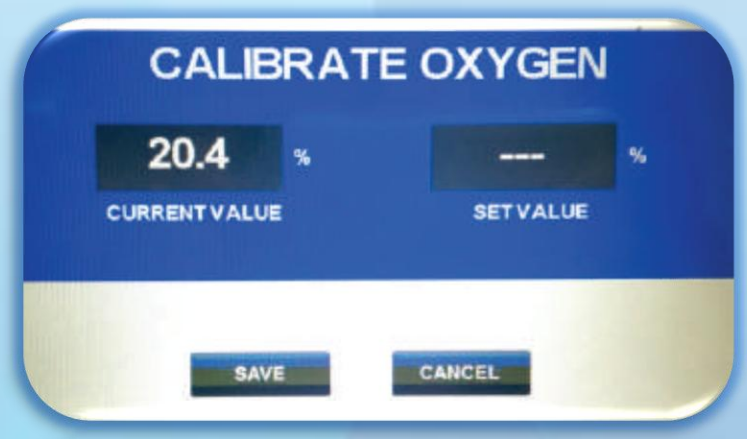



Settings

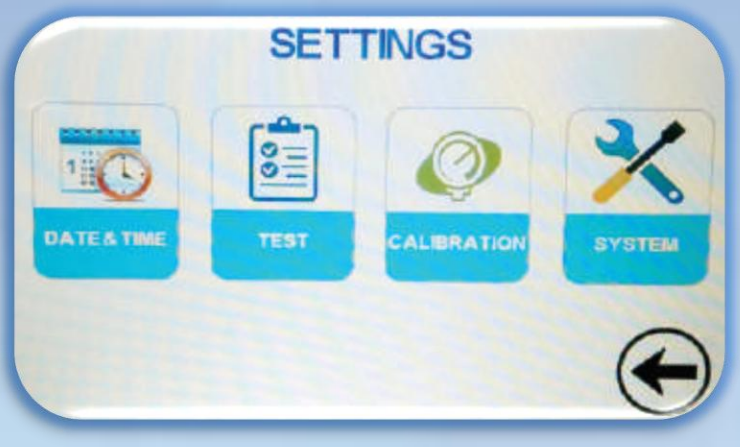

“Flexible hose” One Utility Connection Port




Interlock Transfer



Condensing Cooling Plate



Spot Lamp

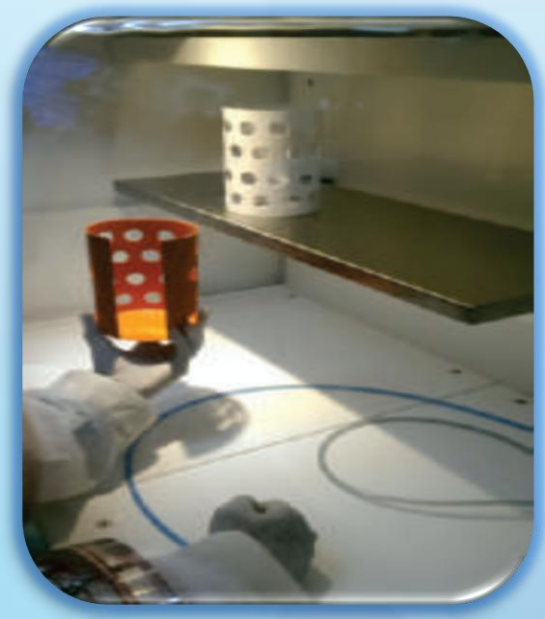

Foot Switch



Bare Hand Facility




Petri Dish Holders





Gloves



Catalyst & Detox Pouch

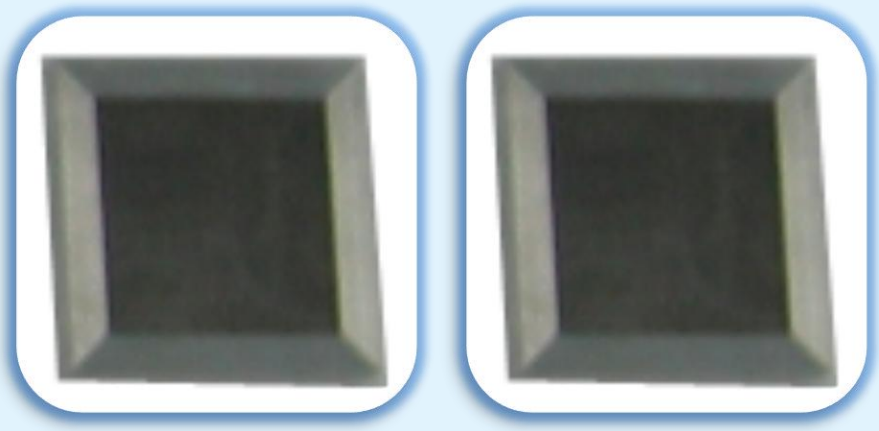

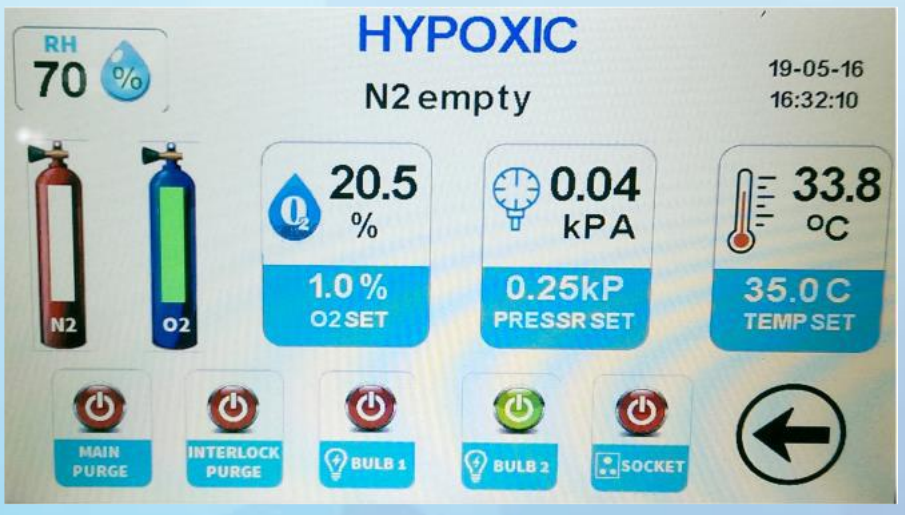

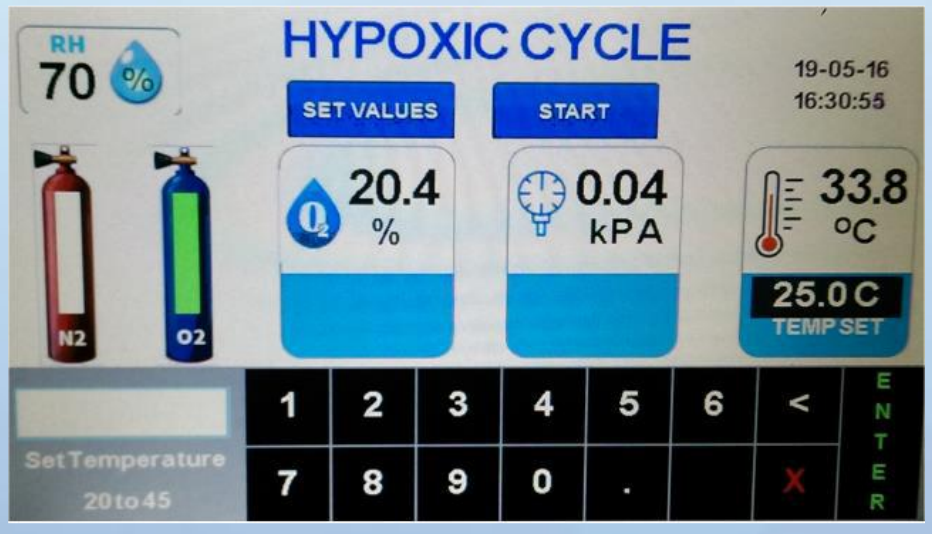

FOR BIOXIA

H-7, Rajlaxmi Commercial Complex, Ground Floor, Kalher,

Tal – Bhiwandi, Dist – Thane, Pincode - 421302

PRODUCT SUMMARY

MODEL	M 800
Max Plate Capacity	950
Interlock Plate Capacity	66
Interlock Cycle Time	45s
Cabinet Mode of Construction	Durable, Non-Corrosive, Opaque sheet of Acrylic Resin of 6mm or 8mm thickness
Max Incubation Temperature	48° C
Gas Supply	Premixed anaerobic gas (H2: Co2: N2 . 10% : 10 % : 80 %), N2, Co2 and Air or Oxygen
Humidity control	√
Condensate Control	√
Positive Pressure Display	√
Safety Excess Pressure Relief Valve	√
Low Gas Alarm	√
Inspection Spot Lamp	√
Fluorescent Illumination	√
Palladium Catalyst	√
Activated Carbon Particles	√
Oxygen Sensor with Display	√
Oxygen Controlled with Display 0.0% to 25.00%	√
Co2 Controlled with Display 1 % to 30 %	√
Ultra Violet (UV) Light	O
Bare Hand Facility	√
Incubator	Integrated
Foot Switch Operation	√
Removable Front	√
Internal Power Supply	√
Utility nozzle Connection	√
LCD Display with control	√
Fan Unit	√
Adjustable Shelf	O
Anaerobic Indicator	√
Cabinet Stand	√
Regulator for Cylinder	√
Pair of Gloves	√
Vacuum Line Port	√
Cable Gland Port	√
Petri Dish Holder	√

√ - Available 0 - Optional N/A - Not Available

Work Address: H-7, Rajalaxmi Commercial Complex, Ground Floor, Kalher, Tal- Bhiwandi, Dist- Thane 421302

Email: bioxia.in@gmail.com | Website: www.bioxia.co.in