



IMSET Maxi-Safe Series
Biosafety Cabinet

"Your Safety, Our Commitment"

International Marketers for Scientific Equipments & Technologies

Tel. : 022 32086999, 9320136999 | **Email:** support@imset.co.in | www.imset.co.in

Works : IMSET - House, 12, Khandelwal Industrial Estate, Pokhran Road No.1, Upvan, Thane (W) 400606 Maharashtra, INDIA.

• Bangalore • Delhi • Pune • Hyderabad

ISO 9001 BEC certified CE

An ISO 9001-2008 Certified Company

www.imset.co.in

SAFETY

- Safety Alarm – For HEPA, UV, Sash door.
- True value for Inflow & Downflow.

EASY TO USE

- User friendly Microprocessor based LCD Display.



COMFORT

- Ergonomic design for easy access.
- Armrest for easy work & maintains unique air flow.

CERTIFICATIONS

- ISO 2001:9008, CE, EN Compline.
- WHO & CED consultation.
- IQ / OQ / PQ certification.

SERVICE

- Prompt & timely Service.

SATISFACTION

- More than 500 satisfied Installation.


ISO 9001 BEC certified CE

An ISO 9001-2008 Certified Company

PRODUCT SUMMARY

FEATURES	SPECIFICATION	MODEL NO.		
		MS BSC C II A2	MS BSC C II B2	MS BSC C III
STD Model working Dimensions (Aprox.)	2x2	✓	✓	✓
	3x2	✓	✓	✓
	4x2	✓	✓	✓
	6x2	✓	✓	✓
Performance Certificates	CE	✓	✓	✓
	ISO 9001: 2008	✓	✓	✓
	EN ISO 14971:2012 Applicable Standards.	✓	✓	✓
	IQ, OQ & PQ. Calibration & Traceability certificates.	✓	✓	✓
	Factory tested DOP certificate.	✓	✓	✓
Air Flow	Air Flow Pattern	70% air exhaust & 30% air recirculated	100% air exhaust	100% air exhaust
Display Velocity	Validated True inflow velocity & down flow velocity.	✓	✓	✓
LCD Display	Digital Microprocessor Control System-LCD display for UV Light, Blower / Motor, Fluorescent Light.	✓	✓	✓
Intelligence Alarm System	Safety purpose Audio & Visual alarm for air fluctuation and for life of the HEPA filter and UV light.	✓	✓	✓
Sleep mode Operation	Automatically Blower Speed reduced up to 30%, this will help to save energy as well as help to maintain sterile work area during Biosafety cabinet is not in operation.	✓	✓	✓
UV Light programming	UV Light programming to avoid operator risk	✓	✓	✓
Interlocking - UV	Automatically switches “ON” when the sash door is closed & switches “OFF” when door is opened.	✓	✓	✓
Illumination of work surface	Fluorescent tube light (intensity > 600 lux) provides excellent illumination for work surface & reduces operator fatigue.	✓	✓	✓
Supply / Exhaust HEPA filter	HN 14 HEPA filter 99.997% at 0.3 micron	✓	✓	✓
Ulpa filter	ULPA filter 99.999% at 0.3 micron	O	O	O
Armrest	To avoid contamination from outside to inside contamination & for easy working with comfort.	✓	✓	✓
Drainage port	Provide beneath work surface to facilitate easy & better cleaning of the interior.	✓	✓	✓
Front control panel	Provided to avoid exposure of UV Light & Lamp outside, making eyes more comfortable.	✓	✓	✓
Heat Emission	Heat Emission at 25°C.Ambiant BTU/hr (kW)	800	1400	2200
Power supply	- 230 V ± 15%, 50 Hz	✓	✓	✓
Weight	Cabinet Net weight in Kg For std 3 x 2 Model	180	220	270
Standard Accessories				
Electrical Socket	2 No. of Electrical Socket provided inside the cabinet	O	O	✓
Glove Port	Glove port for entering hands in work area	O	O	✓
Virus burnout	Temperature reaches upto 200°C	O	✓	✓
Ducting	PVC ducting 6” dia from cabinet to exhaust	O	✓	✓
Clean air system	Helps to reduce bacterial load	O	O	O


SCHEMATIC DRAWING - MAXI SAFE SERIES (Fig. 1)

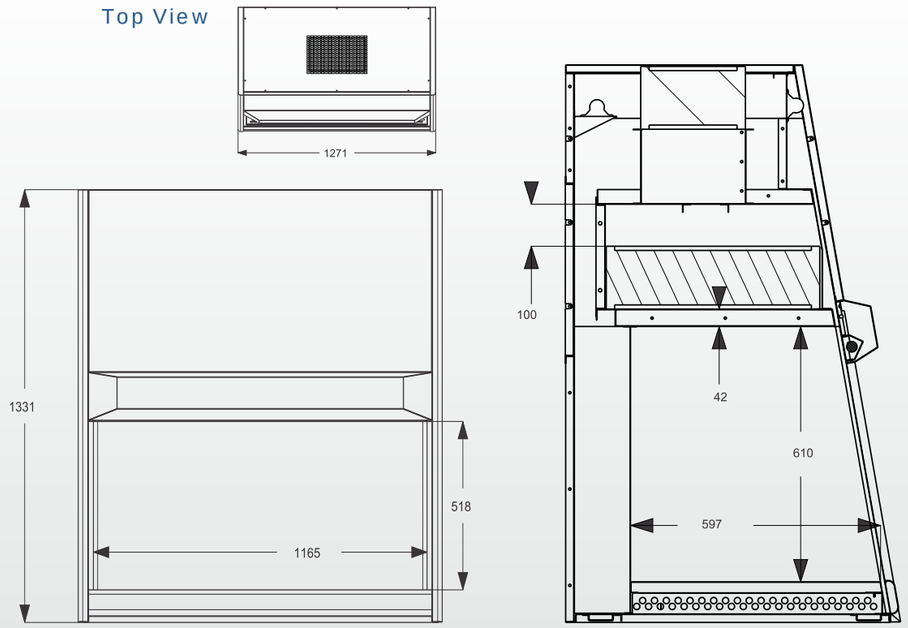

(Figure 1)

LAYOUT FOR WORKING WITHIN BIOSAFETY CABINET (Fig. 2)

ISO 9001 BEC certified CE
An ISO 9001-2008 Certified Company

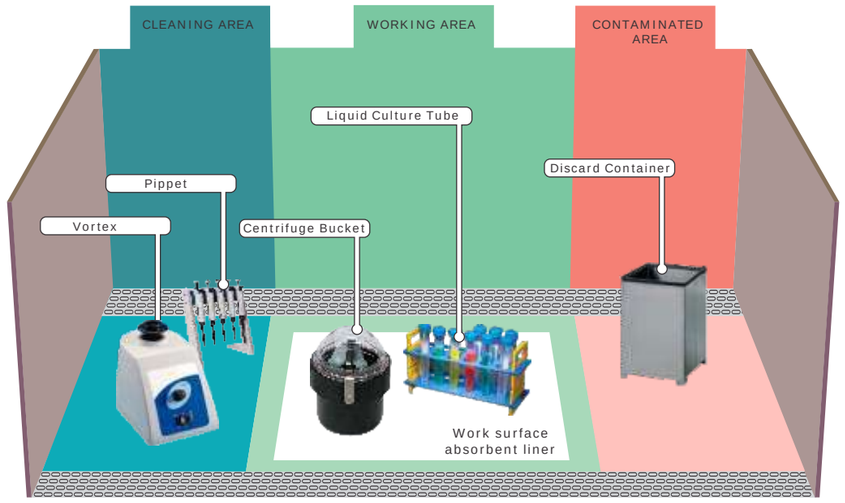

(Figure 2)

Typical layout for working from clean areas to unclean areas within a Class II biological safety cabinet. Clean materials are placed to the left of the cabinet; samples are inoculated in the centre of the cabinet; and contaminated pipettes and other materials are placed into waste containers on the right side of the cabinet. This arrangement can be reversed for people who are left-handed

TOUCH SCREEN LED DISPLAY


- Auto mode
- Manual Mode
- True Value for Inflow & Downflow.
- Safety Audio & Visual Alarm on Display:
  - HEPA blockage
  - UV On
  - Sash door level.
- UV Safety on Display:
  - UV Life indicator
  - UV Counter
  - UV Guard
  - UV auto off when sash door opens
- Blower, Fluorescent light on/off on display





HEPA

- HEPA Factory test certificate (ULPA optional)
- Ergonomic feature

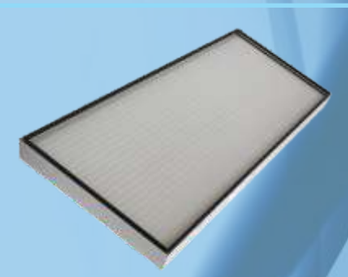

ERGONOMIC SLOPE

- Ergonomic slope

SASH DOOR

- With auto adjust height



STAND

- To mount cabinet and position work area at a comfortable height support stand available with castor wheels & self leveling feet

SS TRAY

- Arm rest bar
- Complete removable & autoclavable tray.
- Easy operation & perforated on all sides for better results
- Drainage Port



Class II A2

Class II Biohazard Safety cabinet should provide personnel, product & environment protection.

Class II Cabinets differ in proportion as 70% air is re-circulated within the cabinet through high efficiency particulate air (HEPA) filtration.

Velocity of airflow to the work zone creates an class 100 environment for product protection, where the remaining exhaust air is discharged out through (HEPA).

Air barrier at the work opening & the contaminated air plenum under positive pressure. An air barrier between the operator & the work zone maintained by a flow of room air through a full width grille in the work opening.

]The barrier air mixes with the laminar flow air in a sump underneath the work surface & is exhausted to the outside environment through a HEPA filter.

Filter

Ulpa Filter is also provided as per request.

Electrical Socket

2 nos. of electrical socket inside the chamber

Sleep Mode Operation

We have a special feature of sleep mode operation wherein your machine runs on low consumption of electricity where the blower speed is reduced for longer performance.

Virus Burnout Unit

Virus Burn out unit recommended for Class II Biosafety Cabinet at the exhaust. Virus Burn out unit is a controlled unit where temperature is controlled up to 200 °C

Ducting System

Ducting connection is used with Class II Cabinet that is ducted to the outside. Ducting constructed in PVC with 6" Diameter from cabinet to exhaust.

The capacity of the exhaust system must be sufficient to capture both, room air and the cabinet exhaust air.





ISO 9001 BEC certified CE

An ISO 9001-2008 Certified Company

Class II B2

Class II B2 Cabinets 100% air exhaust through HEPA filter.

The BSC meets the requirement of Class II B 2 NSF 49 or Class II EN 12469.

Typical Layout for working from clean room areas to dirty areas within a Class II biological safety cabinet (See Fig.2)

Operators :

All individuals working in BSC's should be observed to ensure they follow correct working practices before they routinely perform testing in BSC. The number of movements made across the front opening should be minimized by placing all necessary items into the cabinet before beginning manipulations.

Open Flames :

Open flames must be avoided in BSC's because heat disrupts the patterns of airflow within the cabinets. The use of disposable loops and disposable transfer pipettes is preferred.

Spills :

When a spill occurs inside a BSC, clean up should begin immediately. An effective disinfectant should be used and applied in a manner that minimizes the generation of aerosols

Class III

Class III Design: Personnel, Product / Sample, Environment Protection

Safe: Exhaust air is double-filtered through high-quality HEPA FILTRATIONS for 99.99% typical efficiency

Airflow: 100% Exhaust

Comfortable: Ergonomic 10 Degree Sloped Front

Seamless Tabletop: Allows easy cleaning

Cabinet operates at negative pressure relative to the laboratory in order to prevent migration of pathogenic materials out of the work area.

