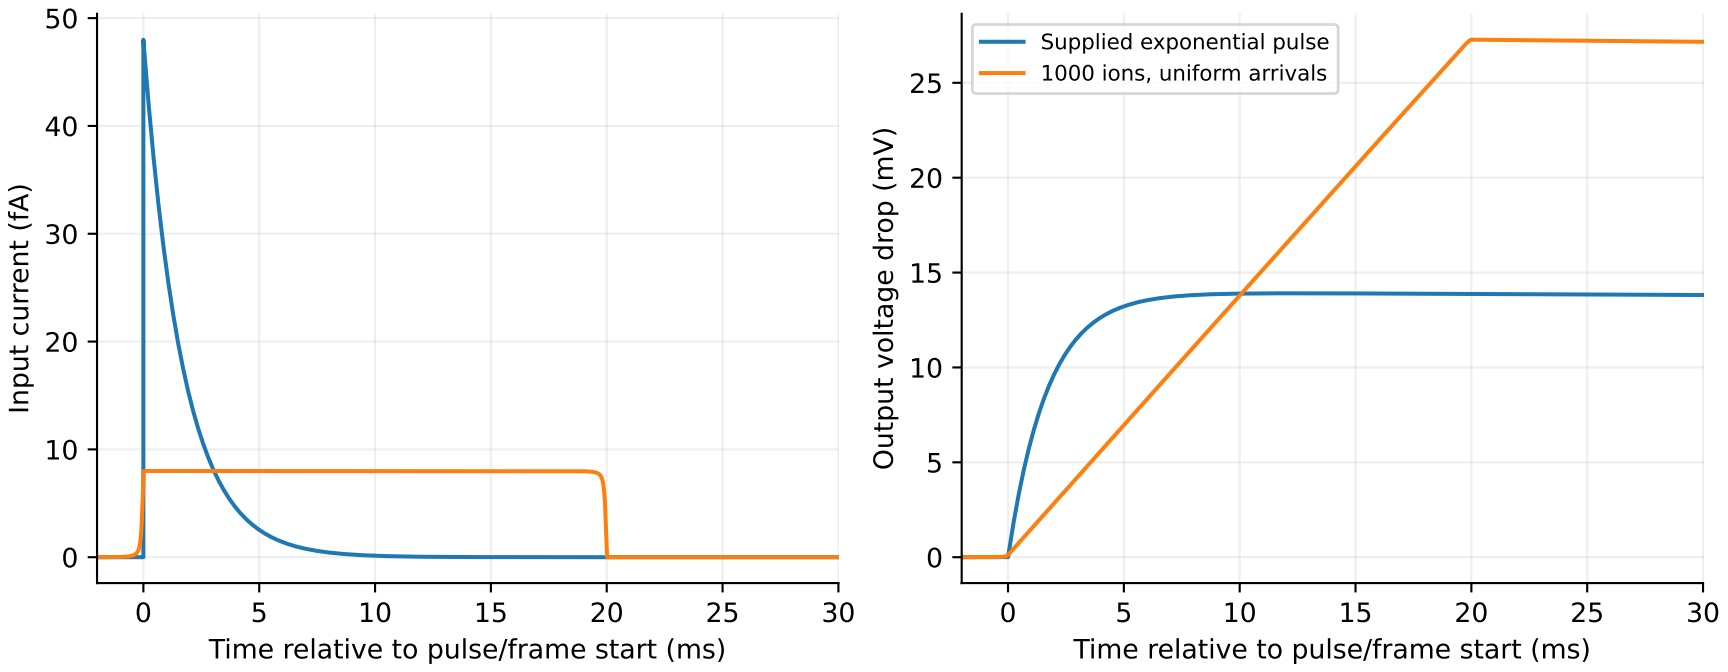
Input current (fA)
Time relative to pulse/frame start (ms)
Output voltage drop (mV)
Time relative to pulse/frame start (ms)
Supplied exponential pulse
1000 ions, uniform arrivals