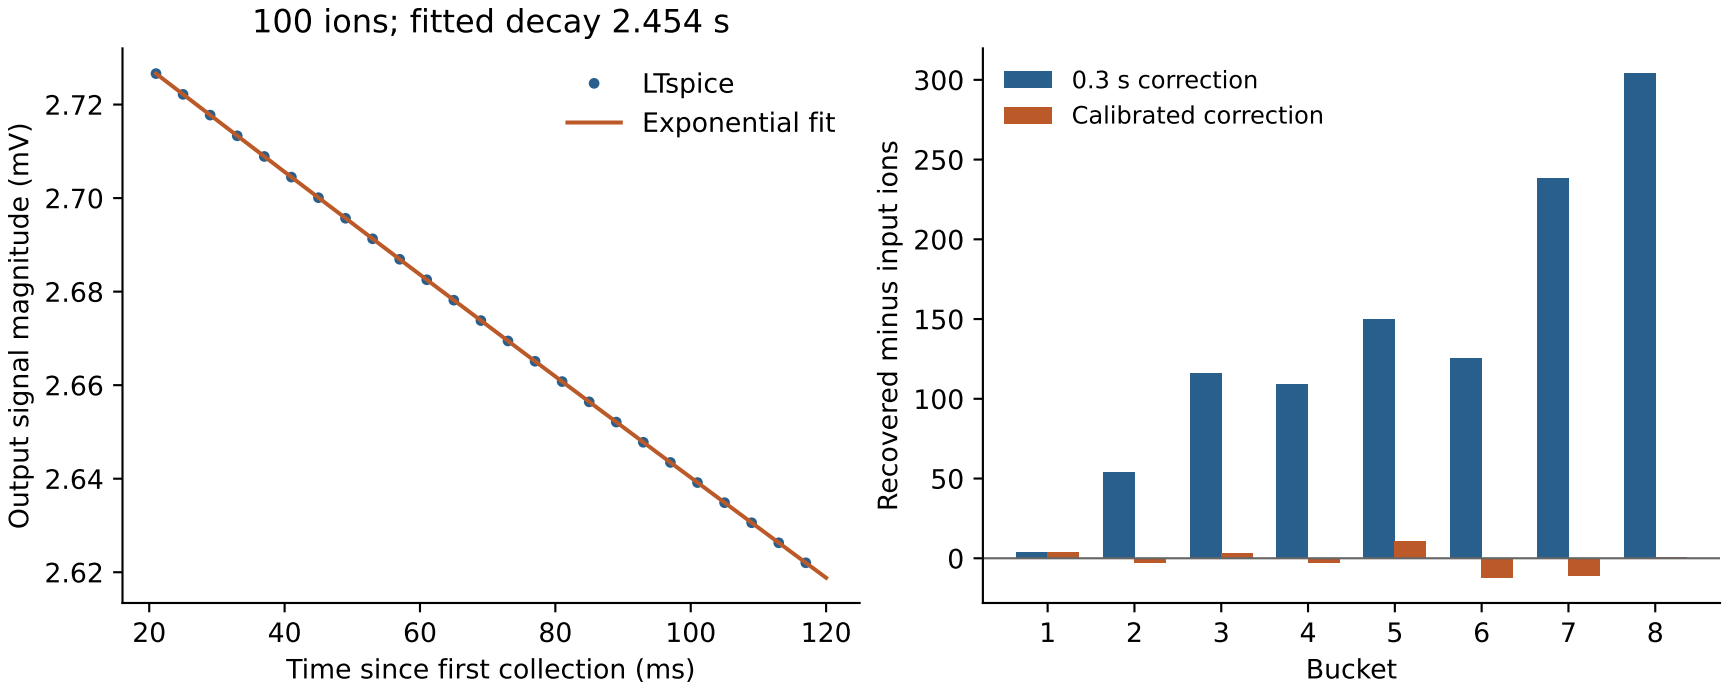
100 ions; fitted decay 2.454 s
LTspice
Exponential fit
Output signal magnitude (mV)
2.72
2.70
2.68
2.66
2.64
2.62
20
40
60
80
100
120
Time since first collection (ms)
0.3 s correction
Calibrated correction
Recovered minus input ions
300
250
200
150
100
50
0
1
2
3
4
5
6
7
8
Bucket