



Mechanism Ablation Context


Higher is better

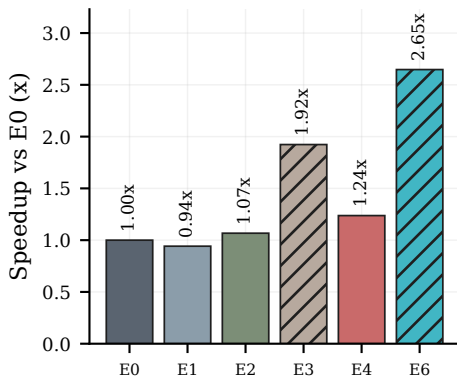

Lower is better

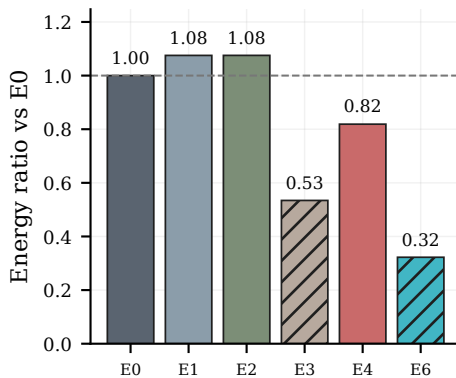

Lower is better

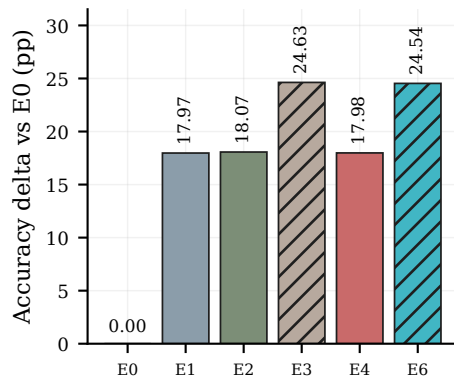

E0 ASTRA | E1 MESO | E2 HOPS | E3 DET | E4 SPARSE | E6 FULLER

Current Phase4-basis mechanism rows; DET/SPARSE/FULLER remain bounded operating points with measured accuracy cost.