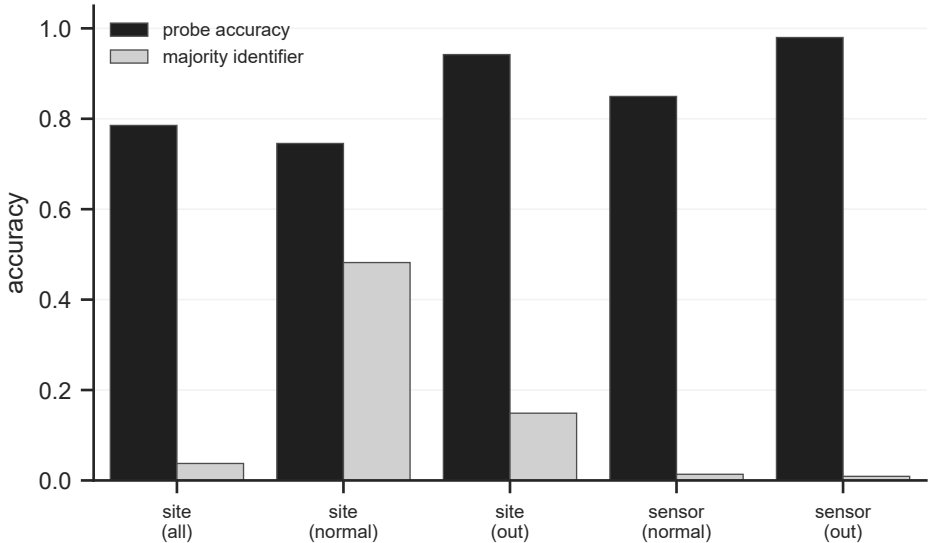
(a) identity decodable from the spectrum
probe accuracy
majority identifier
accuracy
1.0
0.8
0.6
0.4
0.2
0.0
site (all)
site (normal)
site (out)
sensor (normal)
sensor (out)

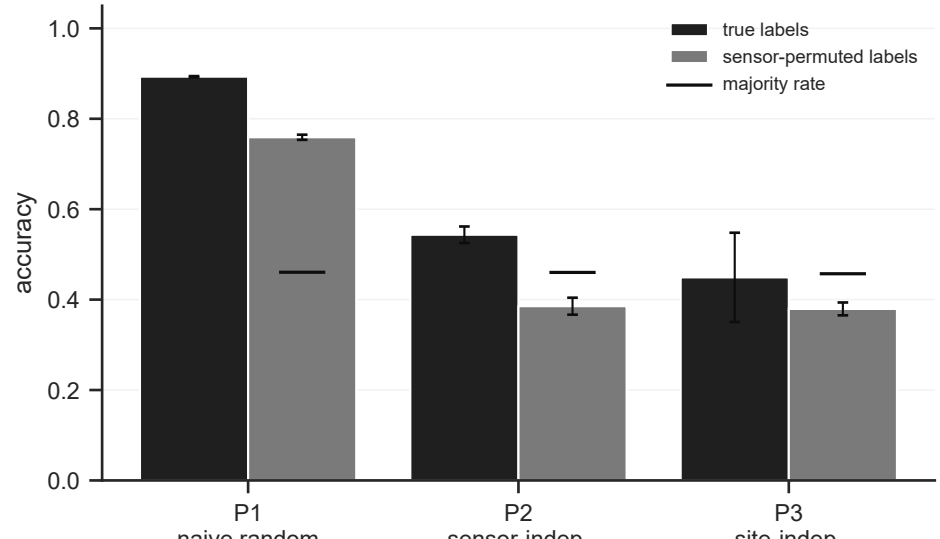
(b) accuracy with labels tied only to sensor identity
true labels
sensor-permuted labels
majority rate
accuracy
1.0
0.8
0.6
0.4
0.2
0.0
P1
naive random
P2
sensor-indep.
P3
site-indep.