

This paper is a non peer-reviewed preprint submitted to EarthArXiv. Future version of this paper may contain slightly different content. Please feel free to contact the authors; your feedback is welcome and appreciated.

Last updated: January 20, 2022

LaserTRAM-DB: A Time Resolved Analysis Module for the complete reduction of Laser Ablation Inductively Coupled Plasma Mass Spectrometry data

Jordan Lubbers^{*1}, Adam Kent², Chris Russo²

¹U.S. Geological Survey, Alaska Volcano Observatory

²College of Earth, Ocean, and Atmospheric Sciences, Oregon State University

^{}jelubber@gmail.com*

Contents

Summary	1
Background	1
Governing Equations	1
Normalizing to an internal standard	2
Drift Correction	2
Uncertainties	3
Installation and Use	4
Installation	4
Walkthrough	4
LaserTRAM: New Project Tab	5
LaserTRAM: Re-processing Tab	7
LaserTRAM profiler	7
LaserCalc: Concentrations Tab	8
LaserCalc: Primary Standard Tab	9
Video Demos	9
Citing	10
Acknowledgements	10
References	11

Summary

LaserTRAM-DB is a dashboard for the complete processing pipeline of Laser Ablation Inductively Coupled Plasma Mass Spectrometry (LA-ICP-MS) data in complex materials such as geologic samples. As LA-ICP-MS data in geologic samples frequently have multiple phases, inclusions, and other compositional complexities within them that do not represent the material of interest, user interaction is required to filter unwanted signals out of the overall ablation signal. LaserTRAM-DB allows the user to filter which portion of the ablation peak is utilized in calculating concentrations, subsequently allowing for more accurate data to be obtained. Furthermore, it allows for the processing of both individual spot analysis data and a line of spots gathered in rapid succession, reducing the time required for data reduction while preserving spatial definition and still ensuring data quality.

Background

With a wide array of applications in the natural sciences (e.g., [Fritz-Endres and Fehrenbacher, 2021](#); [Caricchi et al., 2020](#); [Loewen and Kent, 2012](#); [Lukács et al., 2021](#)), laser ablation inductively coupled plasma mass spectrometry (LA-ICP-MS) is now a commonplace tool for the gathering of *in situ* trace element (i.e., < 0.1 wt%) data from solid materials. The last two decades have seen significant advances in both instrument capabilities and operating software, allowing users to generate large volumes of *in situ* geochemical data in comparatively little time to previous methodologies (i.e., micro-drilling) while still maintaining high degrees of accuracy and precision.

Raw data output from LA-ICP-MS, however, is in the form of counts per second (cps) for the selected analyte isotopes, not elemental concentrations. In order to be converted into accurate concentrations, a modest amount of user input and interpretation is required and should not be automated. Currently, there are several proprietary and open-source softwares for LA-ICP-MS data reduction to accomplish this task: SILLS - [Guillong et al. \(2008\)](#); Lolite - [Paton et al. \(2011\)](#); LAtools - [Branson et al. \(2019\)](#); Termite - [Mischel et al. \(2017\)](#); GLITTER - Macquarie University GEMOC; and countless other “in house” spreadsheet-based tools. All have their strengths and weaknesses, however, there is yet to be a powerful, web-hosted Graphical User Interface (GUI). Built primarily using Plotly-Dash [Plotly Technologies Inc.], numpy ([Harris et al., 2020](#)), and pandas ([McKinney et al., 2010](#)), we present a completely open-source dashboard: Laser Time Resolved Analysis Module Dashboard (LaserTRAM-DB) that allows the user to calculate concentrations from raw LA-ICP-MS data with the flexibility of a GUI interface while maintaining the performance of the numerical python ecosystem. Furthermore, by simultaneously displaying both raw data cps and internal standard normalized cps, it allows for rapid decision making about data quality to be determined. Below we outline the theory, workflow, and structure, behind LaserTRAM-DB in an effort to maximize its effectiveness.

Governing Equations

We calculate the concentration of analyte (i) in an unknown material (u) using the following relationship from [Longerich et al. \(1996\)](#):

$$C_i^u = \frac{R_i^u}{S} \quad (1)$$

Where C_i^u and R_i^u are the concentration of analyte and count rate of analyte (i) in the unknown material, respectively, and S is the normalized sensitivity. When using naturally occurring internal standards, S can be defined as:

$$S = \frac{R_i^{std}}{C_i^{std}} \left[\frac{R_n^u}{R_n^{std}} \frac{C_n^{std}}{C_n^u} \right] \quad (2)$$

R_i^{std} and C_i^{std} are the count rate and concentration of analyte (i) in the calibration standard, R_n^u and R_n^{std} are the mean count rates of the internal standard in the unknown material and calibration standard, C_n^u and C_n^{std} are the concentrations of the internal standard in the unknown material and calibration standard.

[Kent and Ungerer \(2006\)](#) re-arrange this relationship such that the count rate expressions always contain unknown analytes in the numerator:

$$C_i^u = C_n^u \frac{\left[\frac{C_i^{std}}{C_n^{std}} \right]}{\left[\frac{R_i^{std}}{R_n^{std}} \right]} \frac{R_i^u}{R_n^u} \quad (3)$$

Normalizing to an internal standard

The purpose of LaserTRAM-DB is to give the user complete control over which portion of the analytical spectra gets used in calculating concentrations (e.g., filtering out portions of the signal not reflective of the material under investigation). In complex natural materials, selection of this interval and an overall judgement about data quality require an operator to make a decision. This software is optimized to allow that decision to be made as efficiently and rapidly as possible.

When a given interval from the analytical spectra has been chosen, every analyte is normalized to a chosen internal standard. LaserTRAM-DB allows for any analyte in the experiment to be used as the internal standard. Prior to normalization to an internal standard, raw data first has the background analyte levels subtracted from it. Background is determined by taking the median counts per second value for each analyte over the user specified background range. Once data have been background subtracted, each normalized ratio is calculated the following way:

$$N_i = \text{median} \left[\frac{cps_i}{cps_{is}} \right] \quad (4)$$

Where cps_i is the background subtracted counts per second data for analyte (i), and cps_{is} is the background subtracted counts per second data for the internal standard. Since counts per second is analogous to count rate above in Equation 3, we can simplify the above relationship to now reflect our N_i values:

$$C_i^u = C_n^u \frac{\left[\frac{C_i^{std}}{C_n^{std}} \right]}{N_i^{std}} N_i^u \quad (5)$$

Here, N_i^{std} and N_i^u are the normalized counts per second value of analyte i in the calibration standard and unknown, respectively. The uncertainty for any given normalized ratio is expressed as:

$$SE = \frac{\sigma_{N_i}}{\sqrt{n}} \quad (6)$$

σ_N is the standard deviation of a given analyte's normalized ratio for the interval and n is the number of time steps in the interval (i.e., cycles through the mass range). The relative standard error is then:

$$RSE_i^u = \left[\frac{SE}{N_i} \right] 100 \quad (7)$$

Detection Limits

Detection limits for each analyte are determined to [Longerich et al. \(1996\)](#):

$$LOD = \frac{3\sigma_b}{\sqrt{n_b}} \sqrt{2}$$

where σ_b and n_b are the standard deviation and total number of observations in the chosen background range, respectively. This is standard practice in LA-ICP-MS data reduction. To reflect this in data output, measurements that are below detection limit will have values that say "b.d.l." rather than concentrations.

Drift Correction

To check for drift in calibration standard normalized ratios over time, a linear regression is applied to the calibration standard for each analyte, where the dependent variable is the count rate normalized to the internal standard and the independent variable is the timestamp associated with each analysis (Figure 1):

We determine the significance of each regression by evaluating following null hypothesis: there is no relationship between a given analyte's internal standard normalized ratio and time. We reject this if both the following conditions are true: The p-value for the coefficient (i.e., slope) is significant; The F-statistic comparing the regression and observed data is greater than the critical F value. By default, we set the threshold for p-value significance at .01 (i.e., we have 99% confidence that we can reject the null hypothesis) in an effort to mitigate

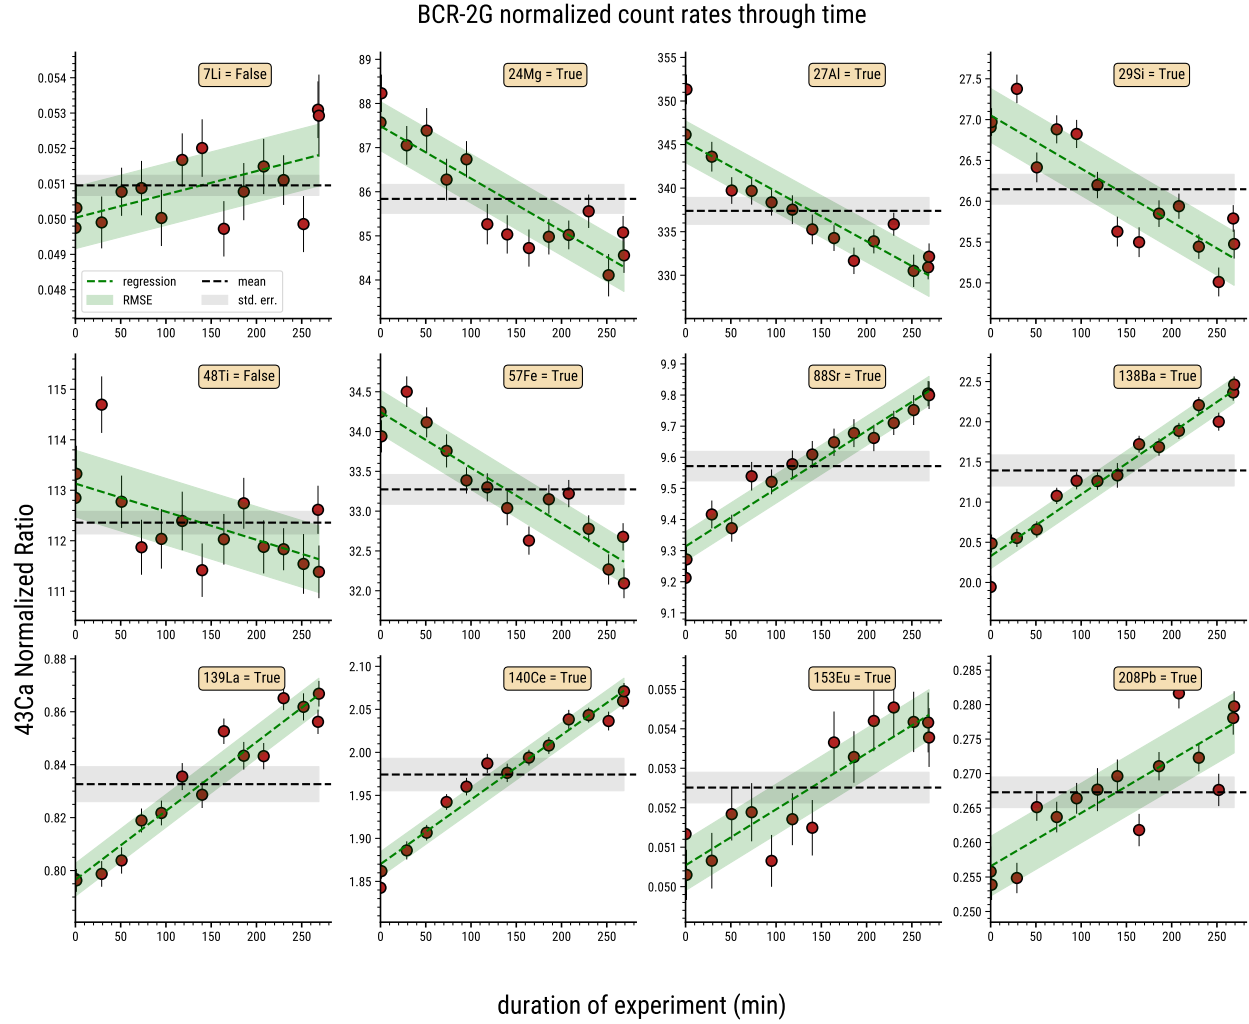


Figure 1: Drift correction test from LaserCalc for a given experiment in which standard reference material BCR-2G was used as the primary standard. We can see here that one experiment may contain analytes that are both drift corrected and not drift corrected.

drift correcting all but the most linear of changes in normalized count rates, but this may be changed by the user. If the null hypothesis for a given analyte is rejected, the analyte is linearly corrected for drift and the regression parameters (e.g., slope and intercept) are used to calculate a normalized count rate for the calibration standard at the point in time where an unknown was analyzed:

$$C_i^u = C_n^u \left[\frac{C_i^{std}}{C_n^{std}} \right] \frac{1}{[m_i x + b_i]} N_i^u \quad (8)$$

Where m is the regression slope, x is the analysis time, and b is the intercept for analyte i .

Uncertainties

Calculating concentrations of a given analyte in an unknown material can be considered a series of nested quotients and products. Therefore, we quantify the overall uncertainty of a given analyte as [Taylor \(1997\)](#) p.61:

$$\sigma_{C_i} = C_i^u \sqrt{\left(\frac{\sigma_{C_u^n}}{C_u^n} \right)^2 + \left(\frac{\sigma_{C_i^{std}}}{C_i^{std}} \right)^2 + \left(\frac{\sigma_{C_n^{std}}}{C_n^{std}} \right)^2 + \left(RSE_i^{std} \right)^2 + \left(RSE_i^u \right)^2} \quad (9)$$

Where RSE_i^{std} is defined as:

$$RSE_i^{std} = \left[\frac{\frac{\sigma_i}{\sqrt{n_i}}}{\mu_i} \right] 100 \quad (10)$$

σ_i and μ_i are the standard deviation and mean of all of the calibration standard normalized ratios respectively and n_i is the total number of calibration standard analyses for analyte (i).

For analytes where drift correction has been applied, RSE_i^{std} is replaced with:

$$100 \left[\frac{RMSE_i}{\mu_i} \right]$$

Where $RMSE_i$ is the Root Mean Squared Error as specified in the Drift Correction section.

Concentrations of internal standard in unknown

To calculate concentrations of a given analyte list in an unknown sample, the concentration of the internal standard must be known. LaserCalc takes these concentrations in the form of wt% oxide and utilizes user interaction to input concentrations of the internal standard and its relative uncertainty. A default value of 1% is used for this, but may be updated by the user.

Installation and Use

Installation

The easiest way to use LaserTRAM-DB is to use the following link:

- <https://lasertram-db.herokuapp.com/>

Alternatively, LaserTRAM-DB can be installed locally and run by creating a virtual environment. If you are new to python, we recommend doing this through [Anaconda](#).

```
git clone https://github.com/jlubbersgeo/laserTRAM-DB
cd /path/to/laserTRAM-DB
conda create -n lasertram-db python=3.7.7
conda activate lasertram-db
conda config --append channels conda-forge
conda install --file requirements.txt
python lasertram-db.py
```

Once the virtual environment is set up you can also open and run the `lasertram-db.py` script from any python IDE (e.g., Spyder, IDLE, PyCharm, etc.)

When the program is running, copy and paste the provided link provided in the terminal window into the browser window and the app will run. From now on any time you wish to use the program, simply re-activate the virtual environment and run the script like above. For optimal performance, we recommend using the virtual environment option for LaserTRAM-DB. Currently, LaserTRAM-DB is hosted through Heroku with limited computing power. Using through a local machine capitalizes on the computing power of that local device, which in almost all instances will be superior to Heroku.

Walkthrough

Here we will walk through each step of the data processing pipeline in LaserTRAM-DB. In brief, it is comprised of 2 parts:

1. Normalizing data to an internal standard

- **LaserTRAM**: Choosing an interval of interest from raw cps data in individual spot analyses and normalizing it to an internal standard.
- **LaserTRAM profiler**: Functionally the same as LaserTRAM, however has tools that allow for the rapid inspection of a line of spot analyses gathered in quick succession.

2. Calculating concentrations from data that has been normalized to an internal standard

- **LaserCalc**: Takes the output from either LaserTRAM or LaserTRAM profiler and converts the normalized data into concentrations using the equations outlined above.

LaserTRAM: New Project Tab

LaserTRAM is comprised of two tabs:

1. New Project tab (Figure 2). This is the default window upon running the software, however none of the figures or tables will be populated yet.
2. Re-processing tab (Figure 3).

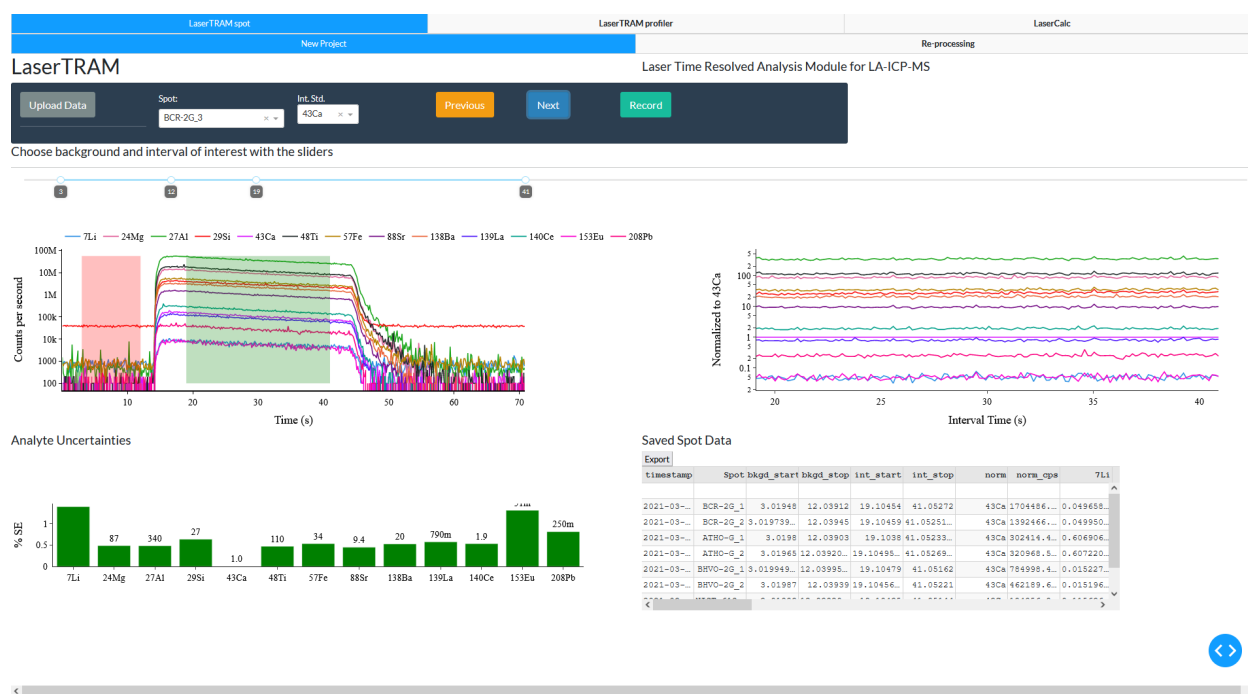


Figure 2: Example of the LaserTRAM New Project tab after data has been loaded in.

To begin a new project, simply click on the “Upload Data” button in the upper left portion of the window. A File Explorer/Finder window will prompt the user to choose their file that has been formatted for LaserTRAM. Once the data are loaded in, options will appear in the “Int. Std.” dropdown menu. Any analyte in the experiment may be chosen as the internal standard, however in order to calculate concentrations in LaserCalc later only analytes that create the following oxides may be chosen: SiO₂ (e.g., ²⁹Si), CaO (e.g., ⁴³Ca), TiO₂ (e.g., ⁴⁷Ti), Al₂O₃, Cr₂O₃, MnO, FeO, K₂O, Na₂O, NiO. To maximize data quality, it is recommended that the internal standard is an analyte that is already well quantified in the unknown (i.e., in silicate minerals ²⁹Si and ⁴³Ca are good options as SiO₂ and CaO are commonly measured accurately via EPMA and are at concentrations in most geologic materials ideal for measurement by LA-ICP-MS). While it is easy to explore many different internal standards and their effect on data quality, only one should be used for recorded intervals that will be used in calculating concentrations later.

To populate the graphs and begin processing data, choose a spot from the “Spot” dropdown menu. The first time this is done it may take a few seconds, as the entire project is being loaded in, however it will be relatively instantaneous from there on out. The layout from upper left to lower right:

- **Raw data graph:** This is the raw signal for each spot being processed. It contains regions indicating the time interval designated for background (red) and signal to be used for concentrations (green).
- **Normalized data graph:** This graph shows the green region in the raw data graph normalized to the chosen internal standard.
- **Analyte uncertainties graph:** Bar chart showing the relative standard error (i.e., Equation 10). Values on the top of each bar indicate the median normalized ratio using SI prefixes. If the relative standard error is < 5% the bar will be green, otherwise it will be yellow.
- **Saved spot data table:** Recorded data for each spot will populate here. Each time the “Record” button is pressed, a new row will be generated. More on this in a bit.

To choose intervals for background and ablation signal, simply drag the handles on the slider bar where it says “Chose background and interval of interest with the sliders”. The left two handles are for background and the right two are for ablation signal of interest. All the graphs are linked to the slider, meaning that when the sliders move they will all update in real time to reflect the decisions made by the user. When the sliders are in the desired spot, the “Record” button will save the requisite data to the “Saved Spot Data” table in the lower right. Each row contains the following:

- **Timestamp:** This is a unique time identifier for each spot that is inherited from the raw data. This will be propagated throughout the pipeline to help keep track of sample and monitor for drift in the primary standard over time (i.e. Equation 9).
- **Spot:** This is the name given to each spot in the raw data.
- **Interval data:** These are columns that contain the time information in each analysis for the start and end of both the background and interval of interest. They are `bkgd_start`, `bkgd_stop`, `int_start`, `int_stop`.
- **Internal standard analyte:** The analyte chosen as the internal standard. The “`norm_cps`” column contains the median counts per second value of the internal standard over the interval of interest.
- **Normalized data:** Columns for each analyte’s internal standard normalized value. Their header is simply the analyte name. Values that are -9999 denote analytes below detection limit for that spot.
- **Uncertainty data:** Columns to the right of the normalized data with the suffix “_se” contain the relative standard error for each analyte in percent (i.e., Equation 7).

Progressing through all spots in the experiment can be accomplished two ways:

1. Using the spot dropdown and picking the spot you wish to process (*not recommended*).
2. Using the “Previous” and “Next” buttons (*recommended*). These will navigate between adjacent spots to efficiently progress through the spot list.

When finished, the “Export” button associated with the “Saved Spot Data” table will export the table exactly how it is shown in the browser. It is recommended that in your browser you adjust the file download settings such that they ask for a save location prior to download. This will allow you more control over where the LaserTRAM completed data is stored.

LaserTRAM: Re-processing Tab

This tab takes the input and output from the “New Project” tab and re-normalizes the experiment to a newly chosen internal standard. Similar to above, use the upload data in the “New Project” tab to upload raw experiment data. This is the only step that is done in that tab, so now navigate to the “Re-processing” tab. Use the “Upload old LT file” button in the upper left to upload the output for the same experiment you wish to re-normalize. It does not matter if all of the spots in the experiment were processed, LaserTRAM will only re-normalize spots that have been previously processed. At this point, the “Old normalized Ratios” table on the left will populate with the previously normalized data, as well as a list of potential analytes in the dropdown above to choose for re-normalizing. After the desired analyte is chosen, hit “Re-process!”. This will take the interval columns from the old data and use them as bounds for the re-normalization. This should be relatively instantaneous and leave you with something that looks like Figure 3. Similar to the “New Project” tab and everywhere else in LaserTRAM-DB, the table with re-normalized data can be exported using the button attached to the table. It will have the same exact output as the “New Project” tab. If you wish to re-normalize to a few different internal standards, this is easily accomplished by choosing a new analyte in the dropdown menu and hitting “Re-process!”.

LaserTRAM spot

New Project

LaserTRAM profiler

Re-processing

LaserCalc

LaserTRAM Re-processing

Re-process an old experiment using a new internal standard

Upload old LT file

Internal Standard:

295

Re-process!

Old normalized ratios

Re-normalized data

Export

timestamp	Spot	bkgd_start	bkgd_stop	int_start	int_stop	norm	norm_ops	7Li	24Mg	27Al	29
2021-03-...	BCR-2G_1	3.01948	11.13704	21.05863	41.05272	43Ca	1467013...	0.049750...	87.57106	346.1430	26.90
2021-03-...	BCR-2G_2	3.019739...	11.13741	21.05893	41.05251...	43Ca	1364077...	0.050314...	86.23107	351.3262	26.97
2021-03-...	ATHO-S_1	3.0198	11.13702	21.05797	41.05233...	43Ca	2704953...	0.067011...	9.797868	1345.794	157.2
2021-03-...	ATHO-S_2	3.01965	11.13727...	21.0594	41.05269...	43Ca	2791833...	0.067884...	9.747460	1337.271	155.6
2021-03-...	BHYO-2G_1	3.019949...	11.13804	21.05902	41.05162	43Ca	5243534...	0.014921...	112.4873	217.4247	15.98
2021-03-...	BHYO-2G_2	3.01987	11.1375	21.05875	41.05221	43Ca	4068133...	0.014699...	112.4457	222.8923	16.24
2021-03-...	NIST-612...	3.01983	11.13722...	21.05876	41.05144	43Ca	1924704...	0.115396...	0.150267	29.89531	19.79
2021-03-...	NIST-612...	3.01969	11.13726	21.05904	41.05224	43Ca	1931813...	0.116219...	0.147278	29.93367	19.69
2021-03-...	BCR-2G_3	3.01959	11.13764...	21.05954	41.05247	43Ca	1333640...	0.049903...	87.05114	343.4064	27.37
2021-03-...	ATHO-S_3	3.01999	11.13778...	21.05894	41.052	43Ca	2905378...	0.060255...	9.809315	1334.206	152.4
2021-03-...	BCR-2G_4	3.01955	11.13711	21.05877	41.05162	43Ca	1342742...	0.050771...	87.38508	339.7267	26.41
2021-03-...	ATHO-S_4	3.01816	11.13707	21.05857	41.05153	43Ca	1773334	0.074540	8.86750	1016.506	157.1

Export

timestamp	Spot	bkgd_start	bkgd_stop	int_start	int_stop	norm	norm_ops	7Li	24Mg	27Al	29
2021-03-...	BCR-2G_1	3.01948	11.13704	21.05863	41.05272	2951	2763520...	-9999	3.235005	12.73500	
2021-03-...	BCR-2G_2	3.01974	11.13741	21.05893	41.05252	2951	2815041...	-9999	3.249927	12.95827	
2021-03-...	ATHO-S_1	3.0198	11.13702	21.05797	41.05234	2951	2776411...	-9999	0.047931	8.556533	
2021-03-...	ATHO-S_2	3.01965	11.13727...	21.0594	41.05269	2951	2813938...	-9999	0.047956	8.545669	
2021-03-...	BHYO-2G_1	3.01995	11.13804	21.05902	41.05162	2951	2021653...	-9999	4.795661	13.63969	
2021-03-...	BHYO-2G_2	3.01987	11.1375	21.05875	41.05221	2951	2009545...	-9999	4.891732	13.66376	
2021-03-...	NIST-612...	3.01983	11.13723	21.05876	41.05144	2951	3309406...	-9999	-9999	1.501574	
2021-03-...	NIST-612...	3.01969	11.13726	21.05904	41.05224	2951	3357225...	-9999	-9999	1.500641	
2021-03-...	BCR-2G_3	3.01959	11.13765	21.05955	41.05247	2951	2689861...	-9999	3.180339	12.48420	
2021-03-...	ATHO-S_3	3.01999	11.13778	21.05894	41.052	2951	2711187...	-9999	0.050033	8.686071	
2021-03-...	BCR-2G_4	3.01955	11.13711	21.05877	41.05162	2951	2610237...	-9999	3.280345	12.62688	
2021-03-...	ATHO-S_4	3.01816	11.13707	21.05857	41.05153	2951	1781411	-9999	0.05193	8.410098	

Figure 3: Example of the LaserTRAM reprocessing tab after data has been loaded in.

LaserTRAM profiler

LaserTRAM profiler is functionally the same as the “New Project” tab in LaserTRAM. It takes in raw data through upload button, has a dropdown for the internal standard, a button for recording the data for a given spot, and all of the quadrants have the same display. The major differences are as follows (Figure 4):

- The addition for a “step size” numeric input box.
- Rather than “Next” and “Previous” buttons to move between spot analyses, we have “Forwards” and “Backwards” buttons. These will step the green interval of interest by the value in the “step size” input box. This can be used in conjunction with the range sliders directly below the buttons to efficiently jump from one peak to the next in the line of spots.
- Unlike the individual spot reduction, the “Saved Spot Data” table in LaserTRAM profiler will have rows that pertain to each spot in the line of spots. They will be named accordingly following the naming scheme: “transectname_spotnumber”.

It is recommended that after each line of spots is processed it is exported and saved as its own spreadsheet. They can then be later combined in order for LaserCalc.

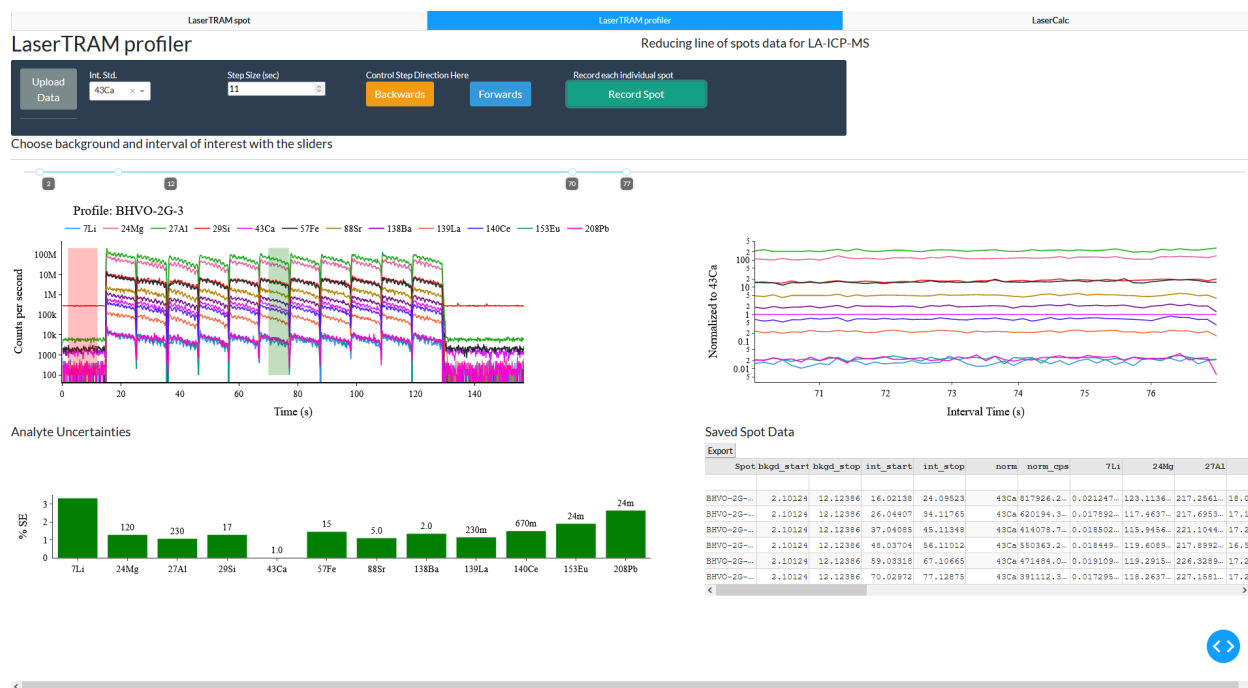


Figure 4: Example of the LaserTRAM profiler illustrating how the software can easily normalize a line of spots gathered in rapid succession to one another.

LaserCalc: Concentrations Tab

This tab takes the output of either the spot or profile versions of LaserTRAM and a spreadsheet of published concentrations for standard reference materials that can be found [here](#) under the file `laicpms_stds_tidy.xlsx`. Begin by uploading the output from LaserTRAM using the "Upload Data" button. This will populate the "Internal Std. Concentrations" table with a column for the spot name, concentration for the internal standard in wt% oxide, and a column for the relative uncertainty for the internal standard concentration. This concentration is analogous to C_n^u in Equation 3. By default it is 10 wt% regardless of the internal standard chosen, however it can be updated later to reflect more accurate concentrations.

LaserCalc will also search the spot names and determine potential calibration standards based on spot name. In order for this to work spot names in your experiment for standard reference materials **must** match those found within the `laicpms_stds_tidy` spreadsheet at least somewhere in the spot name (e.g., BHVO-2G_1, BCR-2G_23, ATHO-G_replicate). There may be extra characters but at a minimum they must contain the proper standard name. Based on the results of this search, the "Calibration Standard" dropdown will populate with options for potential calibrations standards. Data pertaining to these analyses correspond to the N_i^{std} term in Equation 5.

Once a calibration standard is chosen, hit "Calculate!". LaserCalc will apply Equation 5 or Equation 8 to the data on an analyte by analyte basis based on whether or not it needs to be drift corrected. This is relatively quick and upon completion the "Calculated Concentrations" tab will populate with calculated concentrations for all spots in the experiment (Figure 5). These, by default will be incorrect for all unknown analyses as they are using the default concentration for the internal standard. You may now adjust the values in the "Internal Std. Concentrations" table to reflect the actual concentration and uncertainty of the calibration standard for each spot. While doing this, you will notice that the "Calculated Concentrations" table will update in real time to reflect the choice made. You may also change the value for the calibration standard dropdown menu at this time and the concentrations will adjust to reflect that decision. This makes it relatively easy to calculate concentrations using a variety of calibration standards if they exist in enough abundance within your experiment. When complete,

Lower TRAM spot

Calibration Standard

ICR-MS

Drift significance threshold: 0.01

Calculate!

Upload Data

Upload Study

Lower TRAM profile

Primary Standard Data

Lower MS

LaserCalc

Calculating concentrations for LA-ICP-MS spot data

Internal Std. Concentrations:

Spot	Co ⁶⁰ wt%	Co ⁶⁰ Isotopes
ICR-26_1	10	1
ICR-26_2	10	1
ATRO-16_1	10	1
ATRO-16_2	10	1
BAVO-16_1	10	1
BAVO-16_2	10	1
HEAT-16_1	10	1
HEAT-16_2	10	1
ICR-26_3	10	1
ICR-26_4	10	1
ICR-26_5	10	1

Calculated Concentrations:

Spot	Co ⁶⁰ wt%	Co ⁶⁰ Isotopes	TiL	240p	27Al	28Si	43Ca	49Ti	67Fe	88Zr	138Ba	139La	140Ce
MS_1	1	1	1.1911095	50.16190	2110.914	493510.4	71449.76	2489.769	2042.633	488.4296	352.7465	14.10718	19.0896
MS_2	1	1	1.1618034	97.03894	27376.7	533804.3	71449.76	361.2123	2182.805	729.5762	298.0376	12.53372	16.19515
MS_1	1	1	1.2147922	73.44434	137879.9	345106.3	71449.76	356.4222	1409.744	744.4120	477.2083	28.51025	45.2239
MS_2	1	1	1.2541655	73.26458	188144.2	287556.4	71449.76	383.7624	1781.851	757.3847	381.1421	24.9023	21.27142
MS_3	1	1	1.3111564	71.49128	175213.3	348890.6	71449.76	382.2828	1744.076	736.4515	433.8765	29.64317	25.43392
MS_1	1	1	1.2027977	47.45468	177947.3	397320.2	71449.76	354.6184	1744.795	736.2324	490.2275	35.46681	27.45894
MS_2	1	1	1.2325890	49.04064	204443.5	433292.3	71449.76	349.2395	1599.132	647.8504	427.8504	32.99390	16.42114
MS_3	1	1	1.2415863	43.35804	202955.6	425669.8	71449.76	349.7748	1737.927	751.0217	433.8260	31.41088	16.40770
MS_1	1	1	1.2640242	102.7942	173110.7	331313.3	71449.76	364.1762	2042.685	780.7365	35.4372	13.42867	23.48464
MS_2	1	1	1.2638784	92.09932	149994.4	297841.7	71449.76	382.8629	1599.260	739.4529	239.4465	24.08338	26.18352
MS_3	1	1	1.2643335	70.17074	162618.1	404649.4	71449.76	357.3182	1944.395	889.2571	605.7945	32.78274	25.59704
MS_1	1	1	1.2811213	91.30734	136213.8	407941.3	71449.76	364.4068	1465.791	676.7197	431.0542	14.08100	18.56355

LaserCalc: Primary Standard Tab

Annotated on the graph are the relative standard error of the mean for a given analyte (i.e., Equation 10), the relative RMSE of the regression for that analyte over time, other descriptive statistics used in checking for drift (i.e., the p-value for the slope of the regression, the F statistic, and critical F value), and whether or not it has been drift corrected. If it has been drift corrected the equation for the drift correction will be displayed on the chart. Lines for the regression and mean of the values are also displayed. Remember, drift correction only happens when **both** the p-value and F statistic are significant. To change the alpha value of the p-value used in determining significance you may adjust the value in the input area of the “Concentrations” tab that says “Drift significance threshold”. If this change in value changes whether or not an analyte is drift corrected, the “Calculated Concentrations” table will update in real time to reflect those changes.

Video Demos

- LaserTRAM video
- LaserTRAM profiler video
- LaserCalc video

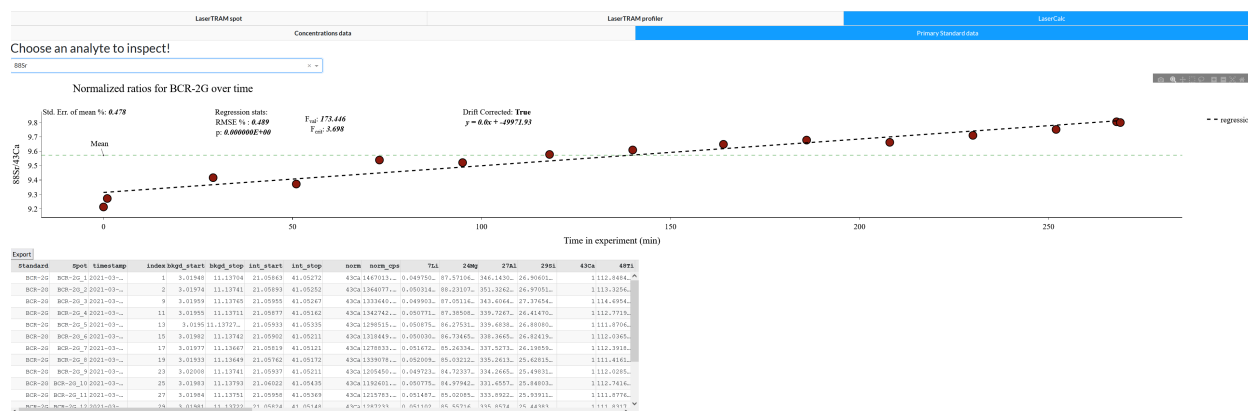


Figure 6: Example of the LaserCalc Primary Standard tab that shows data for the chosen calibration standard both graphically and in a table.

Citing

If you use this software for your research, first off, we hope that it helps bring clarity and efficiency to your LA-ICP-MS data processing life. If there are features you would like to see that are not *totally* unreasonable, please do not hesitate to reach out!

Secondly, we would appreciate that you cite our work accordingly:

- In text: [Lubbers et al. \(2021\)](#)
- bibtex:

```
@misc{lubbers2021lasertram,
author = {
Jordan Lubbers and
Adam Kent and
Russo Chris
},
title = {LaserTRAM-DB},
month = {10},
year = {2021},
doi = {10.5281/zenodo.5620857},
url = {https://github.com/jlubbersgeo/laserTRAM-DB}
}
```

Acknowledgements

We express our gratitude to the W.M. Keck Foundation for helping foster the laboratory environment that led to the genesis of this software, the open-source coding community for developing the tools that made this all possible, and NSF project grants 1763639, 1948862, 1654275.

References

- O. Branson, J. S. Fehrenbacher, L. Vetter, A. Y. Sadekov, S. M. Eggins, and H. J. Spero. Latools: A data analysis package for the reproducible reduction of la-icpms data. *Chemical Geology*, 504:83–95, 2019. doi: 10.1016/j.chemgeo.2018.10.029.
- L. Caricchi, M. Petrelli, E. Bali, T. Sheldrake, L. Pioli, and G. Simpson. A data driven approach to investigate the chemical variability of clinopyroxenes from the 2014–2015 holuhraun–bárdarbunga eruption (iceland). *Frontiers in Earth Science*, 8:18, 2020. doi: 10.3389/feart.2020.00018.
- T. Fritz-Endres and J. Fehrenbacher. Preferential loss of high trace element bearing inner calcite in foraminifera during physical and chemical cleaning. *Geochemistry, Geophysics, Geosystems*, 22(1):e2020GC009419, 2021. doi: 10.1029/2020gc009419.
- M. Guillon, D. L. Meier, M. M. Allan, C. A. Heinrich, and B. W. Yardley. Appendix a6: Sills: A matlab-based program for the reduction of laser ablation icp-ms data of homogeneous materials and inclusions. *Mineralogical Association of Canada Short Course*, 40:328–333, 2008.
- C. R. Harris, K. J. Millman, S. J. van der Walt, R. Gommers, P. Virtanen, D. Cournapeau, E. Wieser, J. Taylor, S. Berg, N. J. Smith, et al. Array programming with numpy. *Nature*, 585(7825):357–362, 2020. doi: 10.1038/s41586-020-2649-2.
- A. J. Kent and C. Ungerer. Analysis of light lithophile elements (li, be, b) by laser ablation icp-ms: Comparison between magnetic sector and quadrupole icp-ms. *American Mineralogist*, 91(8-9):1401–1411, 2006. doi: 10.2138/am.2006.2030.
- M. W. Loewen and A. J. Kent. Sources of elemental fractionation and uncertainty during the analysis of semi-volatile metals in silicate glasses using la-icp-ms. *Journal of Analytical Atomic Spectrometry*, 27(9):1502–1508, 2012. doi: 10.1039/c2ja30075c.
- H. P. Longerich, S. E. Jackson, and D. Günther. Inter-laboratory note. laser ablation inductively coupled plasma mass spectrometric transient signal data acquisition and analyte concentration calculation. *Journal of analytical atomic spectrometry*, 11(9):899–904, 1996. doi: 10.1039/ja9961100899.
- J. Lubbers, A. Kent, and R. Chris. Lasertram-db, 10 2021. URL <https://github.com/jlubbersgeo/laserTRAM-DB>.
- R. Lukács, L. Caricchi, A. K. Schmitt, O. Bachmann, O. Karakas, M. Guillon, K. Molnár, I. Seghedi, and S. Harangi. Zircon geochronology suggests a long-living and active magmatic system beneath the ciomadul volcanic dome field (eastern-central europe). *Earth and Planetary Science Letters*, 565:116965, 2021. doi: 10.1016/j.epsl.2021.116965.
- W. McKinney et al. Data structures for statistical computing in python. In *Proceedings of the 9th Python in Science Conference*, volume 445, pages 51–56. Austin, TX, 2010. doi: 10.25080/majora-92bf1922-00a.
- S. A. Mischel, R. Mertz-Kraus, K. P. Jochum, and D. Scholz. Termite: An r script for fast reduction of laser ablation inductively coupled plasma mass spectrometry data and its application to trace element measurements. *Rapid Communications in Mass Spectrometry*, 31(13):1079–1087, 2017. doi: 10.1002/rcm.7895.
- C. Paton, J. Hellstrom, B. Paul, J. Woodhead, and J. Hergt. Lolite: Freeware for the visualisation and processing of mass spectrometric data. *Journal of Analytical Atomic Spectrometry*, 26(12):2508–2518, 2011. doi: 10.1039/c1ja10172b.
- J. Taylor. *Introduction to error analysis, the study of uncertainties in physical measurements*. 1997.