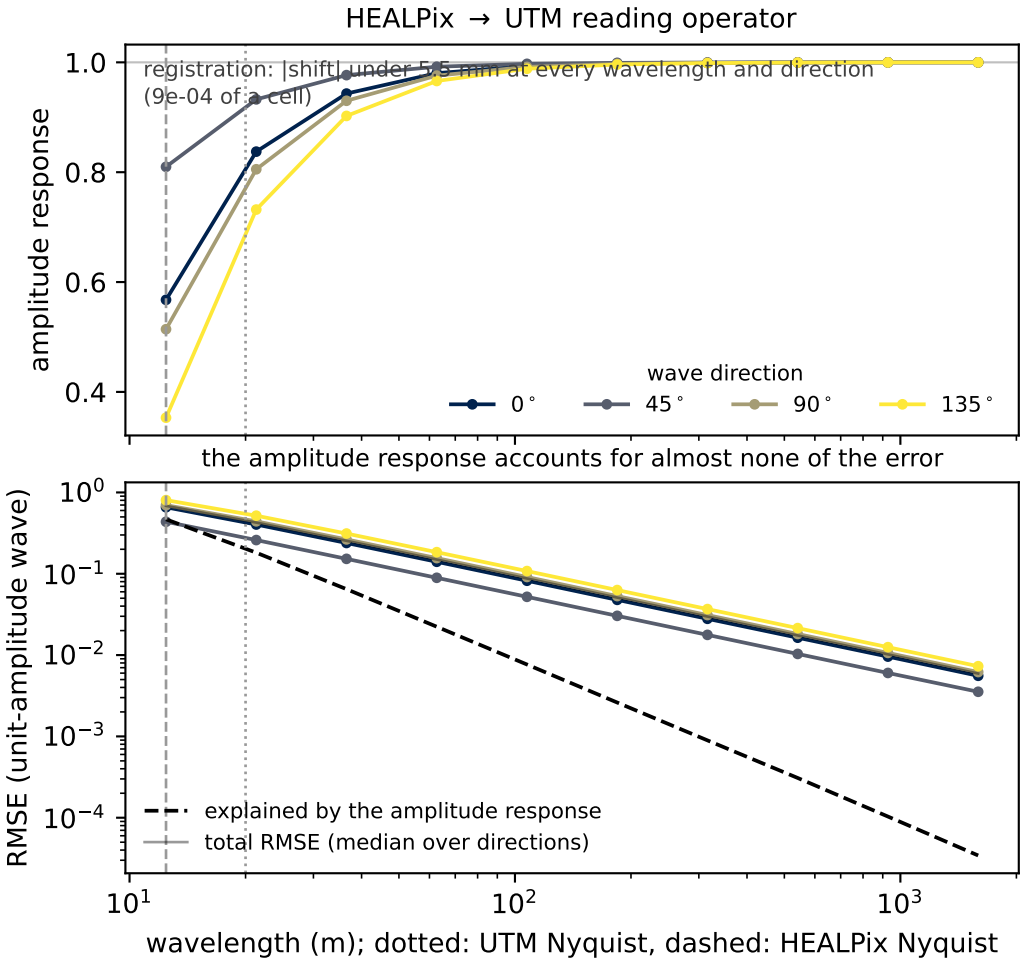
HEALPix → UTM reading operator
registration: |shift| under 5.5 mm at every wavelength and direction
(9e-04 of a cell)
amplitude response
1.0
0.8
0.6
0.4
wave direction
0°
45°
90°
135°
the amplitude response accounts for almost none of the error
RMSE (unit-amplitude wave)
10^{0}
10^{-1}
10^{-2}
10^{-3}
10^{-4}
explained by the amplitude response
total RMSE (median over directions)
10^{1}
10^{2}
10^{3}
wavelength (m); dotted: UTM Nyquist, dashed: HEALPix Nyquist