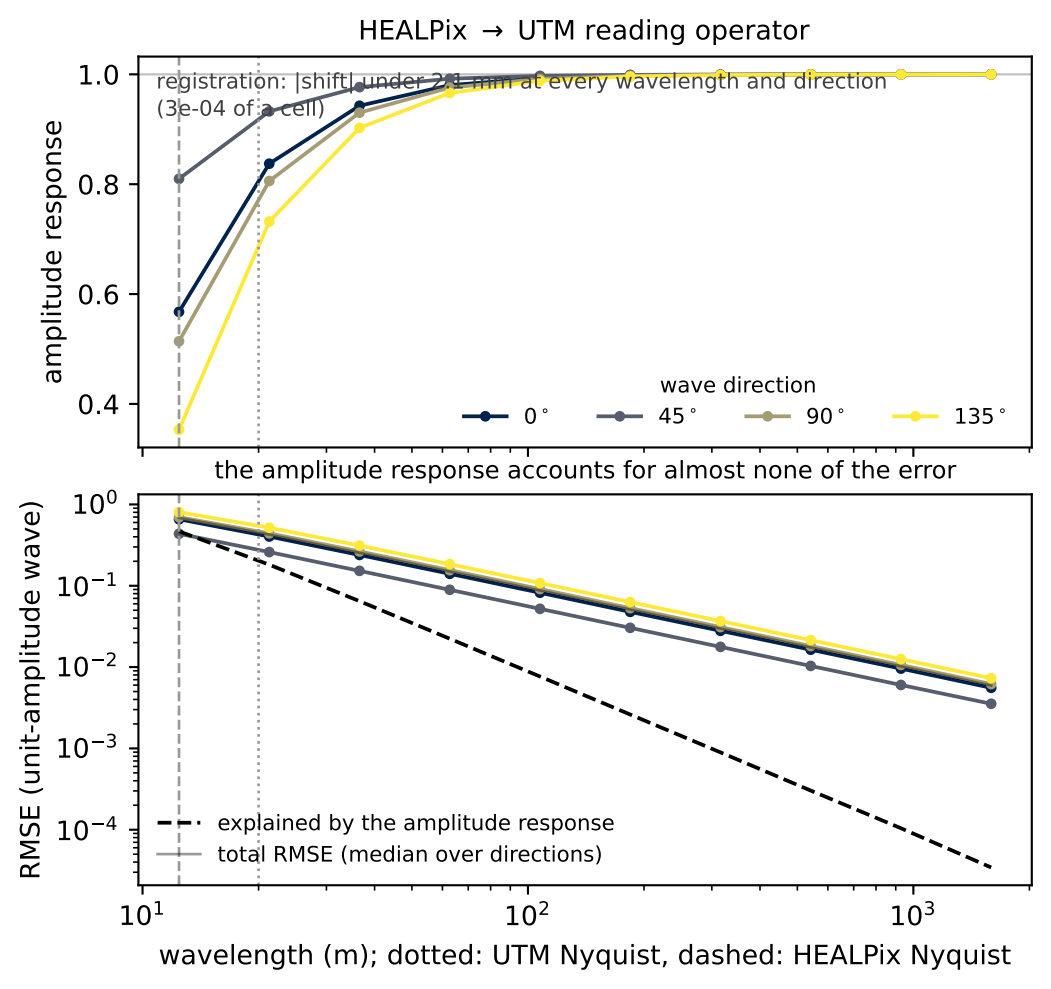
HEALPix → UTM reading operator
registration: |shift| under 2.1 mm at every wavelength and direction
(3e-04 of a cell)
amplitude response
1.0
0.8
0.6
0.4
wave direction
0°
45°
90°
135°
the amplitude response accounts for almost none of the error
RMSE (unit-amplitude wave)
explained by the amplitude response
total RMSE (median over directions)
wavelength (m); dotted: UTM Nyquist, dashed: HEALPix Nyquist