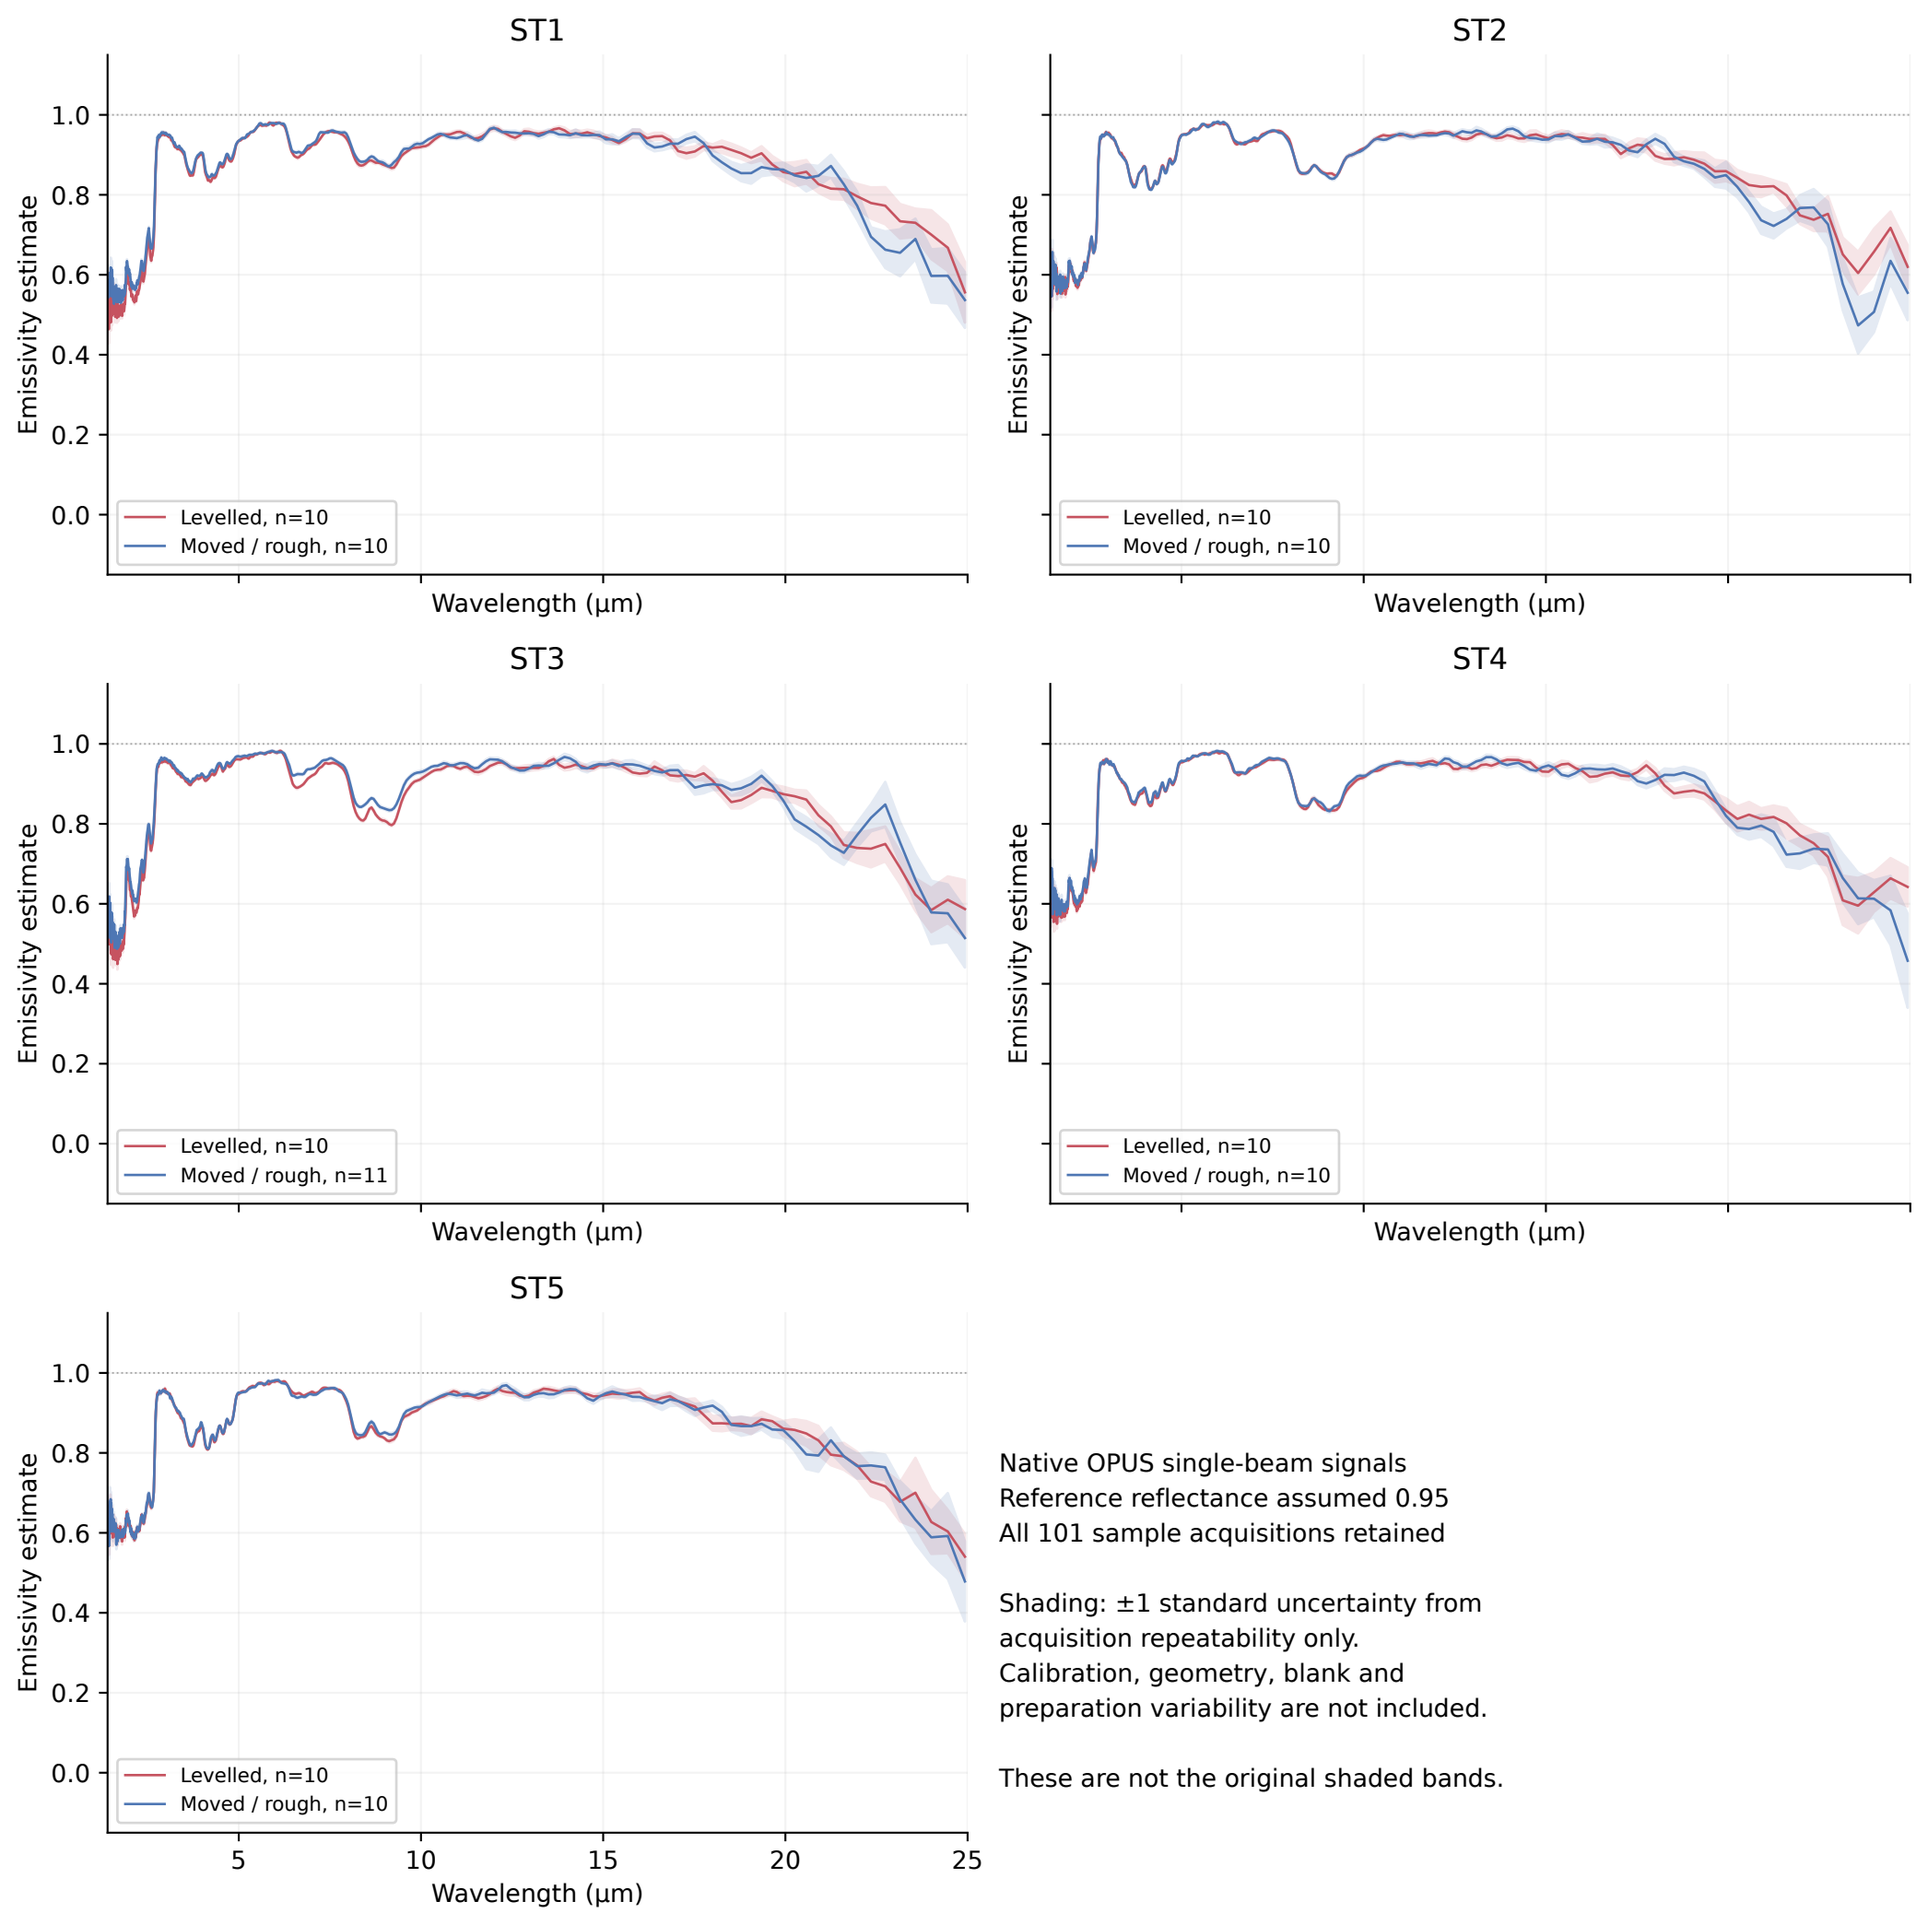


Native OPUS single-beam signals
Reference reflectance assumed 0.95
All 101 sample acquisitions retained

Shading: ±1 standard uncertainty from acquisition repeatability only.
Calibration, geometry, blank and preparation variability are not included.

These are not the original shaded bands.