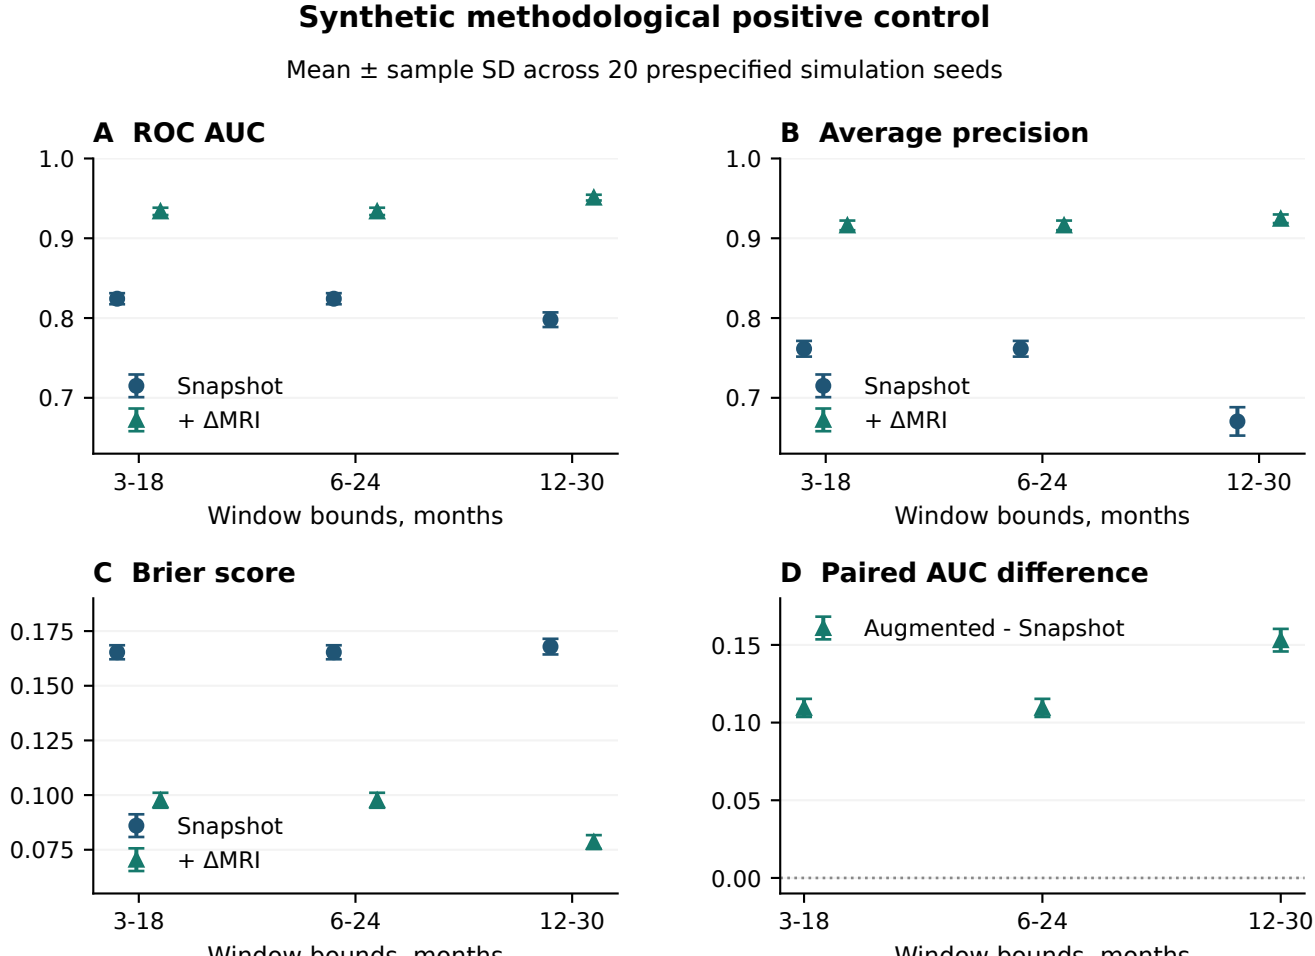
Synthetic methodological positive control
Mean ± sample SD across 20 prespecified simulation seeds
A ROC AUC
1.0
0.9
0.8
0.7
Snapshot
+ ΔMRI
3-18
6-24
12-30
Window bounds, months
B Average precision
1.0
0.9
0.8
0.7
Snapshot
+ ΔMRI
3-18
6-24
12-30
Window bounds, months
C Brier score
0.175
0.150
0.125
0.100
0.075
Snapshot
+ ΔMRI
3-18
6-24
12-30
Window bounds, months
D Paired AUC difference
Augmented - Snapshot
0.15
0.10
0.05
0.00
3-18
6-24
12-30
Window bounds, months
Shorter bounds: identical scans; longer bounds: different eligible participants.
SD is simulation variability, not a confidence interval.