

Imager Quality Analysis

Department: South Bay Radiation Oncology

Machine Name: SB-LA-1

Data Acquired: 1/20/2022

Vendor: Varian

Data Analyzed: 1/21/2022

Model: Truebeam

Serial #: - -

Quick Select: SB_LA1_CBCT_Head • Imager: Varian OBI • Energy: NA

Phantom: Catphan504-SB-Head • Phantom Template: Catphan 504 • Phantom Serial #:1924

Summary

Result category	Results summary
Uniformity And Noise	One or more results in alert range
HU Constancy	One or more results in alert range
Spatial Resolution	One or more results in alert range
Geometric Distortion	One or more results in alert range
Slice Thickness	All results in acceptable range
Low Contrast Visibility	One or more results in error range
Low Contrast Detectability	One or more results in error range



Machine Name: SB-LA-1

Vendor: Varian

Model: Truebeam

Serial #: - -

Data Acquired: 1/20/2022

Data Analyzed: 1/21/2022

Quick Select: SB_LA1_CBCT_Head • Imager: Varian OBI • Energy: NA



Phantom: Catphan504-SB-Head • Phantom Template: Catphan 504 • Phantom Serial #:1924

Uniformity and Noise

ROI	CT # Uniformity	Image Noise
1	27.298	32.359
2	15.032	28.064
3	14.020	29.786
4	16.117	28.039
5	14.407	27.215

Integral non-uniformity

Vertical	Horizontal
2.949	2.897

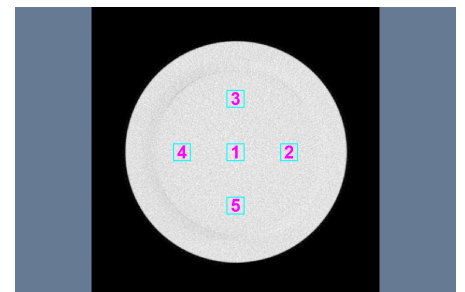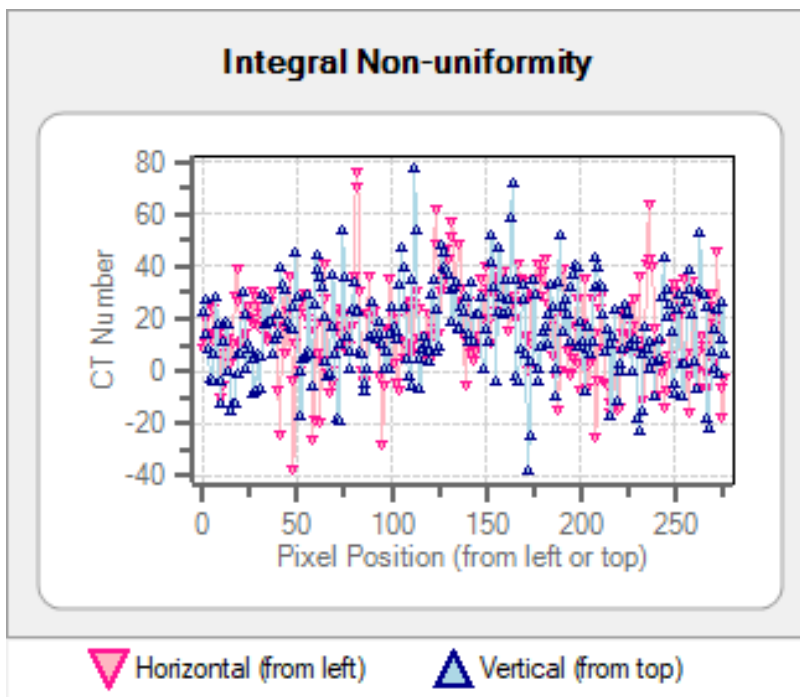

1.2.246.352.62.2.4810492057
1/20/2022 5:03:58 PM



Machine Name: SB-LA-1

Vendor: Varian

Model: Truebeam

Serial #: - -

Data Acquired: 1/20/2022

Data Analyzed: 1/21/2022


Quick Select: SB_LA1_CBCT_Head • Imager: Varian OBI • Energy: NA

Phantom: Catphan504-SB-Head • Phantom Template: Catphan 504 • Phantom Serial #:1924


HU Constancy

ID	Material	Measured (HU)	Expected (HU)
1	Air	-996.526	-1000.000
2	PMP	-191.092	-200.000
3	LDPE	-99.500	-100.000
4	Polystyrene	-36.082	-35.000
5	Air	-998.041	-1000.000
6	Acrylic	129.786	120.000
7	Delrin	377.281	340.000
8	Teflon	1019.811	990.000

Measured vs Expected

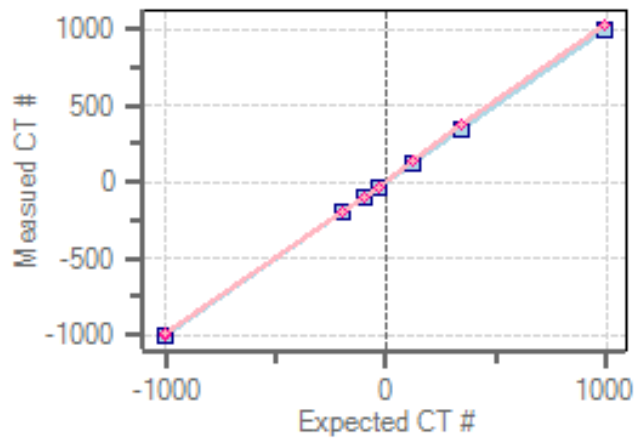

Measured Perfect (measured = expected)

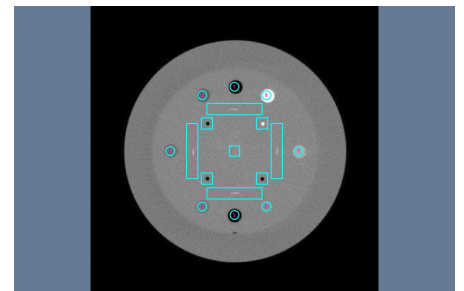

1.2.246.352.62.2.4810492057
1/20/2022 5:03:58 PM



Machine Name: SB-LA-1

Data Acquired: 1/20/2022

Vendor: Varian

Data Analyzed: 1/21/2022

Model: Truebeam



Serial #: - -

Quick Select: SB_LA1_CBCT_Head • Imager: Varian OBI • Energy: NA

Phantom: Catphan504-SB-Head • Phantom Template: Catphan 504 • Phantom Serial #:1924

Spatial Resolution

F50 (lp/mm)	F40 (lp/mm)	F30 (lp/mm)
0.460	0.520	0.592

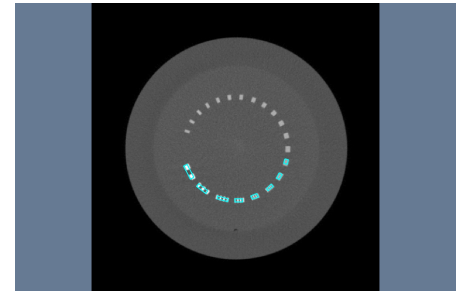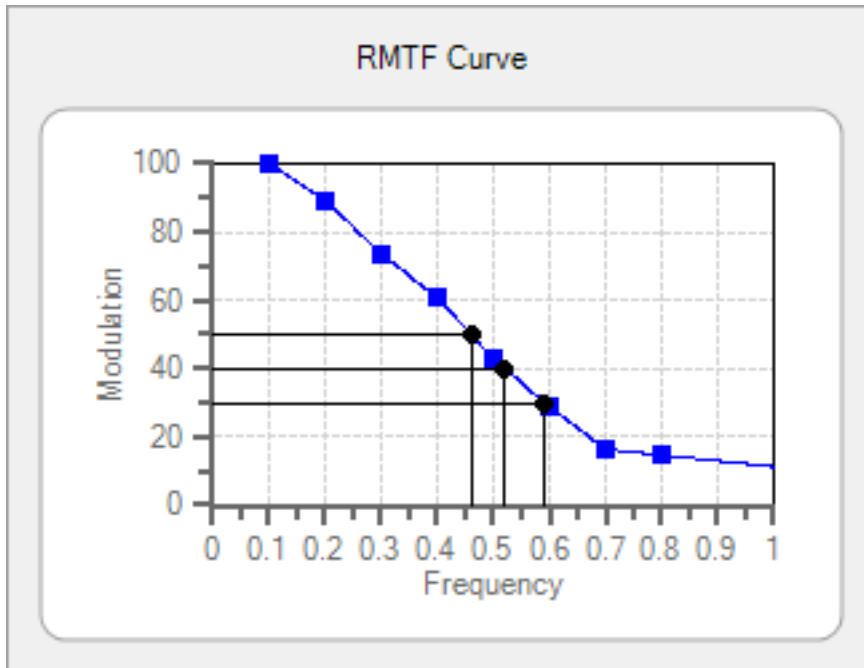

1.2.246.352.62.2.4810492057
1/20/2022 5:03:58 PM



Machine Name: SB-LA-1

Vendor: Varian

Model: Truebeam

Serial #: - -

Data Acquired: 1/20/2022


Data Analyzed: 1/21/2022

Quick Select: SB_LA1_CBCT_Head • Imager: Varian OBI • Energy: NA

Phantom: Catphan504-SB-Head • Phantom Template: Catphan 504 • Phantom Serial #:1924

Geometric Distortion

Position 1	Position 2	Measured distance	Expected distance
Bottom Left	Bottom Right	50.097	50.000
Bottom Right	Top Right	50.097	50.000
Top Right	Top Left	50.099	50.000
Top Left	Bottom Left	50.608	50.000

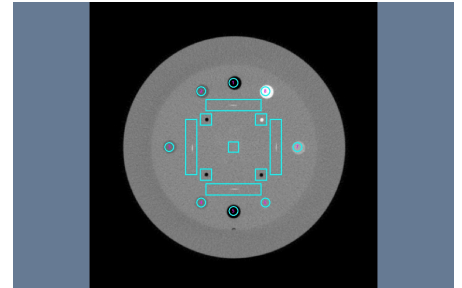

1.2.246.352.62.2.4810492057
1/20/2022 5:03:58 PM

Slice Thickness

Bar	Calculated Thickness (mm)	Expected Thickness (mm)
Bottom	1.874	1.990
Right	1.874	1.990
Top	1.978	1.990
Left	2.083	1.990
Mean	1.953	1.990

Low Contrast Visibility

Material 1	Material 2	LCV
Polystyrene	LDPE	2.709



Machine Name: SB-LA-1

Vendor: Varian

Model: Truebeam

Serial #: - -

Data Acquired: 1/20/2022



Data Analyzed: 1/21/2022

Quick Select: SB_LA1_CBCT_Head • Imager: Varian OBI • Energy: NA

Phantom: Catphan504-SB-Head • Phantom Template: Catphan 504 • Phantom Serial #:1924

Low Contrast Detectability

Contrast Level	Lowest Detected (mm)	Percent Detected	C x D (of Low Detected)
0.3	--	0.0	--
0.5	--	0.0	--
1.0	9.0	22.2	56.7

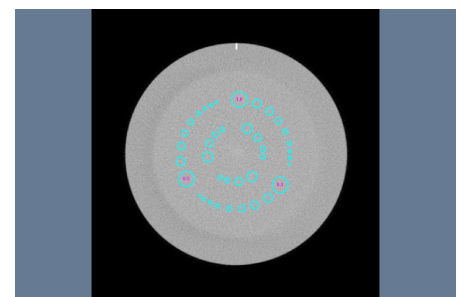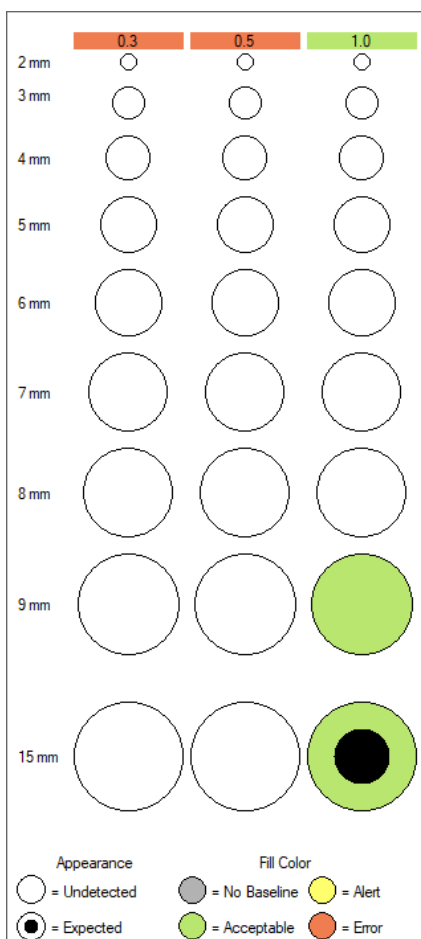

1.2.246.352.62.2.4810492057
1/20/2022 5:03:58 PM

