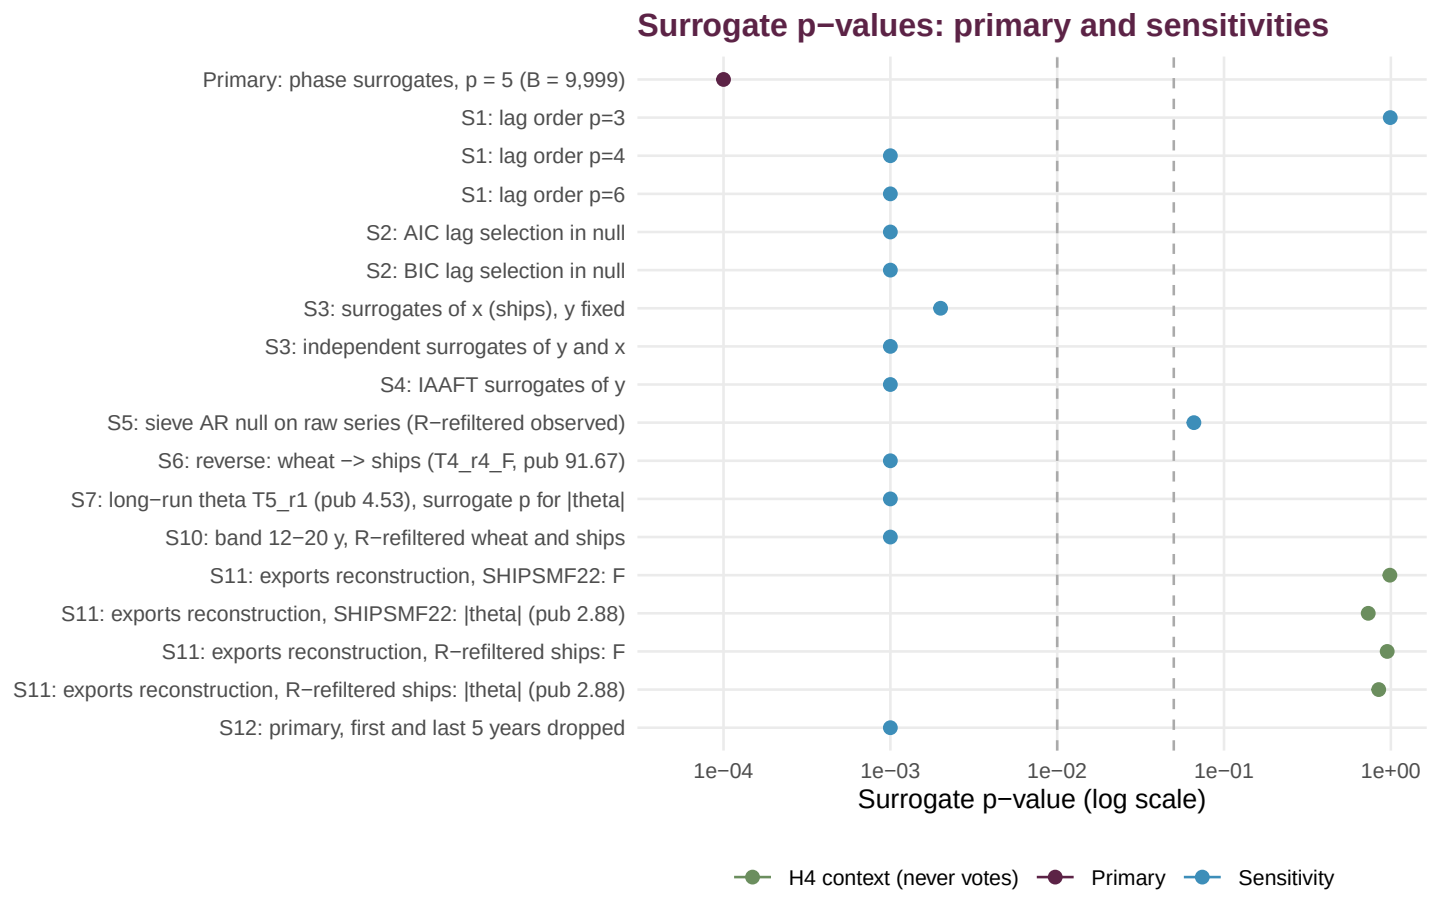

Calibration (report−only): the B = 199 surrogate test rejects in about 47% of independent−series replications at 1%.