

Oralable Research Kit — status for Pedro

To: Dr Pedro Mayoral Sanz (Beacon) · cc Dr Edward Owens
From: John A. Cogan (JAC / Oralable)
As at: 7 Aug 2026 · Meeting today 16:00

Honest status. What we measured and built — not a wish list.
Ready ≠ delivered. Kits still gated on charge-to-temple.

Where we are

- Ship stack: Gen1 hardware · firmware **1.0.70** · patient app **4.3.3** (temple HR + SpO₂).
- Mac Protocol A + overnight report ran on engineering pack TEMPORALIS_20260724. Wear **~6 minutes** — layout / Core ML only. Not a ≥6 h overnight.
- Dual Protocol A on Mac (Oralable + ANR M40, shared cues) is scripted for labeled concordance.
- Partner kits **not yet shipped** until each unit passes charge-to-temple.

Oralable Research Kit

IN THE KIT	ROLE
Oralable MAM (clip + magnetic case / dock)	Optical PPG/ACC · vitals now · jaw-load path on same HW
ANR M40 + 3M Red Dot	Temporalis sEMG comparator (Dual Protocol A on Mac)
Headband (optional)	Long-wear compression for Dual A
iOS Oralable (TestFlight)	1–6 h+ BLE collection

IEEE Paper A (with Koorosh Nabavi / McGill): ≈5 Beacon · your 1–2 h oxygen / MAD arm · stretch ≥6 h. Landscape vs Bruxoff / AcuPebble / GrindCare. No AHI claims. Oralable does not replace AcuPebble AHI.

Commitment

Target: **5 Research Kits to you by 31 August 2026**, each past the charge-to-temple gate. If ANR stock is short, I will say so and ship Oralable first with ANR to follow.

Asks for our 16:00 meeting

1. Beacon ethics / consent path name + next filing step.
2. First calendar window for dry-run + Arm P (1–2 h ± MAD log).
3. Authorship / Beacon affiliation line for Paper A (with Ed + Koorosh).
4. Bruxoff access for descriptive EMG reference?
5. AcuPebble photo or SKU (SA100 vs Ox100) if easy.
6. Optional: interest in short F&F investor leave-behind.

Line drawings — kit & wear (partner-safe)

Matisse contour line figures from research photos (same craft as Dual A stack). Not patent claim text. Not clinical diagnosis figures.

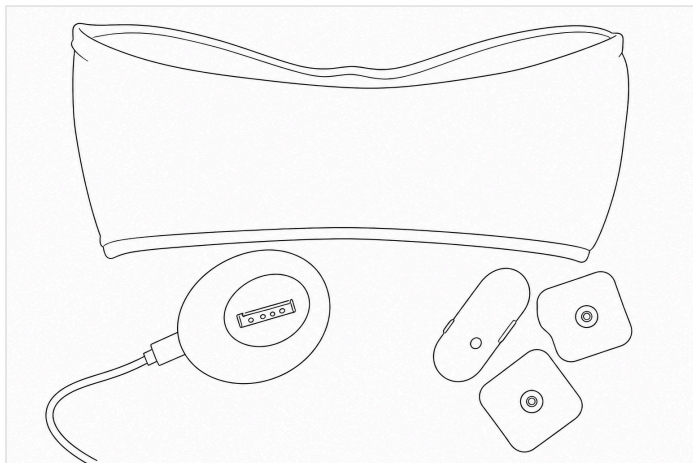


FIG-CO-049 — Research Kit flat-lay (Matisse contour craft): headband · charge dock · ANR · Red Dots.

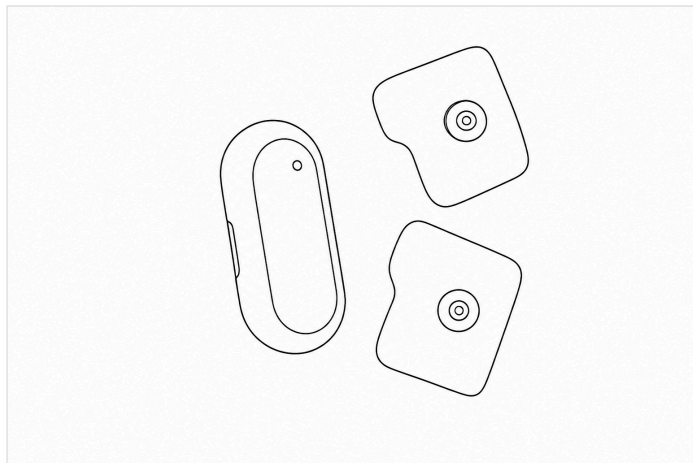


FIG-CO-047 — ANR Muscle Sense + Red Dot pads (Matisse contour craft).

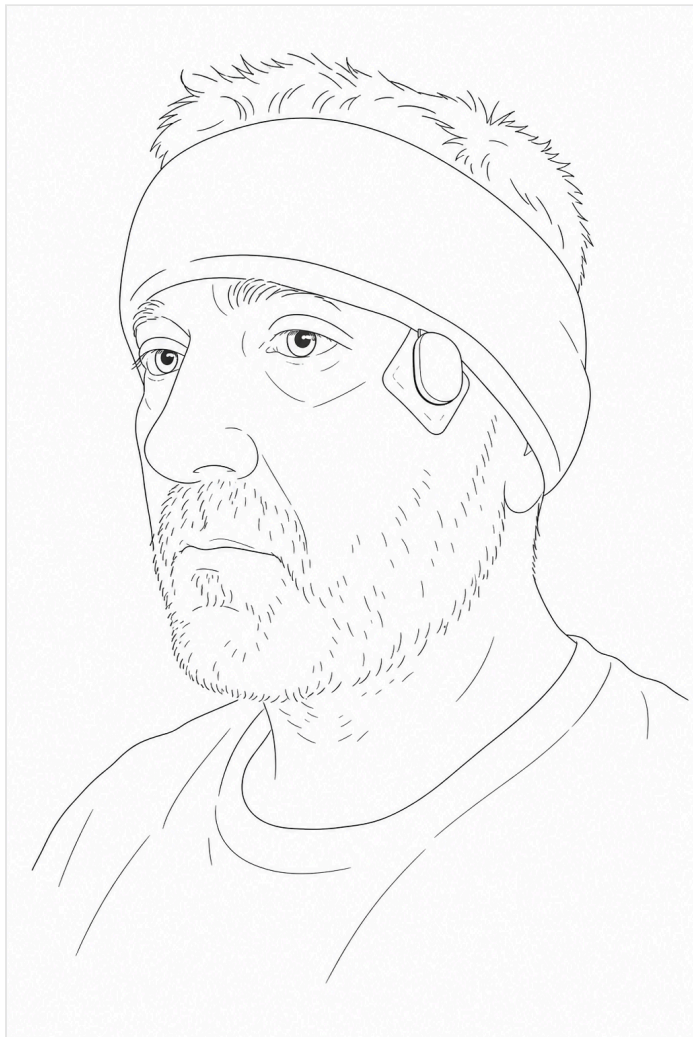


FIG-CO-044 — Worn Dual A: headband + temple sensor (Matisse contour craft).

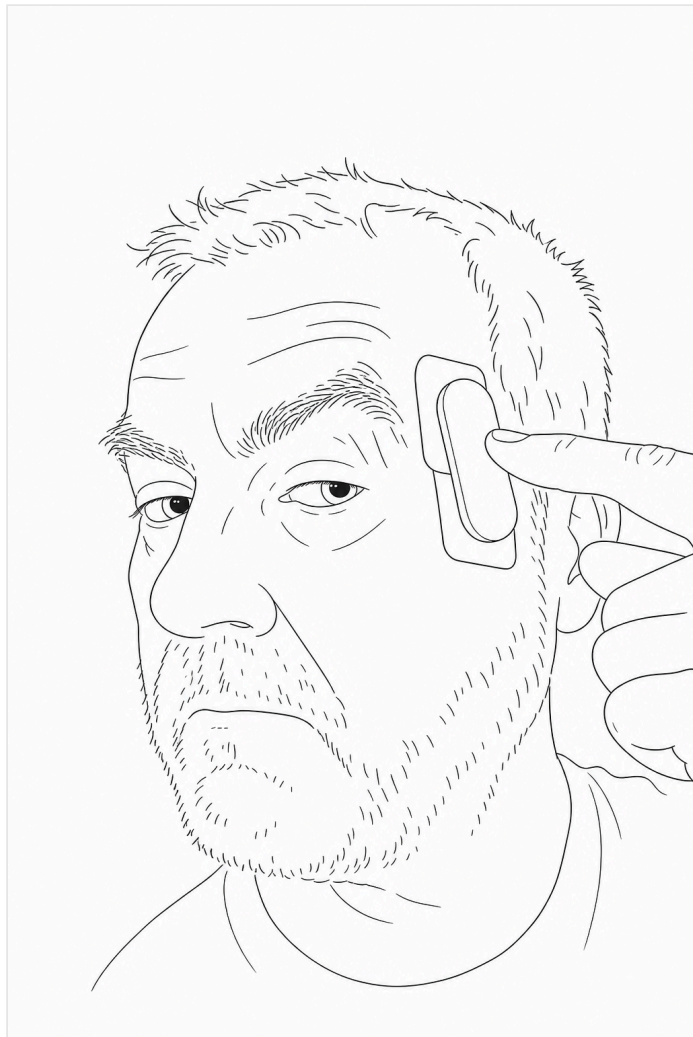


FIG-CO-045 — Temple placement gesture (Matisse contour craft).

IP note (pitch-safe)

US provisional **64/033,978** filed 9 Apr 2026 — *Apparatus and Method for Muscle Activity Monitoring* · **patent pending**.
Do not circulate provisional claim text or the full specification PDF.