


# Fresh TLS scaling measurements

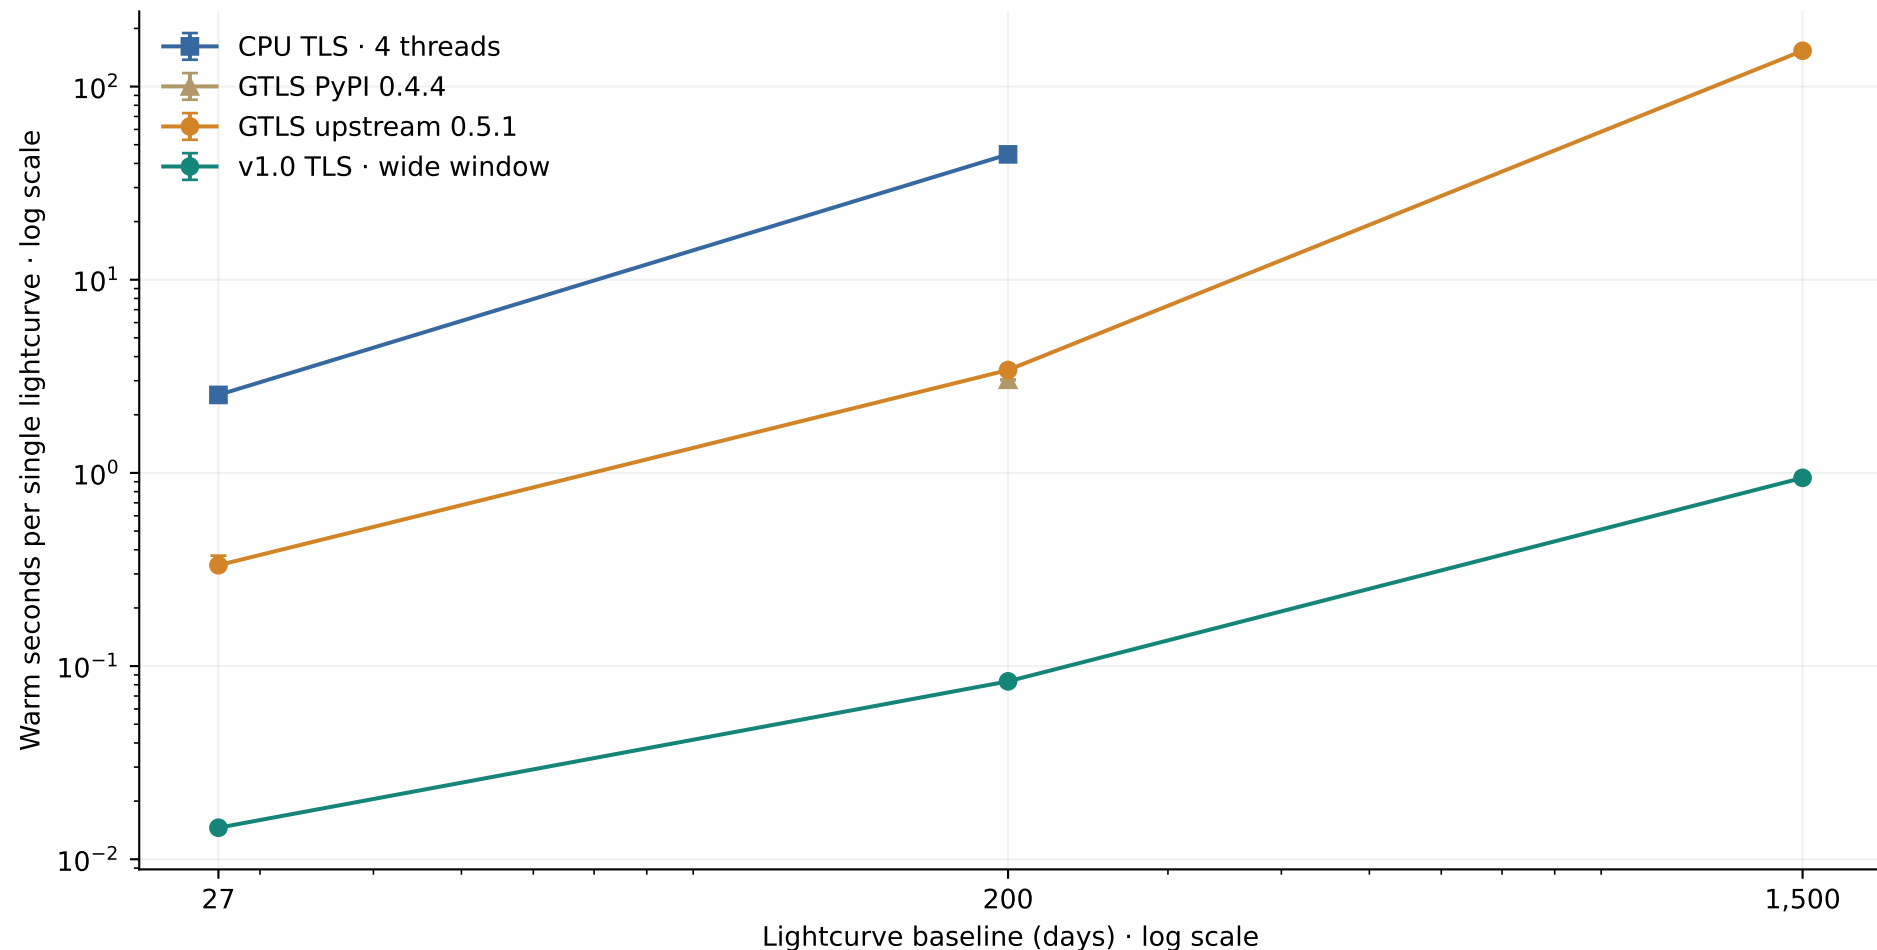

A40 / Xeon Gold 6342. Identical input arrays and period grids; differing templates and effective duration/epoch grids.  
Median of 3 with observed range. Unmeasured/invalid results omitted: CPU and PyPI GTLS at 1,500 d; invalid PyPI GTLS at 27 d.  
Every displayed run recovered this injection within 0.2% in period. One injection per baseline does not establish sensitivity parity.