

Shake Machines: Taylor HT C602

Syrup Calibration Check/Draw Temperature

Frequency

Syrup check - Daily Syrup calibration - Weekly

Draw Temperature (finished product) - Weekly

Models

Taylor HT C602

Estimated Time to Complete

15 Minutes

Health & Safety Hazards

Food Safety



Wash and dry hands **before and after** performing this task




Ensure nuts, bolts & screws are tight

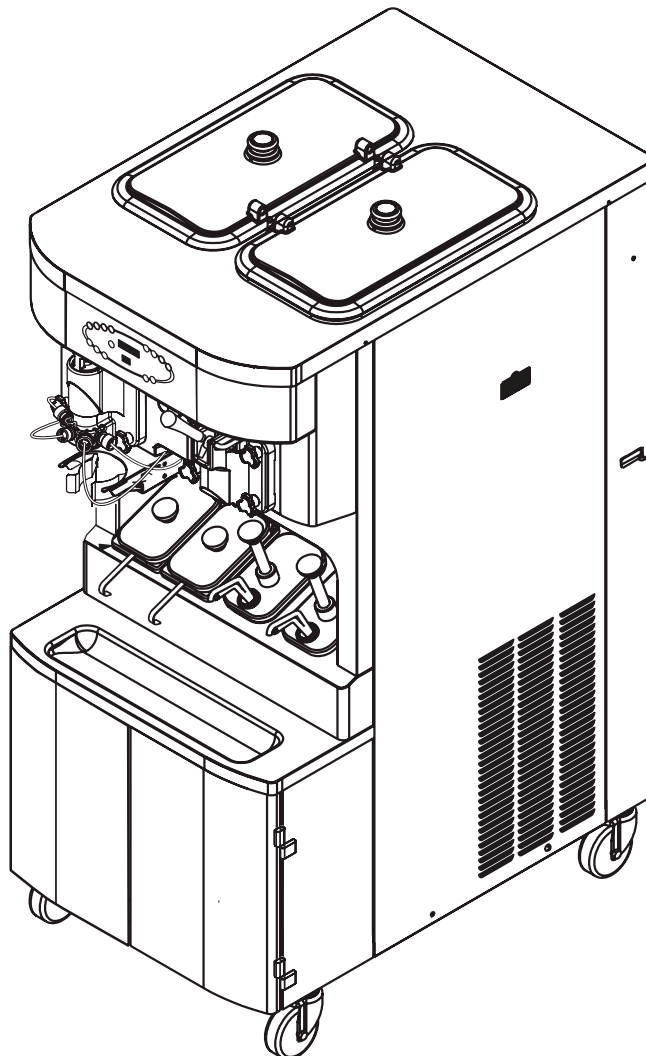


Inspect equipment. Do not use if damaged

Equipment



- 1 Pyrometer & Needle Probe
- 2 Ratio Cup
- 3 White Bucket



1**Syrup Check****14**

ENTER ACCESS CODE



ENTER ACCESS CODE

8 3 0 9



Press the centre of the Cone Symbol. A cursor will be displayed in the LCD screen. Enter the manager code **8309**. To do this, use the AUTO or OPTIONAL FLAVOUR symbols to scroll through until the correct number appears, then press the CALIBRATION symbol to move the cursor to the next number to be entered. Continue until all numbers have been entered correctly. Press the CALIBRATION symbol again to confirm the manager code.

15

EXIT FROM MENU
SYRUP CALIBRATION
VERIFY CALIBRATION
RESET DRAW COUNTER

The screen will display the menu options.

16


> SYRUP CALIBRATION
VERIFY CALIBRATION
RESET DRAW COUNTER
SET CLOCK




Press the AUTO or OPTIONAL FLAVOUR symbols to scroll the arrow to **SYRUP CALIBRATION**. Press the calibration symbol to enter syrup calibration mode.

17

Scroll the arrow to **SYRUP CALIBRATION**. Press the CALIBRATION symbol to enter calibration mode and 'Select a Flavour'.

18


Disconnect the chocolate syrup valve from the freezer door by raising the retainer pin and pulling the syrup valve out.

19

Place a ratio cup beneath the syrup valve and select the chocolate FLAVOUR symbol.

20

The syrup will automatically be dispensed into the ratio cup. When the syrup amount measures **30ml (1fl oz)** press the chocolate FLAVOUR symbol again to stop syrup flow.

21

Place the ratio cup on a level/stable surface to verify the syrup dispensed is **30ml (1fl oz)**. Cleaning: **NB** Rinse the ratio cup after each time it is used.

22

Press the CALIBRATION symbol to exit **SYRUP CALIBRATION**.

23


EXIT FROM MENU
SYRUP CALIBRATION
> VERIFY CALIBRATION
SET DRAW COUNTER

Press the AUTO or OPTIONAL FLAVOUR symbols to scroll the arrow to **VERIFY CALIBRATION**.


24

VERIFY CALIBRATION
< Select a Flavor
Press to Clear


Press the CALIBRATION symbol to enter **VERIFY CALIBRATION** and 'Select a Flavour'.

25

Place the ratio cup underneath the syrup valve and press the chocolate FLAVOUR symbol. The syrup will automatically be dispensed.

26

Place the ratio cup on a level/stable surface to verify **30ml (1fl oz)** has been dispensed.

27

Insert the syrup valve back into the freezer door and secure using the retainer pin.

28

Press the CALIBRATION symbol to exit.

29

Repeat **steps 16-28** for all other syrup flavours **NB** Cleaning: Rinse the ratio cup after each time it is used.

30

Press the calibration symbol to exit. Press the centre of the cone symbol to exit and return to normal operating mode.



> UNFLAVORED DRAW
SYRUP CALIBRATION
SYRUP PRIME
EXIT



NB If **VERIFY CALBRATION** is incorrect, press the **CALIBRATION** symbol to exit **VERIFY CALIBRATION** and scroll the arrow to **SYRUP CALIBRATION** and repeat syrup calibration procedures followed by **VERIFY CALIBRATION** again.

Draw temperature (finished product) Weekly

31




Press the **CALIBRATION** symbol to enter the menu options.



> UNFLAVORED DRAW
SYRUP CALIBRATION
SYRUP PRIME
EXIT


Press the **AUTO** or **OPTIONAL FLAVOUR** symbols to scroll the arrow to **UNFLAVOURED DRAW**

32




Place a 0.4l cold cup into the cup holder (shake side). Select the flavour symbol to draw a finished shake.

34



Insert the needle probe into the cup and allow the temperature reading to stabilise. The temperature reading should be between -3.3 to -4.4°C .

35



Draw a sundae into the flurry cup, repeat **step 34**. The temperature reading should be between -8 to -9°C .

37



If the Syrup calibration or draw temperature cannot be achieved contact your [Service Company](#).