

Shake Machines: Taylor C602

Cleaning Syrup lines & Replacing Peristaltic pump tube, Duckbill Valve & O-Rings

Frequency

Syrup check - Daily Syrup calibration - Weekly

Draw Temperature (finished product) - Weekly

Models

Taylor C602

Estimated Time to Complete

60 Minutes

Health & Safety Hazards



Chemicals



Slippery Floors / Tripping

Food Safety



Critical Control Point




Ensure nuts, bolts & screws are tight



Inspect equipment. Do not use if damaged



Wash & dry hands **before** and **after** performing task

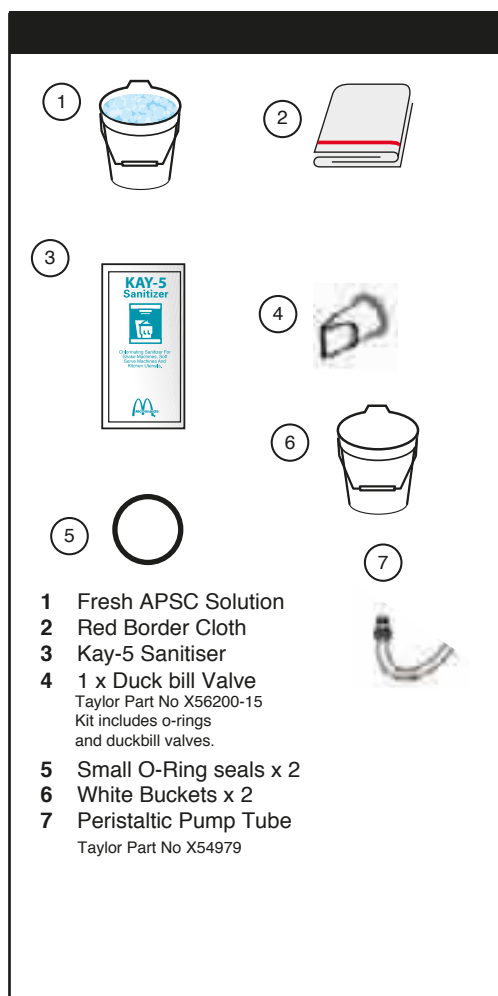

1

Cleaning Syrup Lines

2




Remove syrup suction tube from chocolate syrup pouch and place in a white plastic shake bucket of fresh APSC solution.

2a




3



Pull metal clip up and pull chocolate syrup feed tube nose fitting out of freezer door

4



Place and hold syrup nose fitting inside an empty bucket

5



Press the calibration icon to display menu options

6



Press Blue Up Arrow icon once to select Syrup Prime

7



Press calibration icon to select prime

8



Select and press chocolate syrup icon

9



Chocolate syrup pump will start to flush syrup out of line in to bucket

10



Press press chocolate syrup icon to stop the pump when flow from the line is clean with only warm water being dispensed.

11



Remove chocolate syrup tube from bucket of warm water

12



Now flush out any remaining water in the chocolate syrup line. Press the calibration icon to display menu options

13



Press Blue Up Arrow icon once to select Syrup Prime

14



Press calibration icon to select prime

15



Select and press chocolate syrup icon

16



Press chocolate syrup icon to stop pump when all water has been removed from the chocolate syrup line

17

Repeat steps 2 to 16 inc on all the other syrup lines

18

Replace Peristaltic Pump Tube, Duckbill Valve and O-rings

19



Remove all syrup bags and shelving within syrup cupboard to expose syrup pumps

19a



20



Lift up cover on chocolate syrup pump to expose peristaltic tube inside pump housing

21



Remove peristaltic tube from pump housing

22



Remove plastic clips from both ends to detach peristaltic tube. Install new tube (6 months) and secure clips.

23




Reconnect syrup feed and suction tubes into new Peristaltic tube and refit tube back into pump housing

24




Close pump housing cover

25

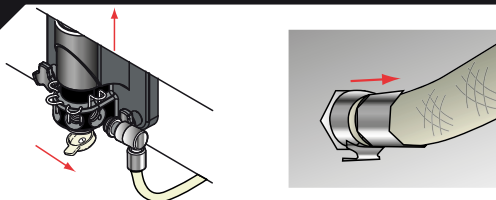


Remove clip and detach nose fitting from door. Press metal tab underneath the QD fitting on the chocolate syrup feed tube, and pull syrup line free.

26

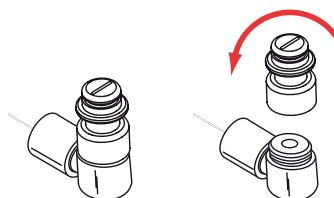


Before reinstalling the Syrup Line Connectors, remove the Syrup Nose Fittings by turning them anti-clockwise.

27



Remove the Duck Bill Valve and O-ring from the Syrup Nose Fittings.

28



Using a Shake Brush, scrub the inside of the Syrup Nose Fitting.

29




Using a sanitised Red Border Cloth, wipe away a sanitised Red Border Cloth wipe away any syrup from the Duck Bill Valves and O-Rings. Replace every three months.

30


Place the Syrup Nose Fittings and Duck Bill Valves in sanitiser for 1-2 minutes.

31

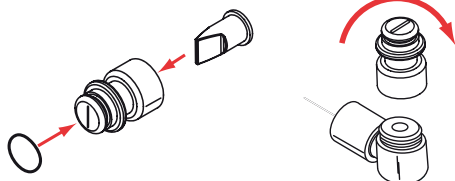

Wearing clear gloves, reinstall the O-rings and Duck Bill Valves into the Syrup Nose Fitting and place back onto the Syrup line fitting by turning it clockwise and hand tighten.

32

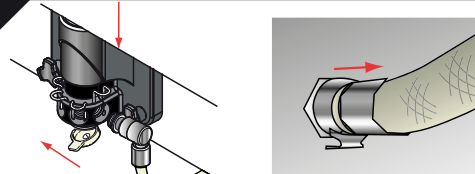

Reconnect the syrup lines into the Quick disconnect fittings on the front panel. Then to syrup port holes on the freezer door and secure with the retainer pins. Refit the restrictor cap.

33

Repeat steps 20-28 on all syrup lines

34

SANITISE THE SYRUP LINES

35



Place chocolate syrup suction tube in white plastic shake bucket of sanitiser solution (1 packet Kay-5 sanitiser in 9.5l luke warm water)

36



UNFLAVORED DRAW
SYRUP CALIBRATION
SYRUP PRIME
> EXIT

Press Calibration icon to select menu options

37



Press Up arrow icon once to select Syrup Prime

38



SYRUP PRIME
Select a Flavor
Press to clear

Press calibration icon to select prime mode

39



Select and press chocolate syrup icon to start sanitising the syrup line

40



Press chocolate syrup icon to stop flow when line is primed and leave sanitiser in line to rest for 5 mins

41



Remove sanitiser suction tube from bucket of sanitiser and connect to chocolate pouch

42

Repeat steps 35-43 inc on all other syrup lines.