



측정 cell (Type 1 → 4b)

selectivity = 0.001
CaseB 우위 321/384 = 83.6%

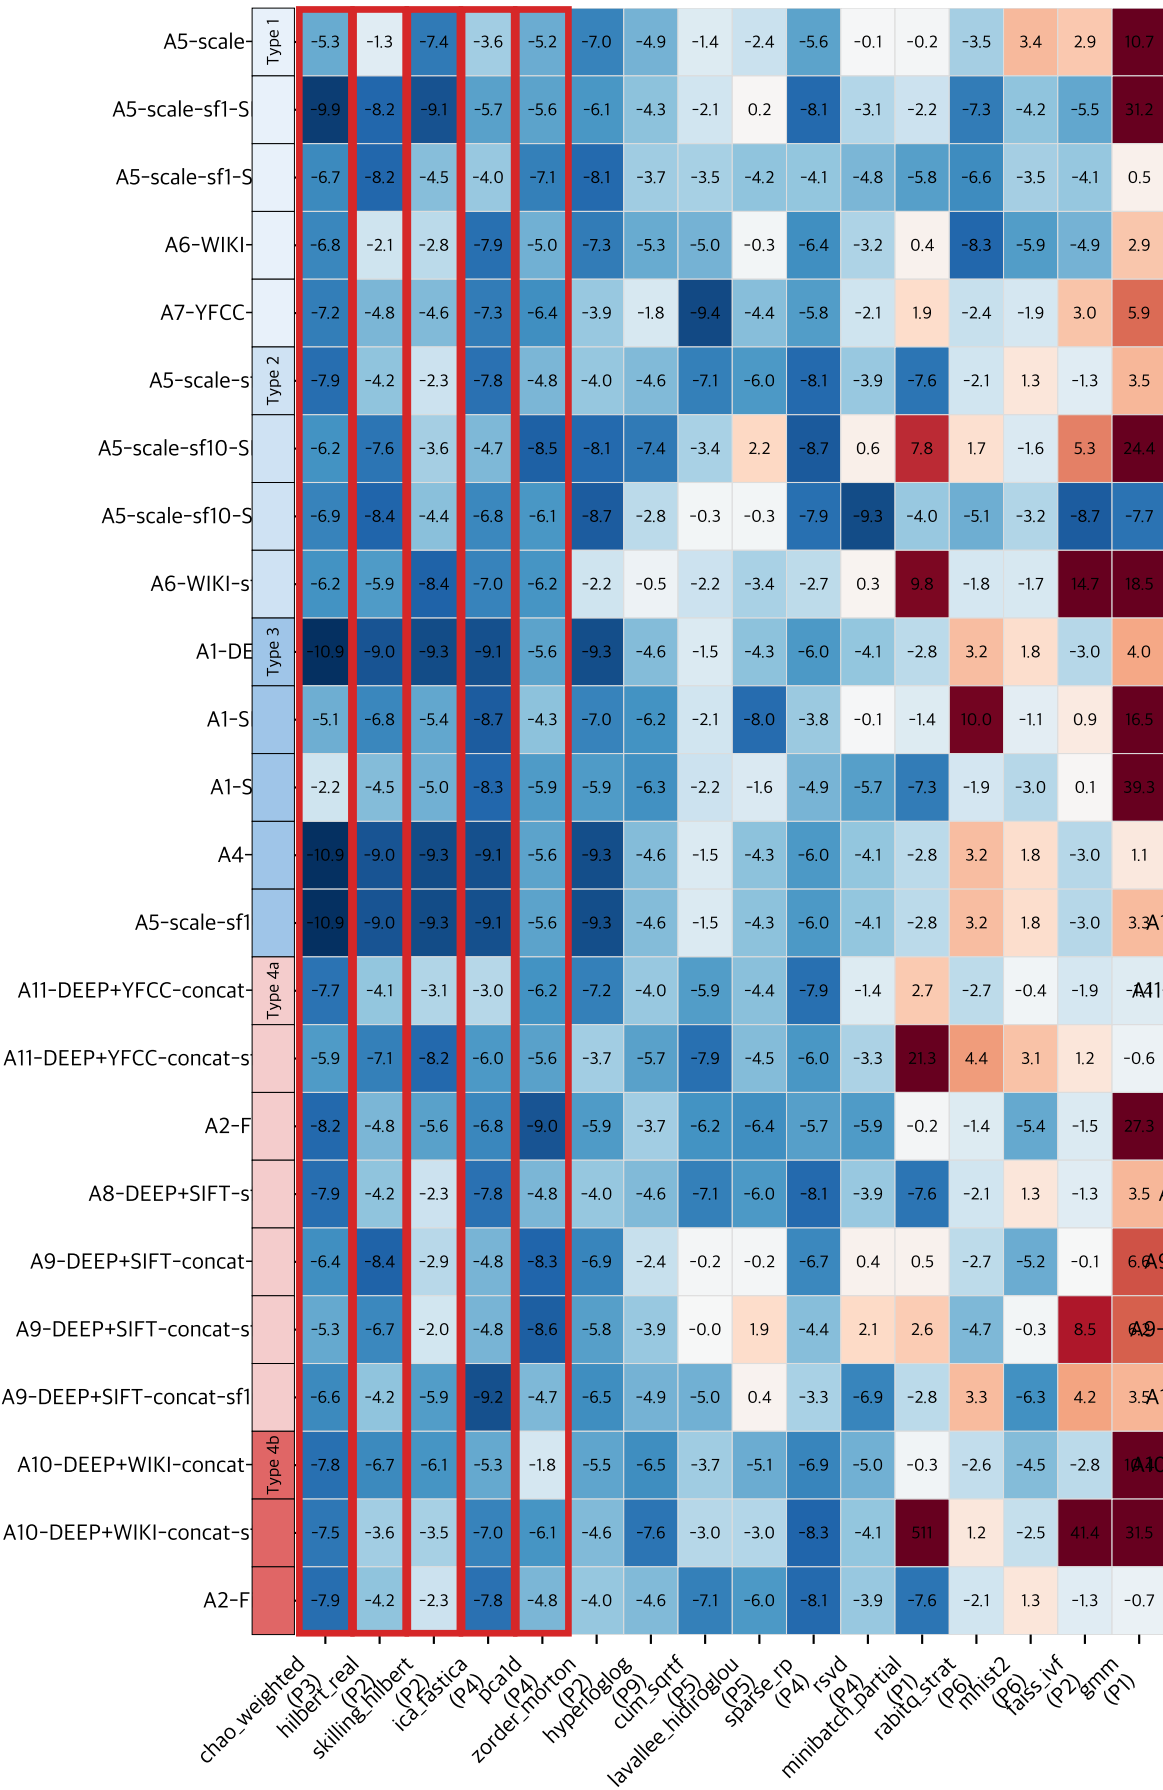


sample selection method (paradigm)

selectivity = 0.01
CaseB 우위 333/372 = 89.5%

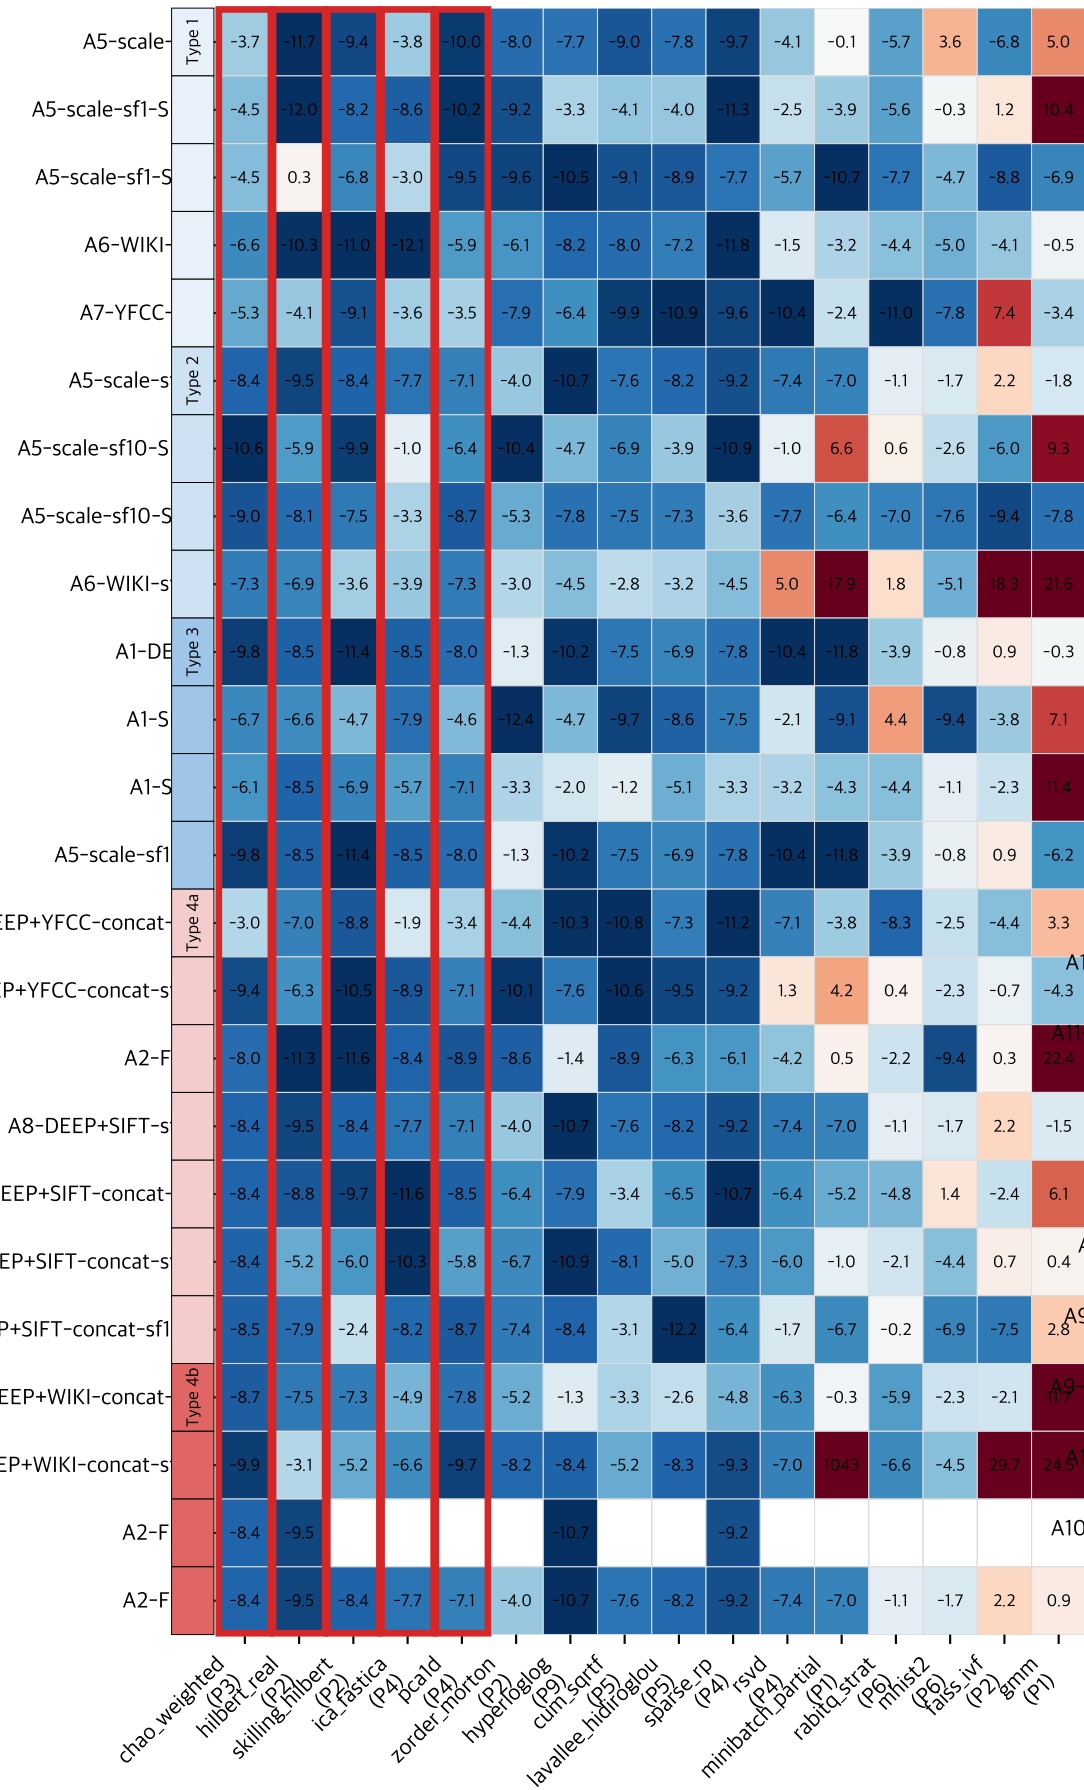

sample selection method (paradigm)

selectivity = 0.1
CaseB 우위 360/368 = 97.8%

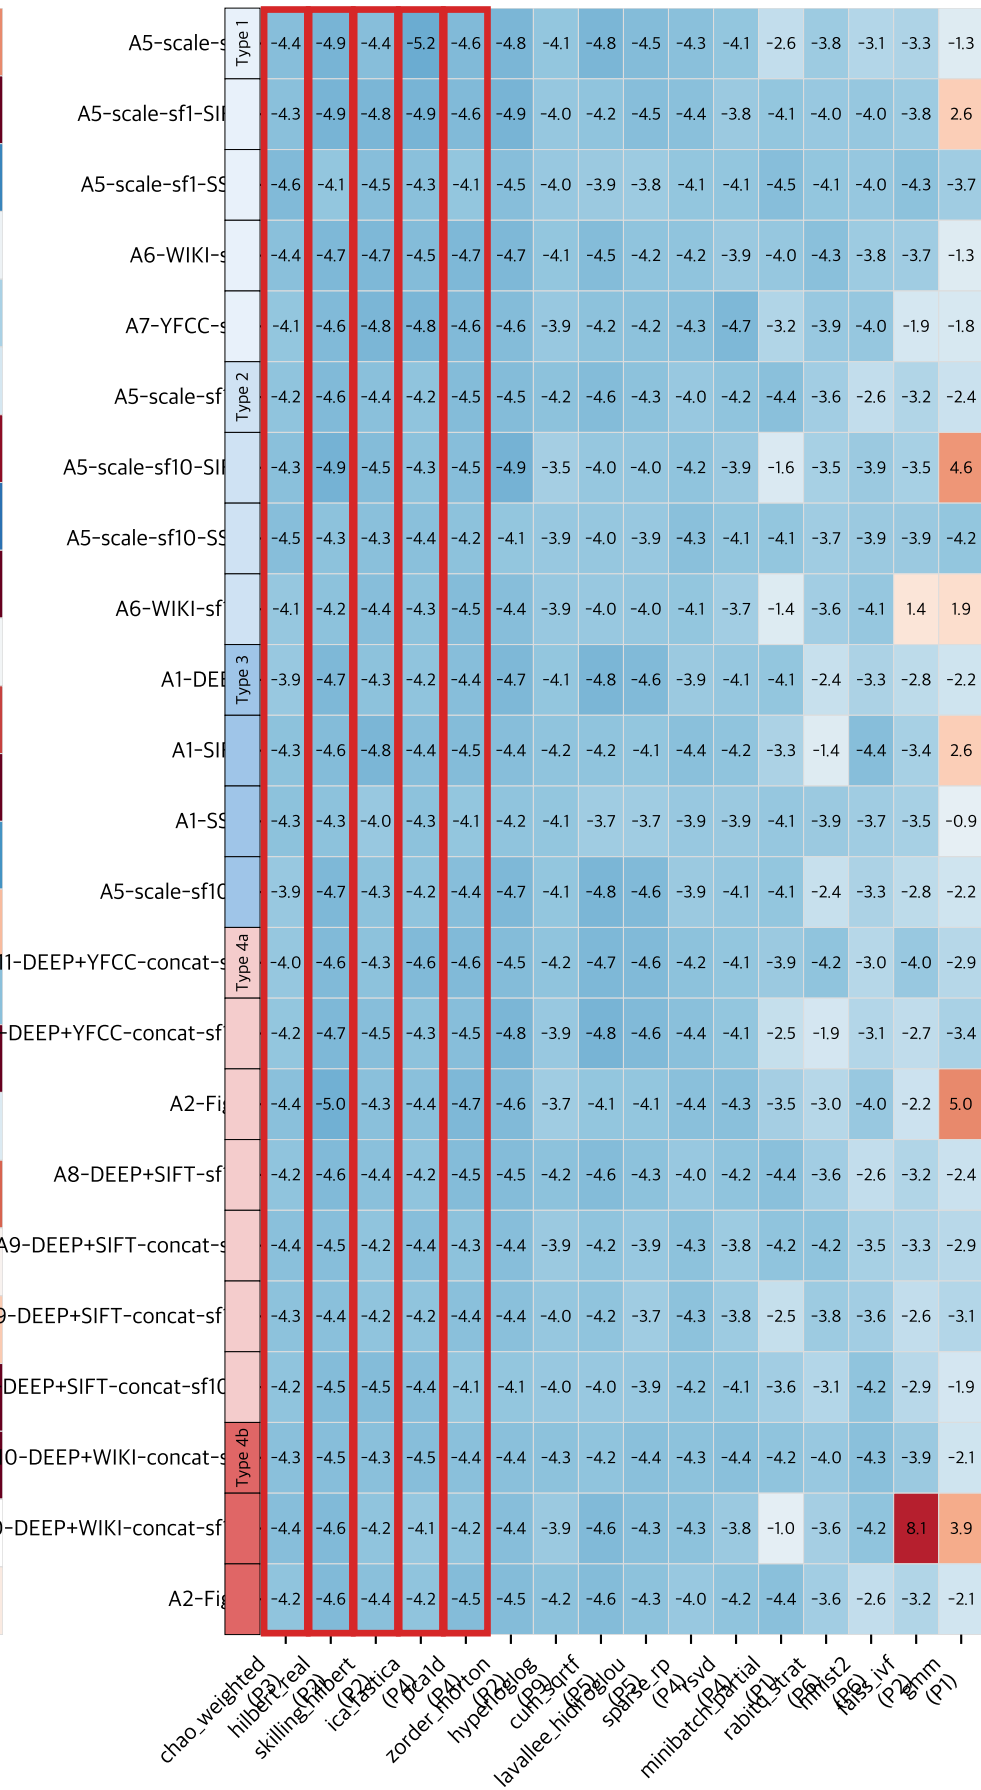

sample selection method (paradigm)

paired Δ% = (CaseB - B1) / B1 × 100
(음수 = 결합 실험군 정확도 개선)