Administrative Data
Institution Samsung Medical Center

Physicist JKH

PatientID 56033983

Patient Name CHANG SANG LYOOL, 104659

Comment

Gamma 2D - Parameters

2.0 mm Distance- To- Agreement
2.0 % Dose difference with ref. to max. dose of calculated volume
Suppress dose below 5.0 % of max. dose of calculated volume
Option "Use 2nd and 3rd pass" selected

Statistics

Number of Dose Points	264
Evaluated Dose Points	89 (33.7 %)
Passed	89 (100.0 %)
Failed	0 (0.0 %)
Result	100.0 % ● (Green)

Gamma 2D


Arithmetic Mean	0.321
Min (LR = 0.0 mm ; TG = 30.0 mm)	0.010
Max (LR = -5.0 mm ; TG = 5.0 mm)	0.927
Median	0.310


Absolute Difference


Arithmetic Mean	0.030	Gy
Min (LR = 0.0 mm ; TG = 30.0 mm)	0.000	Gy
Max (LR = 25.0 mm ; TG = 5.0 mm)	0.103	Ġу
Median	0.022	Gy


Settings

Passing criteria	Gamma ≤ 1.0
Green	90.0 % to 100.0 %
Yellow	75.0 % to 90.0 %
Red	0.0 % to 75.0 %

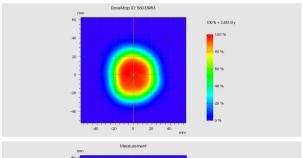



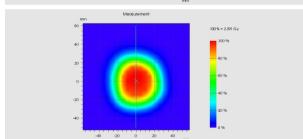



PTW - VeriSoft 7.1 PatientID: 56033983 Patient Name: CHANG SANG LYOOL, 104659 Date: 2025-08-28 00:13:27