Administrative Data

Institution Samsung Medical Center

Physicist JKH

PatientID 56033983

Patient Name CHANG SANG LYOOL, 104659

Comment

Gamma 2D - Parameters

2.0 mm Distance- To- Agreement
2.0 % Dose difference with ref. to max. dose of calculated volume
Suppress dose below 5.0 % of max. dose of calculated volume
Option "Use 2nd and 3rd pass" selected

Statistics

Number of Dose Points	230
Evaluated Dose Points	81 (35.2 %)
Passed	80 (98.8 %)
Failed	1 (1.2 %)
Result	98.8 % 📵 (Green)

Gamma 2D


Arithmetic Mean	0.395
Min (LR = 15.0 mm ; TG = -25.0 mm)	0.022
Max (LR = 0.0 mm ; TG = 10.0 mm)	1.058
Median	0.358


Absolute Difference


Arithmetic Mean	0.037	Gy
Min (LR = 15.0 mm ; TG = -25.0 mm)	0.001	Gy
Max (LR = -20.0 mm ; TG = -10.0 mm)	0.100	Gy
Median	0.031	Gy


Settings

 	
Passing criteria	Gamma ≤ 1.0
Green	90.0 % to 100.0 %
Yellow	75.0 % to 90.0 %
Red	0.0 % to 75.0 %

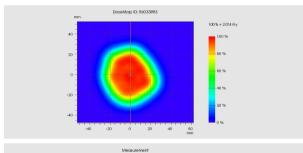







PTW - VeriSoft 7.1 PatientID: 56033983 Patient Name: CHANG SANG LYOOL, 104659 Date: 2025-08-28 00:10:23