


Calibrated feature pulses — site, timing and dose

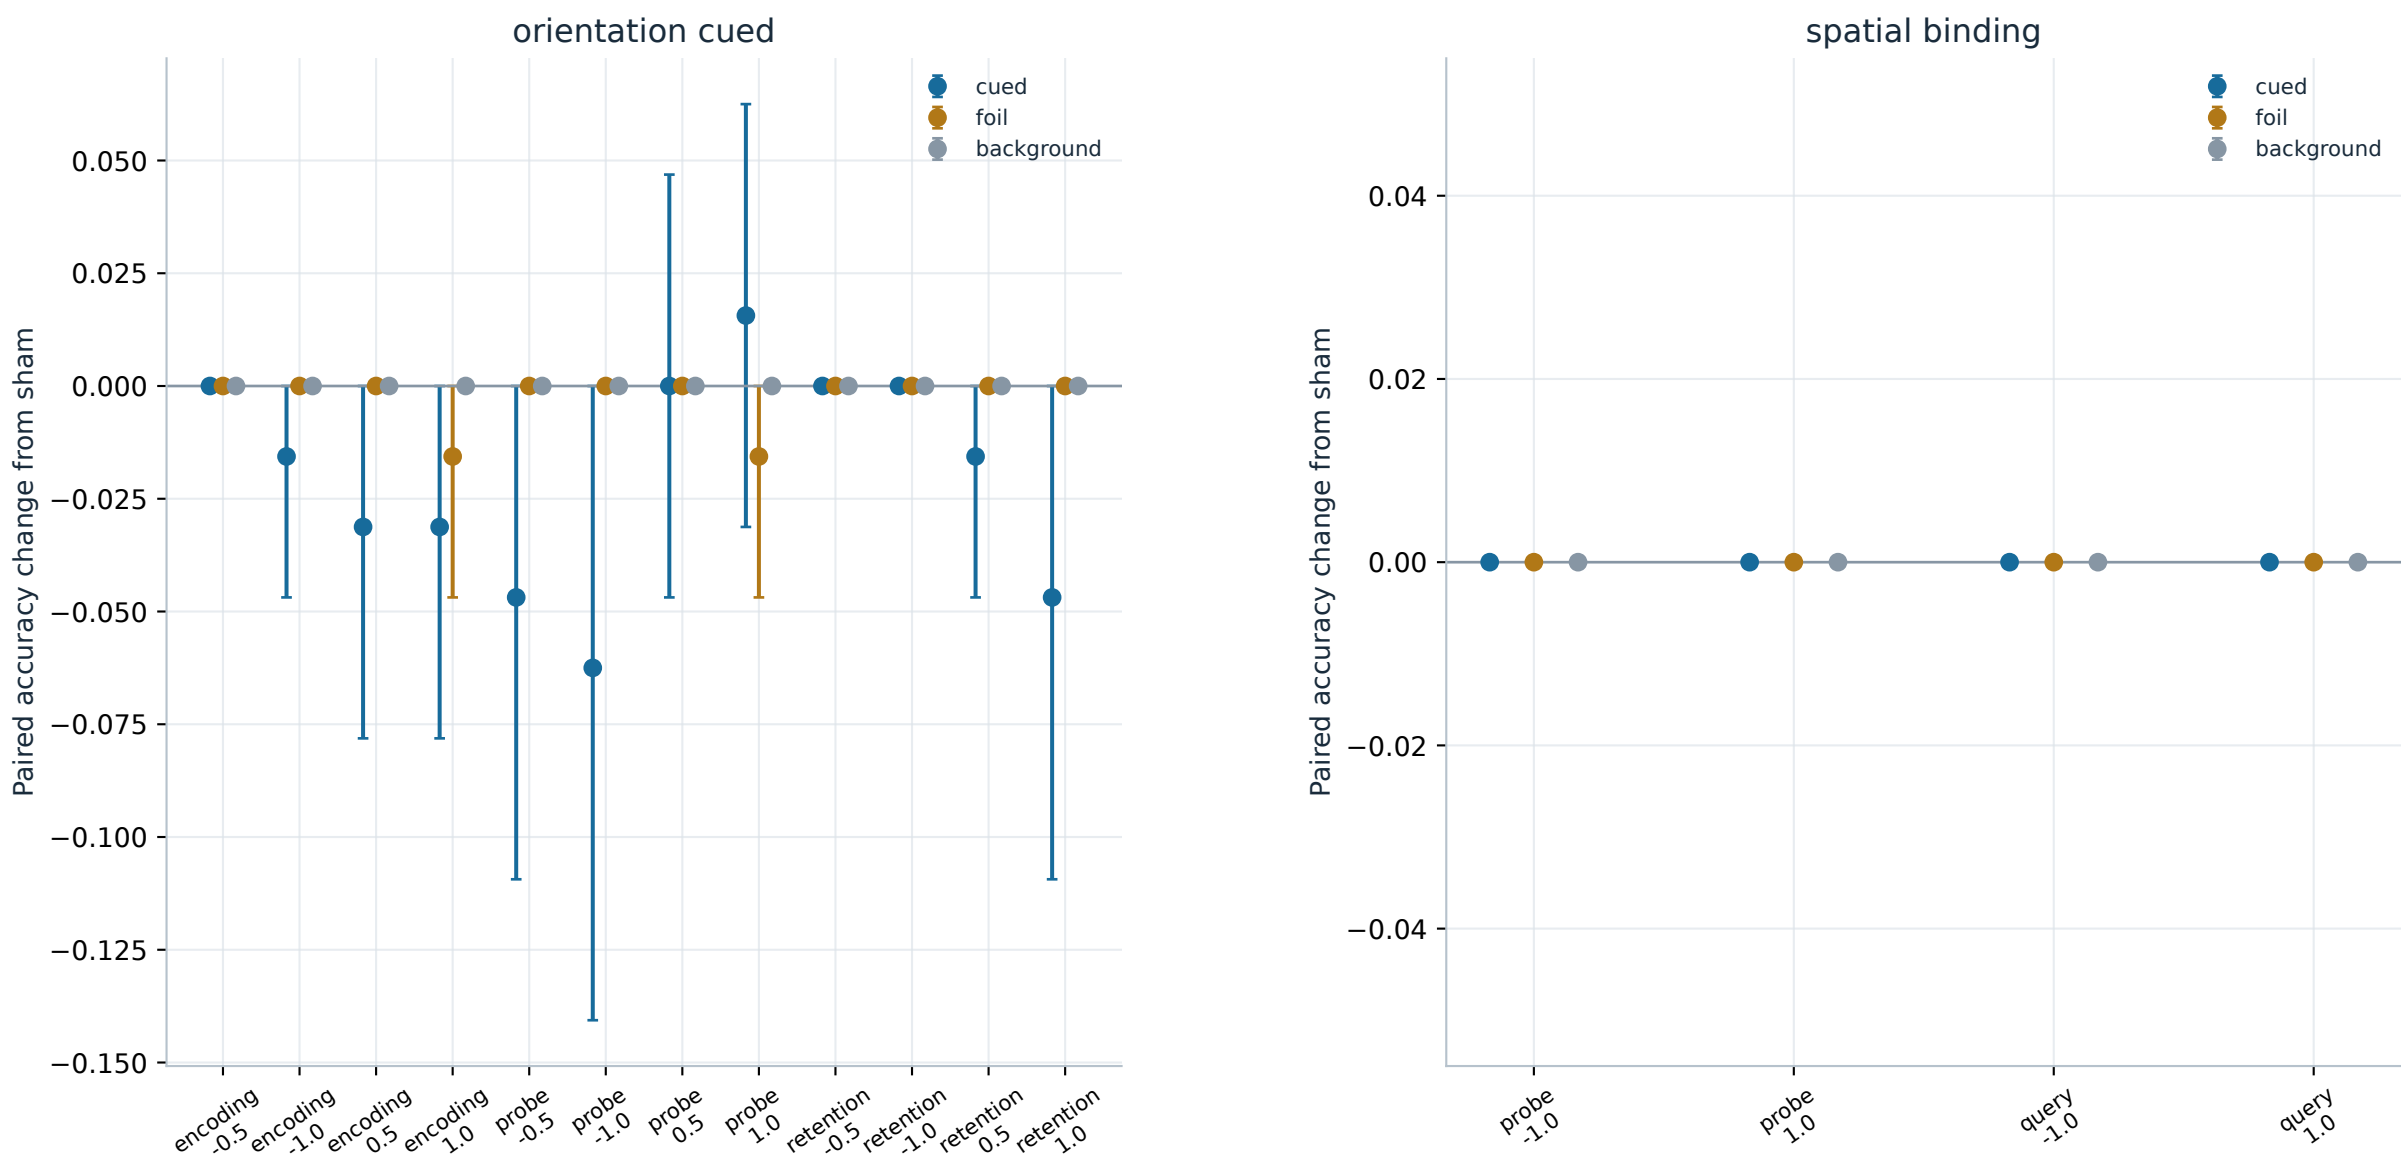

64 paired independent base trials per condition, a prespecified orientation magnitude mixture at D12. One update per pulse. Masks are matched in support/mass, not necessarily removed activation energy; achieved RMS is saved. Error bars 95% paired trial bootstrap; zero-width bars do not prove zero future effect (finite flip bounds in CSV). Binding encoding/retention cued means eventual target, not available cue. Underlying finest-scale KDA state is untouched; downstream recurrence can carry effects.