


Opposite pulses and matched random-direction controls

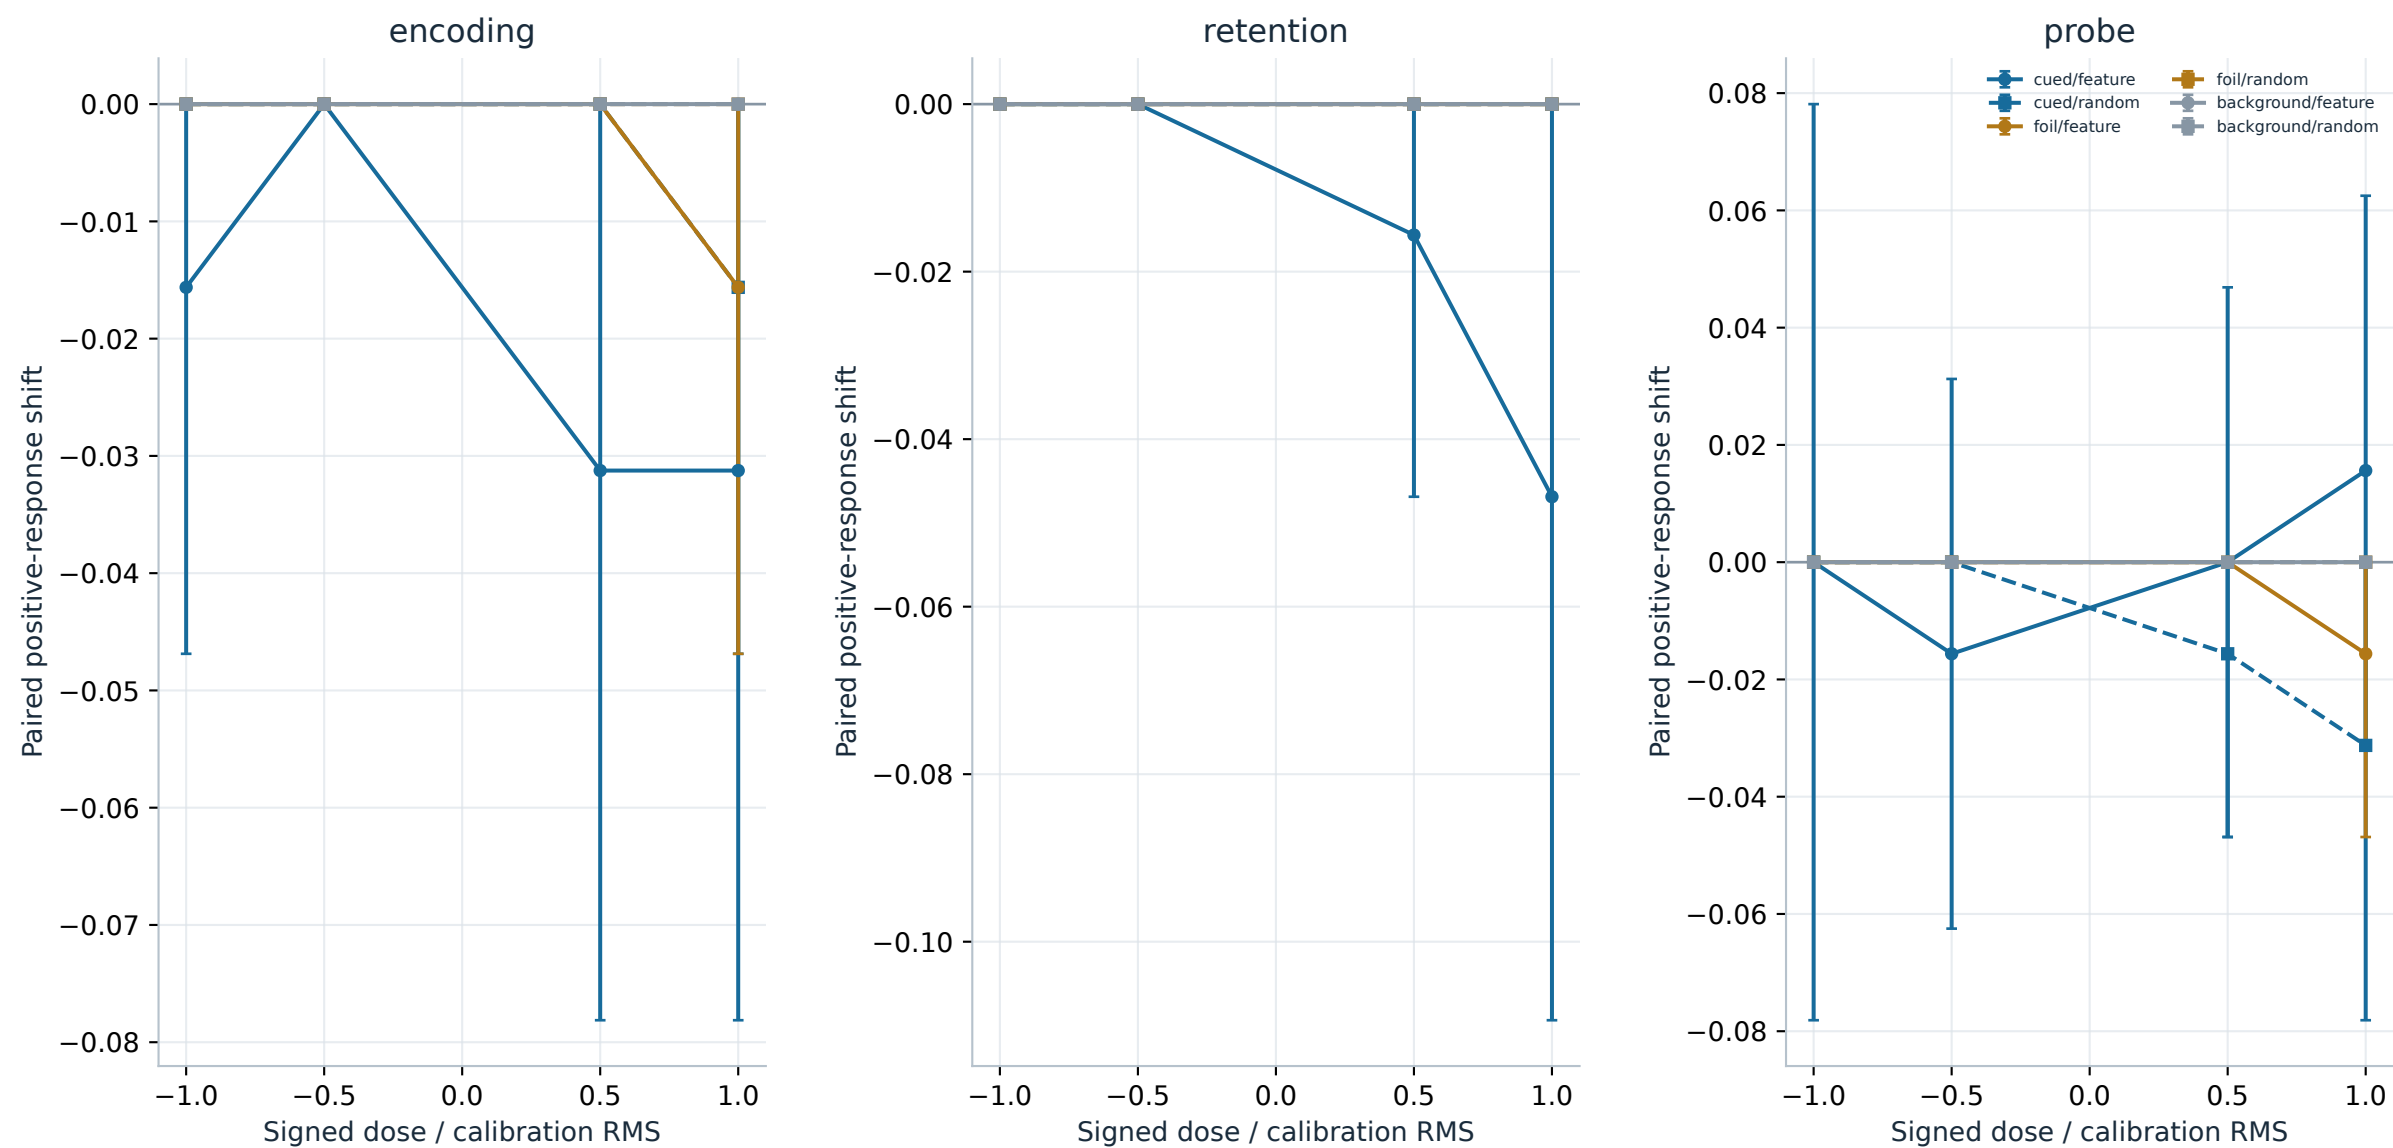

Solid circles: independently calibrated absolute-orientation direction. Dashed squares: orthogonal random direction with identical channel RMS. Positive/negative doses and three matched sites are measured, not inferred. 95% paired bootstrap. A null mean shift can mask opposing sign/location effects; a shift is not necessarily a sensitivity improvement. Physical current, neural cell type and milliseconds are not specified by model units.