Performance Report

Agilent Technologies

Data file:	C:\CHEM32\1\DATA\0_JONO_DATA\2023-02-15_WINES_2023-02-15_15-19-53\006-0601.D		
Sample name:	0101		
Description:			
Sample amount:	10.000	**Sample type:**	Sample
Instrument:	1290 LC	**Location:**	Vial 6
Injection date:	2/15/2023 7:50:05 PM	**Injection:**	1 of 1
Acq. method:	AVANTOR100X4_6C18-H2O-MEOH-2_1.M	**Injection volume:**	10.000
Analysis method:	AVANTOR100X4_6C18-H2O-MEOH-2_1.M	**Acq. operator:**	SYSTEM
Last changed:	2/15/2023 3:13:02 PM		

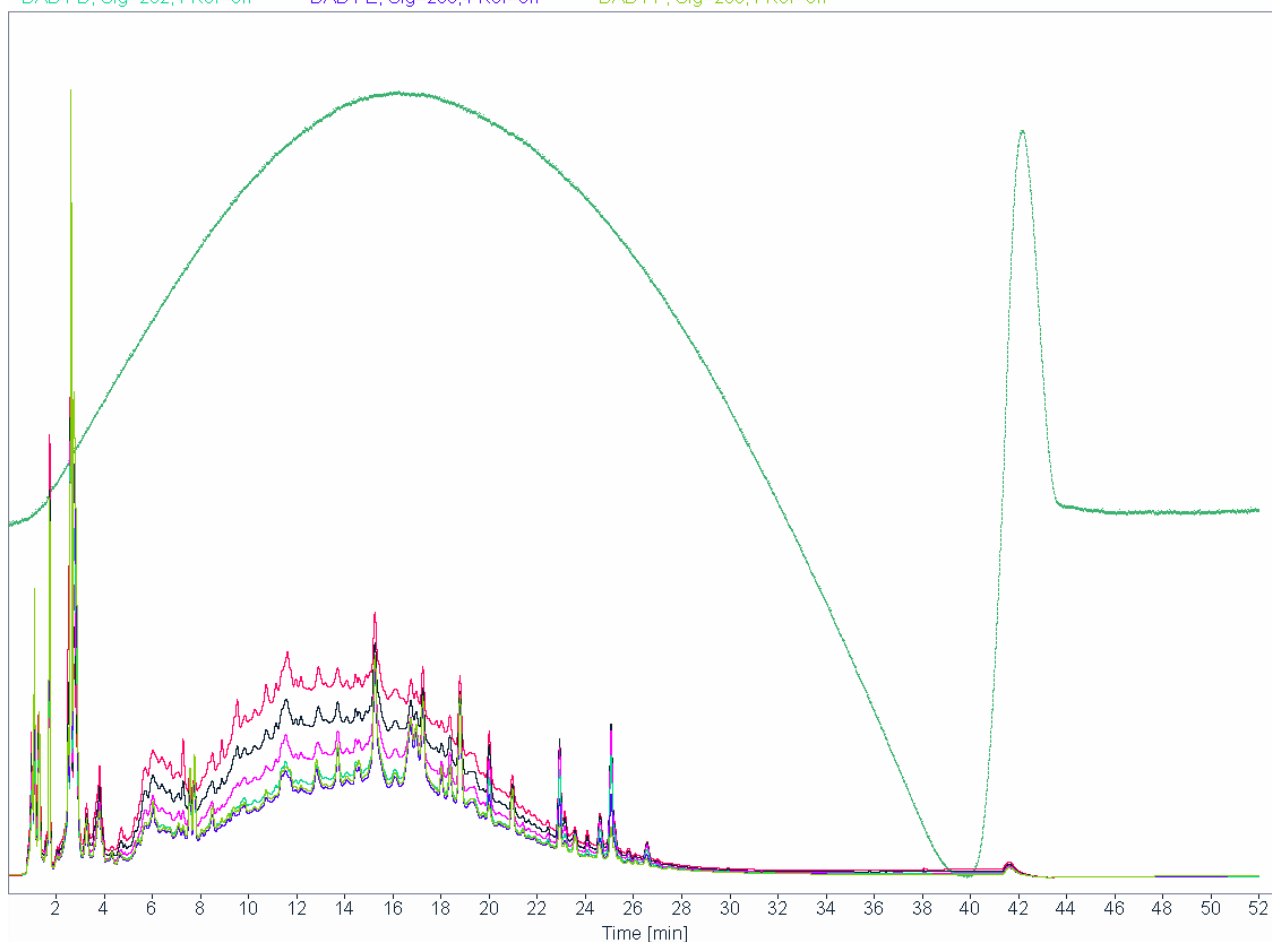|			
Column name:			
Serial #:			
Diameter:	mm	**Length:**	
Dead volume:		**# Injections:**	

PMP1, PMP1B, Pressure   DAD1 A, Sig=240,4 Ref=off   DAD1 B, Sig=244,4 Ref=off   DAD1 C, Sig=248,4 Ref=off
DAD1 D, Sig=252,4 Ref=off   DAD1 E, Sig=256,4 Ref=off   DAD1 F, Sig=260,4 Ref=off

Agilent Technologies

Agilent Technologies

Module	ID	Text	Time
Method		Method started: line# 6 at VIAL 6 inj# 1	2/15/2023 7:48:38 PM
Method		Instrument running sample Vial 6	2/15/2023 7:48:38 PM
G4212A	1	G4212A:DEBAF01058 - Detector: Prepare	2/15/2023 7:48:40 PM
G4212A	1	G4212A:DEBAF01058 - Detector: Idle	2/15/2023 7:48:53 PM
G4212A	1	G4212A:DEBAF01058 - Run	2/15/2023 7:50:05 PM
G1316A	1	G1316A:DEACN17041 - Postrun	2/15/2023 8:42:05 PM
G1329B	1	G1329B:DEAAC15668 - Postrun	2/15/2023 8:42:05 PM
G4220A	1	G4220A:DEBAA01336 - Postrun	2/15/2023 8:42:05 PM
Method		Instrument run completed	2/15/2023 8:42:09 PM
Method		Saving Method AVANTOR100X4_6C18-H2O-MEOH-2_1.M	2/15/2023 8:42:09 PM
CP Macro		Analyzing rawdata 006-0601.D	2/15/2023 8:42:09 PM
Method		Saving Method DA.M	2/15/2023 8:42:09 PM

Agilent Technologies