

# Test Equipment Solutions Datasheet

Test Equipment Solutions Ltd specialise in the second user sale, rental and distribution of quality test & measurement (T&M) equipment. We stock all major equipment types such as spectrum analyzers, signal generators, oscilloscopes, power meters, logic analysers etc from all the major suppliers such as Agilent, Tektronix, Anritsu and Rohde & Schwarz.

We are focused at the professional end of the marketplace, primarily working with customers for whom high performance, quality and service are key, whilst realising the cost savings that second user equipment offers. As such, we fully test & refurbish equipment in our in-house, traceable Lab. Items are supplied with manuals, accessories and typically a full no-quibble 2 year warranty. Our staff have extensive backgrounds in T&M, totalling over 150 years of combined experience, which enables us to deliver industry-leading service and support. We endeavour to be customer focused in every way right down to the detail, such as offering free delivery on sales, covering the cost of warranty returns BOTH ways (plus supplying a loan unit, if available) and supplying a free business tool with every order.

As well as the headline benefit of cost saving, second user offers shorter lead times, higher reliability and multivendor solutions. Rental, of course, is ideal for shorter term needs and offers fast delivery, flexibility, try-before-you-buy, zero capital expenditure, lower risk and off balance sheet accounting. Both second user and rental improve the key business measure of Return On Capital Employed.

We are based near Heathrow Airport in the UK from where we supply test equipment worldwide. Our facility incorporates Sales, Support, Admin, Logistics and our own in-house Lab.

All products supplied by Test Equipment Solutions include:

- No-quibble parts & labour warranty (we provide transport for UK mainland addresses).
- Free loan equipment during warranty repair, if available.
- Full electrical, mechanical and safety refurbishment in our in-house Lab.
- Certificate of Conformance (calibration available on request).
- Manuals and accessories required for normal operation.
- Free insured delivery to your UK mainland address (sales).
- Support from our team of seasoned Test & Measurement engineers.
- ISO9001 quality assurance.

Test equipment Solutions Ltd  
Unit 8 Elder Way  
Waterside Drive  
Langley  
Berkshire  
SL3 6EP


T: +44 (0)1753 596000  
F: +44 (0)1753 596001

Email: [info@TestEquipmentHQ.com](mailto:info@TestEquipmentHQ.com)  
Web: [www.TestEquipmentHQ.com](http://www.TestEquipmentHQ.com)



# Mixed Domain Oscilloscopes

## MDO4000 Series Data Sheet

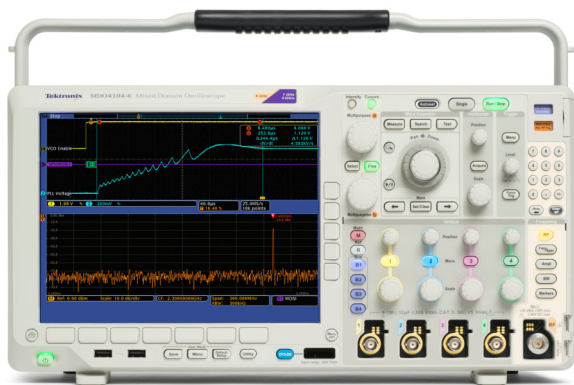

### Features & Benefits

#### Key Performance Specifications

- 4 Analog Channels
  - 500 MHz or 1 GHz Bandwidth Models
- 16 Digital Channels
  - MagniVu™ High-speed Acquisition provides 60.6 ps Fine Timing Resolution
- 1 RF Channel
  - 50 kHz - 3 GHz or 50 kHz - 6 GHz Frequency Range Models
  - Ultra-wide Capture Bandwidth  $\geq 1$  GHz
- Standard Passive Voltage Probes 3.9 pF Capacitive Loading and 500 MHz or 1 GHz Analog Bandwidth

#### Mixed Domain Analysis

- Time-correlated Analog, Digital, and RF Signal Acquisitions in a Single Instrument
- Wave Inspector® Controls provide Easy Navigation of Time-correlated Data from both the Time and Frequency Domains
- Amplitude, Frequency, and Phase vs. Time Waveforms derived from RF Input
- Selectable Spectrum Time to Discover and Analyze how RF Spectrum Changes over Time – Even on a Stopped Acquisition

#### Spectral Analysis

- Dedicated Front-panel Controls for Commonly Performed Tasks
- Automated Peak Markers Identify Frequency and Amplitude of Spectrum Peaks
- Manual Markers enable Non-peak Measurements
- Trace Types Include: Normal, Average, Max Hold, and Min Hold
- Detection Types Include: +Peak, -Peak, Average, and Sample
- Spectrogram Display enables Easy Observation and Insight into Slowly Changing RF Phenomena
- Automated Measurements Include: Channel Power, Adjacent Channel Power Ratio (ACPR), and Occupied Bandwidth (OBW)
- Trigger on RF Power Level
- Triggered or Free Run Spectral Analysis

#### Ease of Use Features

- 10.4 in. (264 mm) Bright XGA Color Display
- Small Footprint and Lightweight – Only 5.8 in. (147 mm) Deep and 11 lb. (5 kg)

#### Connectivity

- Two USB 2.0 Host Ports on the Front Panel and Two on the Rear Panel for Quick and Easy Data Storage, Printing, and Connecting a USB Keyboard
- USB 2.0 Device Port on Rear Panel for Easy Connection to a PC or Direct Printing to a PictBridge®-compatible Printer
- Integrated 10/100/1000BASE-T Ethernet Port for Network Connection and Video Out Port to Export the Oscilloscope Display to a Monitor or Projector

#### Optional Serial Triggering and Analysis

- Serial Protocol Trigger, Decode, and Search for I<sup>2</sup>C, SPI, USB, Ethernet, CAN, LIN, FlexRay, RS-232/422/485/UART, MIL-STD-1553, and I<sup>2</sup>S/LJ/RJ/TDM

#### Optional Application Support

- Advanced RF Triggering
- Power Analysis
- Limit and Mask Testing
- HDTV and Custom Video Analysis


## Introducing the Mixed Domain Oscilloscope

Introducing the world's first and only oscilloscope with a built-in spectrum analyzer. For the first time ever, you can capture time-correlated analog, digital, and RF signals for a complete system view of your device. See both the time and frequency domain in a single glance. View the RF spectrum at any point in time to see how it changes over time or with device state. Solve the most complicated design issues, quickly and efficiently, with an oscilloscope as integrated as your design.

Based on the industry-standard MSO4000B Oscilloscope Series, you can now use your tool of choice, the oscilloscope, to look at the frequency domain rather than having to find and re-learn a spectrum analyzer. However, the power of the MDO goes well beyond simply observing the frequency domain as you would on a spectrum analyzer. The real power is in its ability to correlate events in the frequency domain with the time domain phenomena that caused them.

When both the RF channel and any analog or digital channels are on, the oscilloscope display is split into two views. The upper half of the display is a traditional oscilloscope view of the Time Domain. The lower half of the display is a Frequency Domain view of the RF input. Note that the Frequency Domain view is not simply an FFT of the analog or digital channels in the instrument, but is the spectrum acquired from the RF input.

The spectrum shown in the Frequency Domain view is taken from the period of time indicated by the short orange bar in the time domain view – known as the Spectrum Time. With the MDO4000 Series, Spectrum Time can be moved through the acquisition to investigate how the RF spectrum changes over time. And this can be done while the oscilloscope is live and running or on a stopped acquisition.

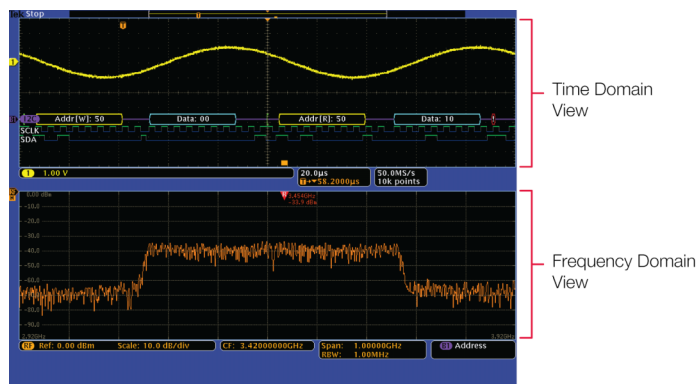

The upper half of the MDO4000 Series display shows the Time Domain view of the analog and digital channels, while the lower half shows the Frequency Domain view of the RF channel. The orange bar – Spectrum Time – shows the period of time used to calculate the RF spectrum.

Figures 1 through 4 show a simple everyday application – tuning of a VCO/PLL. This application illustrates the powerful connection between the time domain and the frequency domain that the MDO4000 Series provides. With its wide capture bandwidth and ability to move Spectrum Time throughout the acquisition, this single capture includes the same spectral content as approximately 1,500 unique test setups and acquisitions on a traditional spectrum analyzer. For the first time ever, correlating events, observing interactions, or measuring timing latencies between the two domains is exceptionally easy, giving you quick insight to your design's operation.

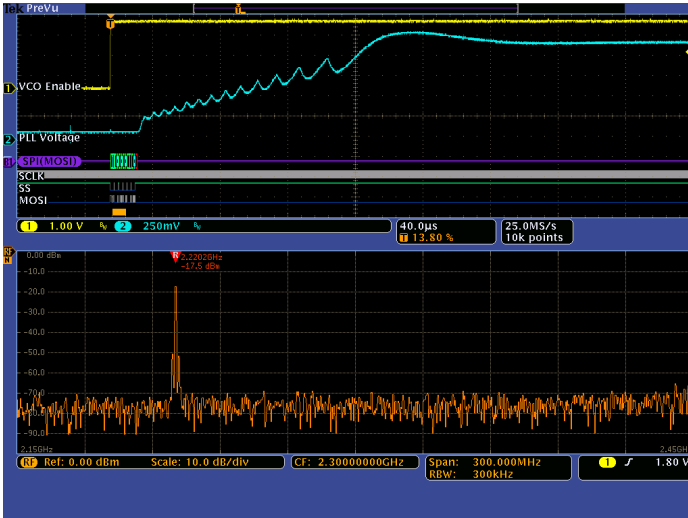


Figure 1 – Time and Frequency Domain view showing the turn-on of a VCO/PLL. Channel 1 (yellow) is probing a control signal that enables the VCO. Channel 2 (cyan) is probing the PLL voltage. The SPI bus which is programming the VCO/PLL with the desired frequency is probed with three digital channels and automatically decoded. Notice Spectrum Time is placed after the VCO was enabled and coincident with the command on the SPI bus telling the VCO/PLL the desired frequency.

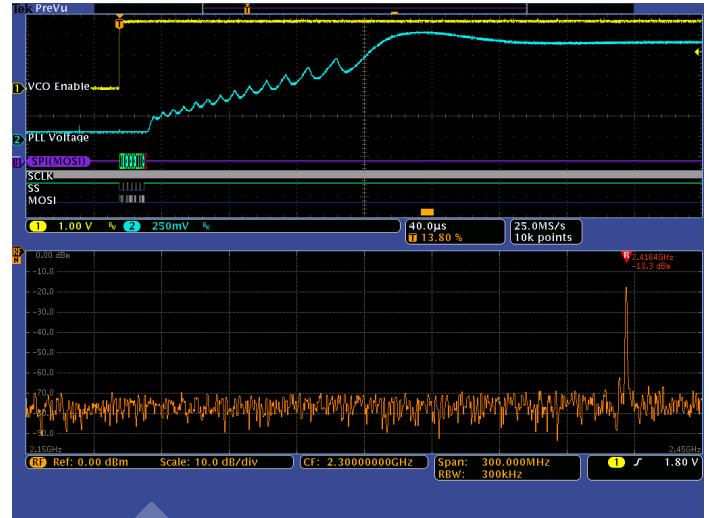


Figure 3 – Spectrum Time is moved another 120  $\mu$ s to the right. At this point the spectrum shows that the VCO/PLL has actually overshoot the correct frequency and gone all the way to 2.4164 GHz.

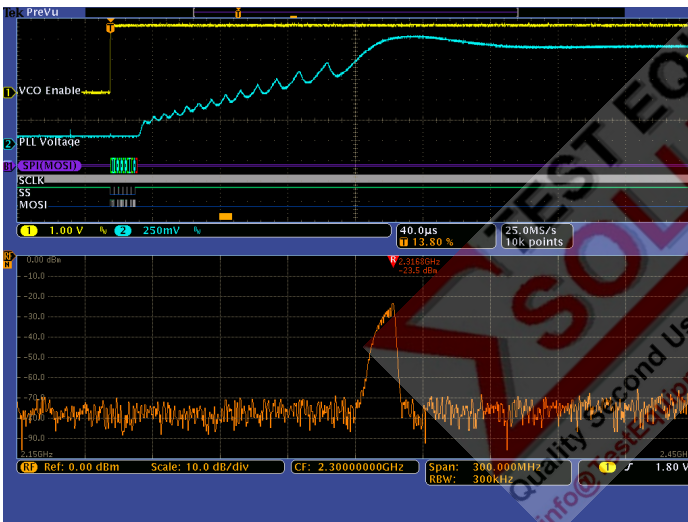


Figure 2 – Spectrum Time is moved about 60  $\mu$ s to the right. At this point, the spectrum shows that the VCO/PLL is in the process of tuning to the correct frequency (2.400 GHz). It has made it up to 2.3168 GHz.


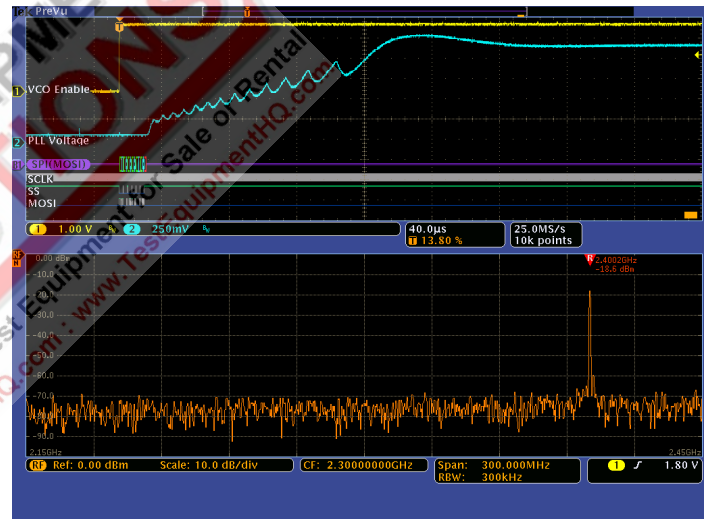


Figure 4 – The VCO/PLL eventually settles on the correct 2.400 GHz frequency about 340  $\mu$ s after the VCO was enabled.

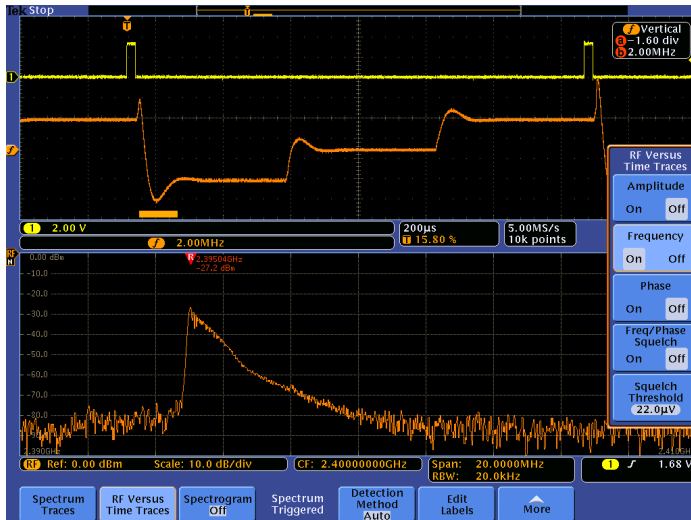

The orange waveform in the Time Domain view is the frequency vs. time trace derived from the RF input signal. Notice that Spectrum Time is positioned during a transition from the highest frequency to the lowest frequency, so the energy is spread across a number of frequencies. With the frequency vs. time trace, you can easily see the different frequency hops, simplifying characterization of how the device switches between frequencies.

### Visualizing Changes in Your RF Signal

The time domain graticule on the MDO4000 Series display provides support for three RF time domain traces that are derived from the underlying I and Q data of the RF input including:

- Amplitude – The instantaneous amplitude of the RF input vs. time
- Frequency – The instantaneous frequency of the RF input, relative to the center frequency vs. time
- Phase – The instantaneous phase of the RF input, relative to the center frequency vs. time


Each of these traces may be turned on and off independently, and all three may be displayed simultaneously. RF time domain traces make it easy to understand what's happening with a time-varying RF signal.

### Advanced Triggering


In order to deal with the time-varying nature of modern RF applications, the MDO4000 Series provides a triggered acquisition system that is fully integrated with the RF, analog, and digital channels. This means that a single trigger event coordinates acquisition across all channels, allowing you to capture a spectrum at the precise point in time where an interesting time domain event is occurring. A comprehensive set of time domain triggers are available, including Edge, Sequence, Pulse Width, Timeout, Runt, Logic, Setup/Hold Violation, Rise/Fall Time, Video, and a variety of parallel and serial bus packet triggers. In addition, you can trigger on the power level of the RF input. For example, you can trigger on your RF transmitter turning on.

The optional MDO4TRIG application module provides advanced RF triggering. This module enables the RF input power level to be used as a source for Sequence, Pulse Width, Timeout, Runt, and Logic trigger types. For example, you can trigger on a RF pulse of a specific length or use the RF channel as an input to a logic trigger, enabling the oscilloscope to trigger only when the RF is on while other signals are active.



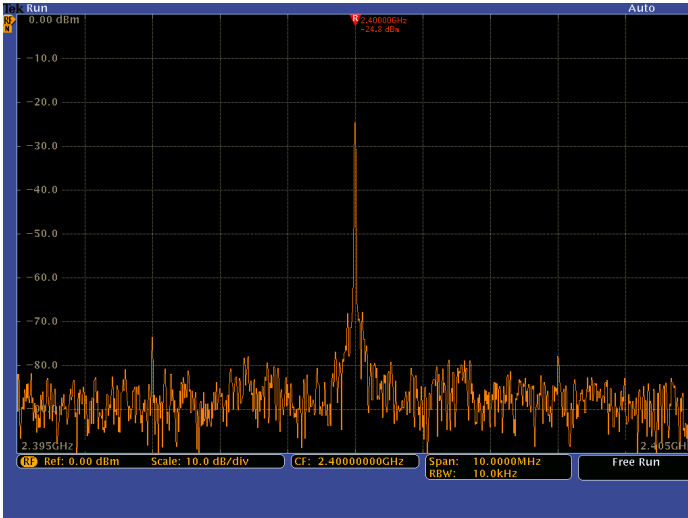

MDO4000 Frequency Domain display.

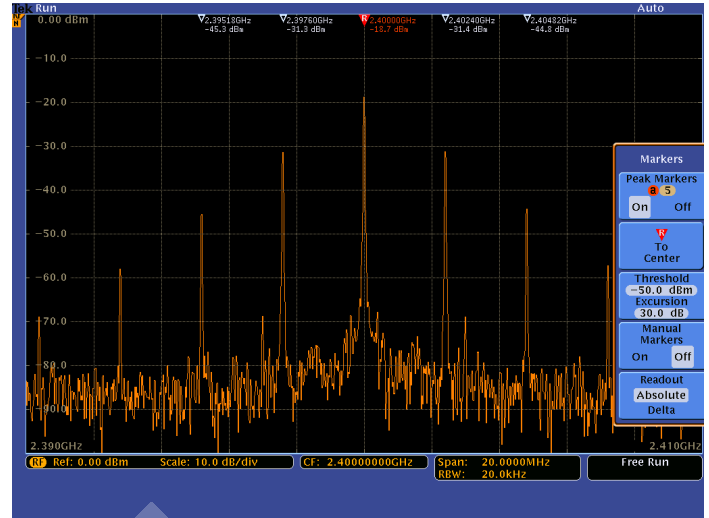

Automated peak markers identify critical information at a glance. As shown here, the five highest amplitude peaks that meet the threshold and excursion criteria are automatically marked.

Key spectral parameters such as Center Frequency, Span, Reference Level, and Resolution Bandwidth are all adjusted quickly and easily using the dedicated front-panel menus and keypad.

### Intelligent, Efficient Markers

In a traditional spectrum analyzer, it can be a very tedious task to turn on and place enough markers to identify all your peaks of interest. The MDO4000 Series makes this process far more efficient by automatically placing markers on peaks that indicate both the frequency and the amplitude of each peak. The criteria used to determine what a peak is can be adjusted by the user.

The highest amplitude peak is referred to as the reference marker and is shown in red. Marker readouts can be switched between Absolute and Delta readouts. When Delta is selected, marker readouts show each peak's delta frequency and delta amplitude from the reference marker.


Two manual markers are also available for measuring non-peak portions of the spectrum. When enabled, the reference marker is attached to one of the manual markers, enabling delta measurements from anywhere in the spectrum. In addition to frequency and amplitude, manual marker readouts also include noise density and phase noise readouts depending on whether Absolute or Delta readouts are selected. A "Reference Marker to Center" function instantly moves the frequency indicated by the reference marker to center frequency.



Key spectral parameters are adjusted quickly with the dedicated front-panel menus and keypad.

### Fast and Accurate Spectral Analysis

When using the RF input by itself, the MDO4000 Series display becomes a full-screen Frequency Domain view.

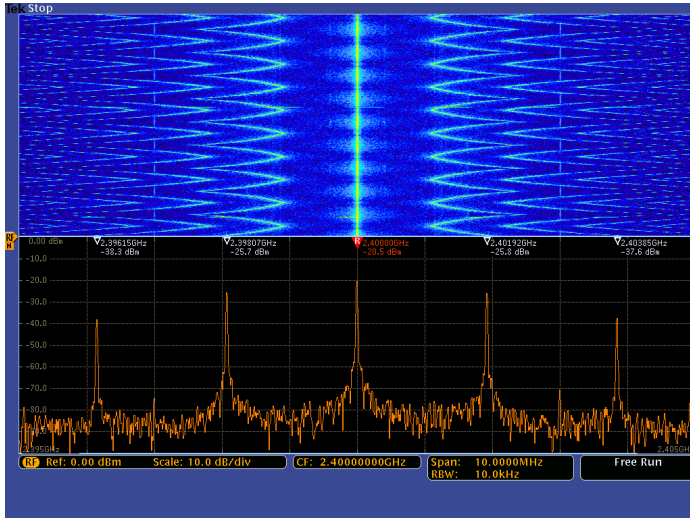

Spectrogram display illustrates slowly moving RF phenomena. As shown here, a signal that has multiple peaks is being monitored. As the peaks change in both frequency and amplitude over time, the changes are easily seen in the Spectrogram display.


### Spectrogram

The MDO4000 Series includes a spectrogram display which is ideal for monitoring slowly changing RF phenomena. The x-axis represents frequency, just like a typical spectrum display. However, the y-axis represents time, and color is used to indicate amplitude.

Spectrogram slices are generated by taking each spectrum and “flipping it up on its edge” so that it’s one pixel row tall, and then assigning colors to each pixel based on the amplitude at that frequency. Cold colors (blue, green) are low amplitude and hotter colors (yellow, red) are higher amplitude. Each new acquisition adds another slice at the bottom of the spectrogram and the history moves up one row. When acquisitions are stopped, you can scroll back through the spectrogram to look at any individual spectrum slice.

### Triggered vs. Free Run Operation

When both the time and frequency domains are displayed, the spectrum shown is always triggered by the system trigger event and is time correlated with the active time-domain traces. However, when only the frequency domain is displayed, the RF input can be set to Free Run. This is useful when the frequency domain data is continuous and unrelated to events occurring in the time domain.

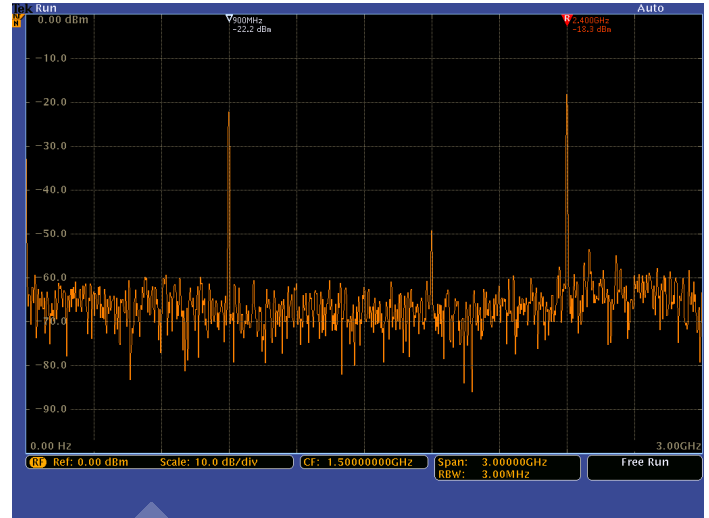


Spectral display of a bursted communication both into a device through Zigbee at 900 MHz and out of the device through Bluetooth at 2.4 GHz, captured with a single acquisition.

### Ultra-wide Capture Bandwidth


Today’s wireless communications vary significantly with time, using sophisticated digital modulation schemes and, often, transmission techniques that involve bursting the output. These modulation schemes can have very wide bandwidth as well. Traditional swept or stepped spectrum analyzers are ill equipped to view these types of signals as they are only able to look at a small portion of the spectrum at any one time.

The amount of spectrum acquired in one acquisition is called the capture bandwidth. Traditional spectrum analyzers sweep or step the capture bandwidth through the desired span to build the requested image. As a result, while the spectrum analyzer is acquiring one portion of the spectrum, the event you care about may be happening in another portion of the spectrum. Most spectrum analyzers on the market today have 10 MHz capture bandwidths, sometimes with expensive options to extend that to 20, 40, or even 140 MHz in some cases.

In order to address the bandwidth requirements of modern RF, the MDO4000 Series provides  $\geq 1$  GHz of capture bandwidth. At span settings of 1 GHz and below, there is no requirement to sweep the display. The spectrum is generated from a single acquisition, thus guaranteeing you’ll see the events you’re looking for in the frequency domain.

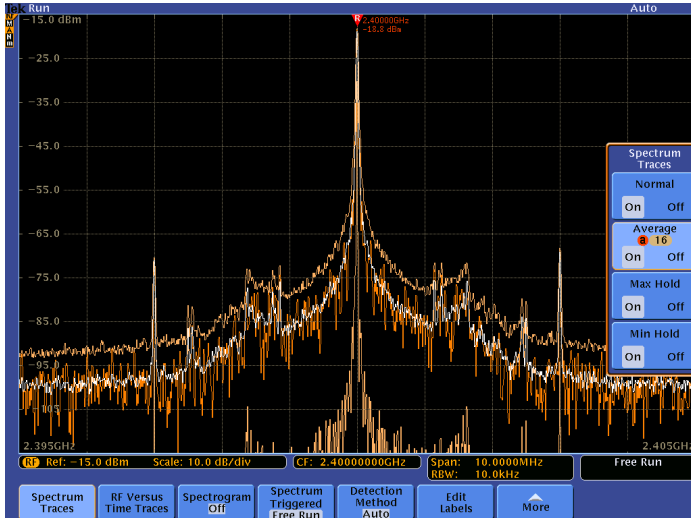


Normal, Average, Max Hold, and Min Hold spectrum traces.

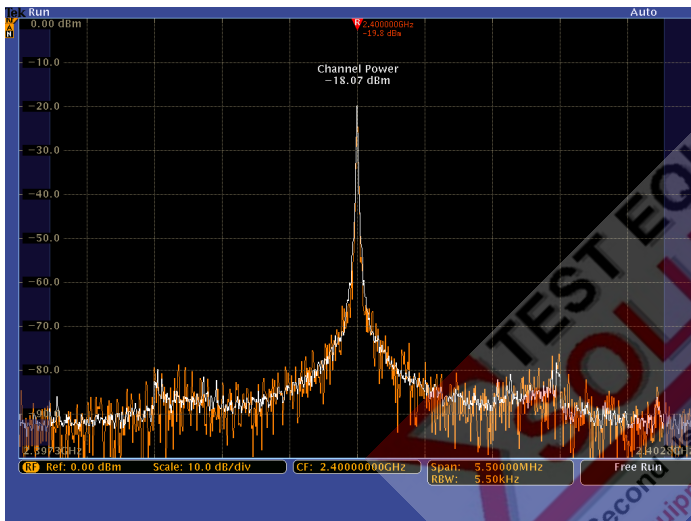

Automated Channel Power measurement.

### Spectrum Traces

The MDO4000 Series offers four different traces or views of the RF input including Normal, Average, Max Hold, and Min Hold. You can set the

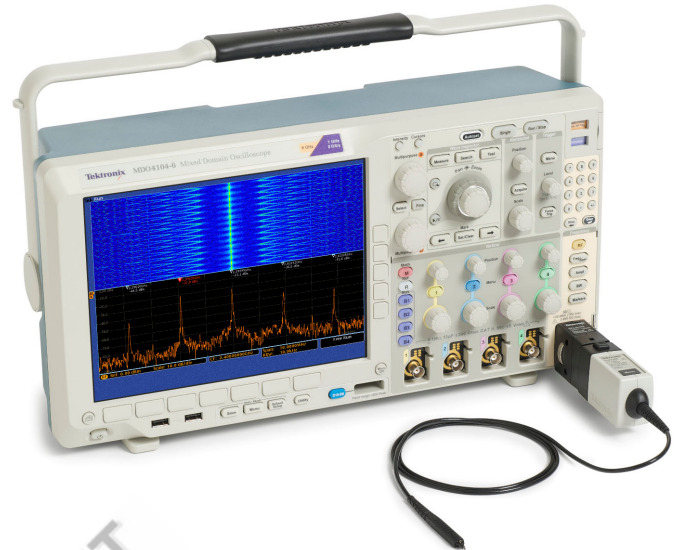

The optional TPA-N-VPI adapter enables any active, 50  $\Omega$  TekVPI probe to be connected to the RF input.

detection method used for each trace type independently or you can leave the oscilloscope in the default Auto mode that sets the detection type optimally for the current configuration. Detection types include +Peak, -Peak, Average, and Sample.


### RF Measurements

The MDO4000 Series includes three automated RF measurements – Channel Power, Adjacent Channel Power Ratio, and Occupied Bandwidth. When one of these RF measurements is activated, the oscilloscope automatically turns on the Average spectrum trace and sets the detection method to Average for optimal measurement results.

### RF Probing

Signal input methods on spectrum analyzers are typically limited to cabled connections or antennas. But with the optional TPA-N-VPI adapter, any active, 50  $\Omega$  TekVPI probe can be used with the RF input on the MDO4000 Series. This enables additional flexibility when hunting for noise sources and enables easier spectral analysis by using true signal browsing on an RF input.



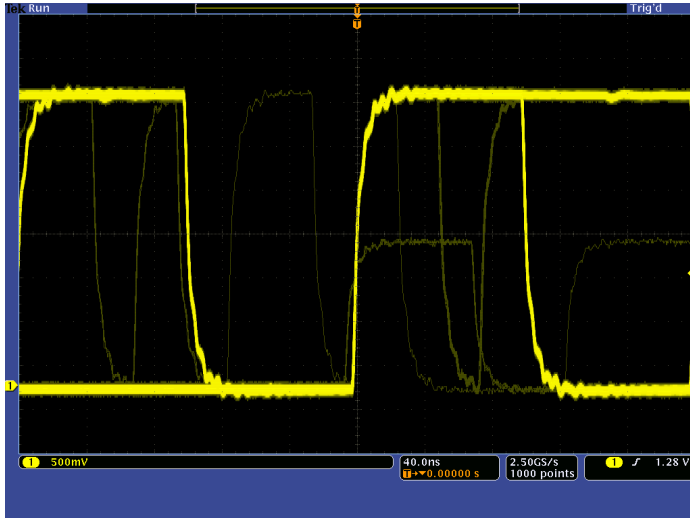

**Discover** – Fast waveform capture rate - over 50,000 wfms/s - maximizes the probability of capturing elusive glitches and other infrequent events.


## Built-on the Award Winning MSO4000B Series of Mixed Signal Oscilloscopes

The MDO4000 Series provides you with the same comprehensive set of features available in the MSO4000B Mixed Signal Oscilloscope Series. This robust set of tools will help you speed through every stage of debugging your design – from quickly discovering an anomaly and capturing it, to searching your waveform record for the event and analyzing its characteristics and your device's behavior.

### Discover

To debug a design problem, first you must know it exists. Every design engineer spends time looking for problems in their design, a time-consuming and frustrating task without the right debug tools.

The MDO4000 Series offers the industry's most complete visualization of signals, providing fast insight into the real operation of your device. A fast waveform capture rate – greater than 50,000 waveforms per second – enables you to see glitches and other infrequent transients within seconds, revealing the true nature of device faults. A digital phosphor display with intensity grading shows the history of a signal's activity by intensifying areas of the signal that occur more frequently, providing a visual display of just how often anomalies occur.

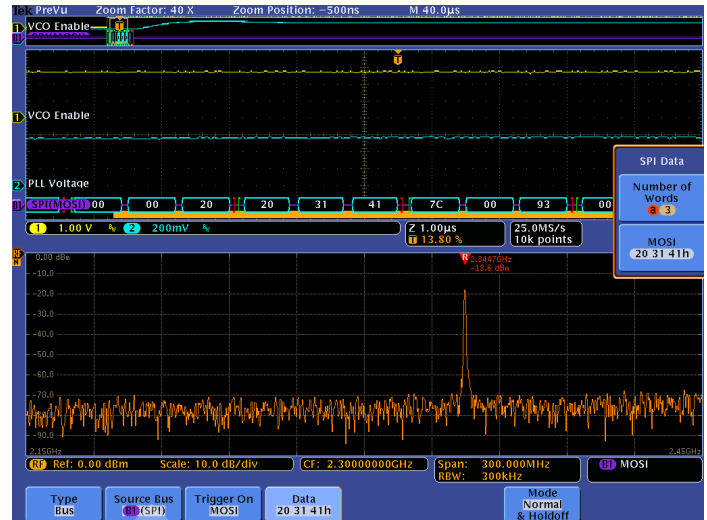

**Capture** – Triggering on a specific transmit data packet going across a SPI bus. A complete set of triggers, including triggers for specific serial packet content, ensures you quickly capture your event of interest.

### Capture


Discovering a device fault is only the first step. Next, you must capture the event of interest to identify root cause.

Accurately capturing any signal of interest begins with proper probing. The MDO4000 Series includes four low-capacitance probes for accurate signal capture. These industry-first high-impedance passive voltage probes have less than 4 pF of capacitive loading to minimize the affect of the probe on your circuit's operation, offering the performance of an active probe with the flexibility of a passive probe.

The MDO4000 Series provides a complete set of triggers – including Runt, Timeout, Logic, Pulse Width/Glitch, Setup/Hold Violation, Serial Packet, and Parallel Data – to help quickly find your event. With up to a 20M point record length, you can capture many events of interest, even thousands of serial packets, in a single acquisition for further analysis while maintaining high resolution to zoom in on fine signal details.

From triggering on specific packet content to automatic decode in multiple data formats, the MDO4000 Series provides integrated support for the industry's broadest range of serial buses – I<sup>2</sup>C, SPI, USB, Ethernet, CAN, LIN, FlexRay, RS-232/422/485/UART, MIL-STD-1553, and I<sup>2</sup>S/LJ/RJ/TDM. The ability to decode up to four serial and/or parallel buses simultaneously means you gain insight into system-level problems quickly.

To further help troubleshoot system-level interactions in complex embedded systems, the MDO4000 Series offers 16 digital channels. The MagniVu™ high-speed acquisition on these channels enables you to acquire fine signal detail (up to 60.6 ps resolution) around the trigger point for precision measurements. MagniVu is essential for making accurate timing measurements for setup and hold, clock delay, signal skew, and glitch characterization.

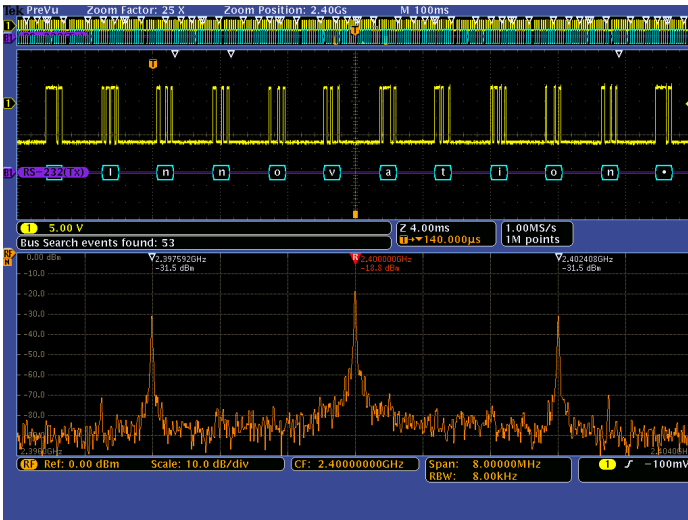


**Search** – RS-232 decode showing results from a Wave Inspector® search for data value "n". Wave Inspector controls provide unprecedented efficiency in viewing and navigating waveform data.

### Search

Finding your event of interest in a long waveform record can be time consuming without the right search tools. With today's record lengths pushing beyond a million data points, locating your event can mean scrolling through thousands of screens of signal activity.

The MDO4000 Series offers the industry's most comprehensive search and waveform navigation with its innovative Wave Inspector® controls. These controls speed panning and zooming through your record. With a unique force-feedback system, you can move from one end of your record to the other in just seconds. User marks allow you to mark any location that you may want to reference later for further investigation. Or, automatically search your record for criteria you define. Wave Inspector will instantly search your entire record, including analog, digital, and serial bus data. Along the way it will automatically mark every occurrence of your defined event so you can quickly move between each occurrence.

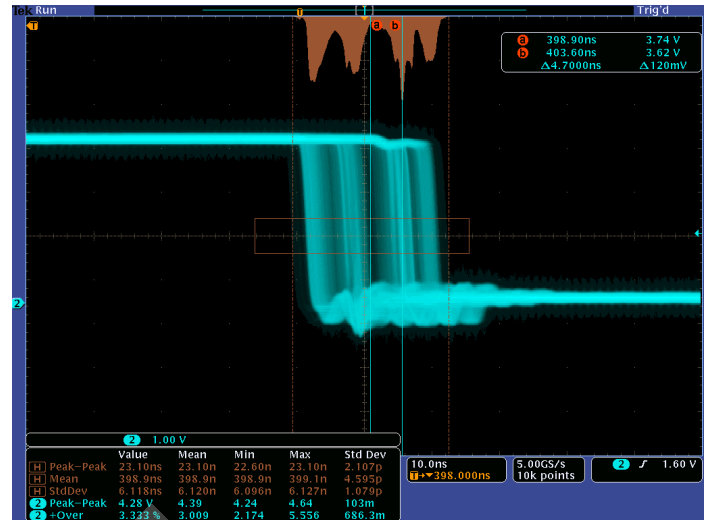

**Analyze** – Waveform histogram of a falling edge showing the distribution of edge position (jitter) over time. Included are numeric measurements made on the waveform histogram data. A comprehensive set of integrated analysis tools speeds verification of your design's performance.

### Analyze

Verifying that your prototype's performance matches simulations and meets the project's design goals requires analyzing its behavior. Tasks can range from simple checks of rise times and pulse widths to sophisticated power loss analysis and investigation of noise sources.

The MDO4000 Series offers a comprehensive set of integrated analysis tools including waveform- and screen-based cursors, 44 automated measurements, and advanced waveform math including arbitrary equation editing, waveform histograms, FFT analysis, and trend plots for visually determining how a measurement is changing over time. Specialized application support for serial bus analysis, power supply design, limit and mask testing, and video design and development is also available.

For extended analysis, National Instrument's LabVIEW SignalExpress™ Tektronix Edition provides over 200 built-in functions including time and frequency domain analysis, data logging, and customizable reports.

## Specifications

| Characteristic   | MDO4054-3   | MDO4104-3 | MDO4054-6      | MDO4104-6 |
|--|---|-----------|----------------|-----------|
| Analog Channels  | 4   |           |                |           |
| Bandwidth  | 500 MHz   | 1 GHz     | 500 MHz        | 1 GHz     |
| Sample Rate (1-2 ch)   | 2.5 GS/s  | 5 GS/s    | 2.5 GS/s       | 5 GS/s    |
| Sample Rate (3-4 ch)   | 2.5 GS/s  |           |                |           |
| Digital Channels   | 16  |           |                |           |
| RF Channels  | 1   |           |                |           |
| Frequency Range  | 50 kHz - 3 GHz  |           | 50 kHz - 6 GHz |           |
| Real-time Capture Bandwidth                                    | ≥1 GHz  |           |                |           |
| Span   | 1 kHz - 3/6 GHz in a 1-2-5 sequence   |           |                |           |
| Resolution Bandwidth   | 20 Hz - 10 MHz in a 1-2-3-5 sequence  |           |                |           |
| Reference Level  | −140 dBm to +30 dBm in steps of 5 dBm   |           |                |           |
| Vertical Scale   | 1 dB/div to 20 dB/div in a 1-2-5 sequence   |           |                |           |
| Vertical Position  | −10 divs to +10 divs  |           |                |           |
| Vertical Units   | dBm, dBmV, dBμV, dBμW, dBmA, dBμA   |           |                |           |
| Displayed Average Noise Level (DANL)                           | 50 kHz - 5 MHz: < −130 dBm/Hz (< −134 dBm/Hz typical)<br>5 MHz - 3 GHz: < −148 dBm/Hz (< −152 dBm/Hz typical)<br>3 GHz - 6 GHz: < −140 dBm/Hz (< −143 dBm/Hz typical) |           |                |           |
| Spurious Response  |   |           |                |           |
| 2nd and 3rd Harmonic Distortion (>30 MHz)                      | < −55 dBc (< −60 dBc typical)   |           |                |           |
| 2nd Order Intermodulation Distortion                           | < −55 dBc (< −60 dBc typical)   |           |                |           |
| 3rd Order Intermodulation Distortion                           | < −60 dBc (< −63 dBc typical)   |           |                |           |
| Other A/D Spurs  | < −55 dBc (< −60 dBc typical)   |           |                |           |
| Image and IF Rejection   | < −50 dBc (< −55 dBc typical)   |           |                |           |
| Residual Response  | < −78 dBm   |           |                |           |
| Crosstalk to RF Channel from Scope Channels                    | ≤1 GHz input frequencies: < −68 dB from ref level<br>>1 GHz - 2 GHz input frequencies: < −48 dB from ref level  |           |                |           |
| Phase Noise at 2 GHz CW  | 10 kHz: < −90 dBc/Hz, < −95 dBc/Hz (typical)<br>100 kHz: < −95 dBc/Hz, < −98 dBc/Hz (typical)<br>1 MHz: < −113 dBc/Hz, < −118 dBc/Hz (typical)                        |           |                |           |
| Level Measurement Uncertainty (Input level +10 dBm to −50 dBm) | 20 °C - 30 °C: < ±1 dB (< ±0.5 dB typical)<br>Over operating range: < ±1.5 dB   |           |                |           |
| Residual FM  | ≤100 Hz peak-to-peak in 100 ms  |           |                |           |
| Maximum Operating Input Level                                  |   |           |                |           |
| Average Continuous Power                                       | +30 dBm (1 W)   |           |                |           |
| DC Maximum Before Damage                                       | ±40 V DC  |           |                |           |
| Maximum Power Before Damage (CW)                               | +33 dBm (2 W)   |           |                |           |
| Maximum Power Before Damage (Pulse)                            | +45 dBm (32 W)<br>(<10 μs pulse width, <1% duty cycle, and reference level of ≥ +10 dBm)  |           |                |           |
| Power Level Trigger  |   |           |                |           |
| Frequency Range  | 1 MHz - 3 GHz   |           | 1 MHz - 6 GHz  |           |
| Amplitude Range  | +30 dBm to −40 dBm  |           |                |           |
| Limits   | With CF 1 MHz - 3.25 GHz: −35 dB from ref level<br>With CF >3.25 GHz: −15 dB from ref level   |           |                |           |
| Minimum Pulse Duration   | 10 μs On Time with a minimum settling Off Time of 10 μs   |           |                |           |
| RF to Analog Channel Skew                                      | <5 ns   |           |                |           |

| Characteristic               | MDO4054-3  | MDO4104-3 | MDO4054-6 | MDO4104-6 |
|------------------------------|--|-----------|-----------|-----------|
| Frequency Domain Trace Types | Normal, Average, Max Hold, Min Hold  |           |           |           |
| Time Domain Trace Types      | Amplitude vs. Time, Frequency vs. Time, Phase vs. Time                             |           |           |           |
| Detection Methods            | +Peak, -Peak, Average, Sample  |           |           |           |
| Automatic Markers            | 1-11 peaks identified based on user-adjustable threshold and excursion values      |           |           |           |
| Manual Markers               | Two manual markers indicating frequency, amplitude, noise density, and phase noise |           |           |           |
| Marker Readouts              | Absolute or Delta  |           |           |           |

**RF Acquisition Length**

| Span               | Maximum RF Acquisition Time |
|--------------------|-----------------------------|
| >2 GHz             | 2.5 ms                      |
| >1 GHz - 2 GHz     | 5 ms                        |
| >800 MHz - 1 GHz   | 10 ms                       |
| >500 MHz - 800 MHz | 12.5 ms                     |
| >400 MHz - 500 MHz | 20 ms                       |
| >250 MHz - 400 MHz | 25 ms                       |
| >200 MHz - 250 MHz | 40 ms                       |
| >160 MHz - 200 MHz | 50 ms                       |
| >125 MHz - 160 MHz | 62.5 ms                     |
| <125 MHz           | 79 ms                       |

**FFT Windows**

| FFT Window      | Factor |
|-----------------|--------|
| Kaiser          | 2.23   |
| Rectangular     | 0.89   |
| Hamming         | 1.30   |
| Hanning         | 1.44   |
| Blackman-Harris | 1.90   |
| Flat-Top        | 3.77   |

**TEST EQUIPMENT SOLUTIONS**  
 Quality Second User Test Equipment for Sale or Rental  
 info@TestEquipmentHQ.com : www.TestEquipmentHQ.com



## Vertical System Analog Channels

| Characteristic                                 | MDO4054-X  | MDO4104-X |
|--|--|-----------|
| Input Channels                                 | 4  |           |
| Analog Bandwidth (-3 dB)<br>5 mV/div - 1 V/div | 500 MHz  | 1 GHz     |
| Calculated Rise Time<br>5 mV/div (typical)     | 700 ps   | 350 ps    |
| Hardware Bandwidth Limits                      | 20 MHz or 250 MHz  |           |
| Input Coupling                                 | AC, DC   |           |
| Input Impedance                                | 1 M $\Omega$ $\pm$ 1%, 50 $\Omega$ $\pm$ 1%  |           |
| Input Sensitivity, 1 M $\Omega$                | 1 mV/div to 10 V/div   |           |
| Input Sensitivity, 50 $\Omega$                 | 1 mV/div to 1 V/div  |           |
| Vertical Resolution                            | 8 bits (11 bits with Hi Res)   |           |
| Max Input Voltage, 1 M $\Omega$                | 300 V <sub>RMS</sub> CAT II with peaks $\leq$ $\pm$ 425 V  |           |
| Max Input Voltage, 50 $\Omega$                 | 5 V <sub>RMS</sub> with peaks $<$ $\pm$ 20 V   |           |
| DC Gain Accuracy                               | $\pm$ 1.5%, derated at 0.10%/°C above 30 °C  |           |
| Channel-to-Channel Isolation                   | $\geq$ 100:1 at $\leq$ 100 MHz and $\geq$ 30:1 at $>$ 100 MHz up to the rated bandwidth for any two channels having equal volts/div settings |           |

## Offset Range

| Range                      | 1 M $\Omega$ | 50 $\Omega$ |
|----------------------------|--------------|-------------|
| 1 mV/div to 50 mV/div      | $\pm$ 1 V    | $\pm$ 1 V   |
| 50.5 mV/div to 99.5 mV/div | $\pm$ 0.5 V  | $\pm$ 0.5 V |
| 100 mV/div to 500 mV/div   | $\pm$ 10 V   | $\pm$ 10 V  |
| 505 mV/div to 995 mV/div   | $\pm$ 5 V    | $\pm$ 5 V   |
| 1 V/div to 5 V/div         | $\pm$ 100 V  | $\pm$ 5 V   |
| 5.05 V/div to 10 V/div     | $\pm$ 50 V   | NA          |

## Vertical System Digital Channels

| Characteristic               | All MDO4000 Models  |
|------------------------------|---|
| Input Channels               | 16 Digital (D15 - D0)   |
| Thresholds                   | Per-channel Thresholds  |
| Threshold Selections         | TTL, CMOS, ECL, PECL, User Defined                                    |
| User-defined Threshold Range | $\pm$ 40 V  |
| Maximum Input Voltage        | $\pm$ 42 V <sub>peak</sub>  |
| Threshold Accuracy           | $\pm$ (100 mV + 3% of threshold setting)                              |
| Input Dynamic Range          | 30 V <sub>p-p</sub> $\leq$ 200 MHz<br>10 V <sub>p-p</sub> $>$ 200 MHz |
| Minimum Voltage Swing        | 400 mV  |
| Input Impedance              | 100 k $\Omega$  |
| Probe Loading                | 3 pF  |
| Vertical Resolution          | 1 bit   |

## Horizontal System Analog Channels

| Characteristic  | MDO4054-X                                 | MDO4104-X         |
|---|---|-------------------|
| Maximum Record Length (All channels)                        | 20M points                                |                   |
| Maximum Duration at Highest Sample Rate (All/Half channels) | 8/8 ms                                    | 8/4 ms            |
| Time Base Range   | 1 ns to 1,000 s                           | 400 ps to 1,000 s |
| Time Base Delay Time Range                                  | -10 divisions to 5000 s                   |                   |
| Channel-to-Channel Deskew Range                             | $\pm$ 125 ns                              |                   |
| Time Base Accuracy  | $\pm$ 5 ppm over any $\geq$ 1 ms interval |                   |

## Horizontal System Digital Channels

| Characteristic                           | All MDO4000 Models   |
|--|--|
| Maximum Sample Rate (Main)               | 500 MS/s (2 ns resolution)   |
| Maximum Record Length (Main)             | 20M points   |
| Maximum Sample Rate (MagniVu)            | 16.5 GS/s (60.6 ps resolution)   |
| Maximum Record Length (MagniVu)          | 10k points centered around the trigger   |
| Minimum Detectable Pulse Width (Typical) | 1 ns   |
| Channel-to-Channel Skew (Typical)        | 200 ps   |
| Maximum Input Toggle Rate                | 500 MHz  |
|  | Maximum frequency sine wave that can accurately be reproduced as a logic square wave. Requires the use of a short ground extender on each channel. |
|  | This is the maximum frequency at the minimum swing amplitude. Higher toggle rates can be achieved with higher amplitudes.                          |

**Trigger System**

| Characteristic        | Description  |
|-----------------------|--|
| Main Trigger Modes    | Auto, Normal, and Single   |
| Trigger Coupling      | DC, AC, HF reject (attenuates >50 kHz), LF reject (attenuates <50 kHz), noise reject (reduces sensitivity) |
| Trigger Holdoff Range | 20 ns to 8 s   |

**Trigger Sensitivity**

| Characteristic                 | Description   |
|--------------------------------|---|
| <b>Internal DC Coupled</b>     |   |
| 1 M $\Omega$ Path (All models) | For 1 mV/div to 4.98 mV/div; 0.75 div from DC to 50 MHz, increasing to 1.3 div at rated bandwidth |
| 50 $\Omega$ Path (MDO4054-X)   | For $\geq 5$ mV/div; 0.4 div from DC to 50 MHz, increasing to 1 div at rated bandwidth            |
| 50 $\Omega$ Path (MDO4104-X)   | 0.4 div from DC to 50 MHz, increasing to 1 div at rated bandwidth                                 |

**Trigger Level Range**

| Characteristic | Description                             |
|----------------|---|
| Any Channel    | $\pm 8$ divisions from center of screen |
| Line           | Fixed at about 50% of line voltage      |

**Trigger Frequency Readout**

Provides 6-digit frequency readout of triggerable events.

**Trigger Modes**

| Mode                        | Description  |
|-----------------------------|--|
| Edge                        | Positive or negative slope on any channel. Coupling includes DC, AC, HF reject, LF reject, and noise reject  |
| Sequence (B-trigger)        | Trigger Delay by Time – 4 ns to 8 s. Or Trigger Delay by Events – 1 to 4,000,000 events  |
| Pulse Width                 | Trigger on width of positive or negative pulses that are >, <, =, or $\neq$ a specified period of time (4 ns to 8 s)   |
| Timeout                     | Trigger when no pulse is detected within a specified time (4 ns to 8 s)  |
| Runt                        | Trigger on a pulse that crosses one threshold but fails to cross a second threshold before crossing the first again  |
| Logic                       | Trigger when any logical pattern of channels goes false or stays true for specified period of time (4 ns to 8 s). Any input can be used as a clock to look for the pattern on a clock edge. Pattern (AND, OR, NAND, NOR) specified for all analog and digital input channels defined as High, Low, or Don't Care |
| Setup and Hold              | Trigger on violations of both setup time and hold time between clock and data present on any of the input channels   |
| Rise/Fall Time              | Trigger on pulse edge rates that are faster or slower than specified. Slope may be positive, negative, or either   |
| Video                       | Trigger on all lines, odd, even, or all fields on NTSC, PAL, and SECAM video signals   |
| Extended Video (Optional)   | Trigger on 480p/60, 576p/50, 720p/30, 720p/50, 720p/60, 875i/60, 1080i/50, 1080i/60, 1080p/24, 1080p/24sF, 1080p/25, 1080p/30, 1080p/50, 1080p/60, and custom bi-level and tri-level sync video standards  |
| I <sup>2</sup> C (Optional) | Trigger on Start, Repeated Start, Stop, Missing ACK, Address (7 or 10 bit), Data, or Address and Data on I <sup>2</sup> C buses up to 10 Mb/s  |
| SPI (Optional)              | Trigger on SS active, MOSI, MISO, or MOSI and MISO on SPI buses up to 50 Mb/s  |

| Mode                           | Description   |
|--------------------------------|---|
| USB (Optional)                 | <p>Low-speed: Trigger on Sync, Reset, Suspend, Resume, End of Packet, Token (Address) Packet, Data Packet, Handshake Packet, Special Packet, Error.</p> <p>Token packet trigger – Any token type, SOF, OUT, IN, SETUP; Address can be specified for Any Token, OUT, IN, and SETUP token types. Address can be further specified to trigger on <math>\leq</math>, <math>&lt;</math>, <math>=</math>, <math>&gt;</math>, <math>\geq</math>, <math>\neq</math> a particular value, or inside or outside of a range. Frame number can be specified for SOF token using binary, hex, unsigned decimal and don't care digits.</p> <p>Data packet trigger – Any data type, DATA0, DATA1; Data can be further specified to trigger on <math>\leq</math>, <math>&lt;</math>, <math>=</math>, <math>&gt;</math>, <math>\geq</math>, <math>\neq</math> a particular data value, or inside or outside of a range.</p> <p>Handshake packet trigger – Any handshake type, ACK, NAK, STALL.</p> <p>Special packet trigger – Any special type, Reserved.</p> <p>Error trigger – PID Check, CRC5 or CRC16, Bit Stuffing.</p> <hr/> <p>Full-speed: Trigger on Sync, Reset, Suspend, Resume, End of Packet, Token (Address) Packet, Data Packet, Handshake Packet, Special Packet, Error.</p> <p>Token packet trigger – Any token type, SOF, OUT, IN, SETUP; Address can be specified for Any Token, OUT, IN, and SETUP token types. Address can be further specified to trigger on <math>\leq</math>, <math>&lt;</math>, <math>=</math>, <math>&gt;</math>, <math>\geq</math>, <math>\neq</math> a particular value, or inside or outside of a range. Frame number can be specified for SOF token using binary, hex, unsigned decimal and don't care digits.</p> <p>Data packet trigger – Any data type, DATA0, DATA1; Data can be further specified to trigger on <math>\leq</math>, <math>&lt;</math>, <math>=</math>, <math>&gt;</math>, <math>\geq</math>, <math>\neq</math> a particular data value, or inside or outside of a range.</p> <p>Handshake packet trigger – Any handshake type, ACK, NAK, STALL.</p> <p>Special packet trigger – Any special type, PRE, Reserved.</p> <p>Error trigger – PID Check, CRC5 or CRC16, Bit Stuffing.</p> <hr/> <p>High-speed: Trigger on Sync, Reset, Suspend, Resume, End of Packet, Token (Address) Packet, Data Packet, Handshake Packet, Special Packet, Error.</p> <p>Token packet trigger – Any token type, SOF, OUT, IN, SETUP; Address can be specified for Any Token, OUT, IN, and SETUP token types. Address can be further specified to trigger on <math>\leq</math>, <math>&lt;</math>, <math>=</math>, <math>&gt;</math>, <math>\geq</math>, <math>\neq</math> a particular value, or inside or outside of a range. Frame number can be specified for SOF token using binary, hex, unsigned decimal and don't care digits.</p> <p>Data packet trigger – Any data type, DATA0, DATA1, DATA2, DATAM; Data can be further specified to trigger on <math>\leq</math>, <math>&lt;</math>, <math>=</math>, <math>&gt;</math>, <math>\geq</math>, <math>\neq</math> a particular data value, or inside or outside of a range.</p> <p>Handshake packet trigger – Any handshake type, ACK, NAK, STALL, NYET.</p> <p>Special packet trigger – Any special type, ERR, SPLIT, PING, Reserved. SPLIT packet components that can be specified include:</p> <ul style="list-style-type: none"> <li>Hub Address</li> <li>Start/Complete – Don't Care, Start (SSPLIT), Complete (CSPLIT)</li> <li>Port Address</li> <li>Start and End bits – Don't Care, Control/Bulk/Interrupt (Full-speed Device, Low-speed Device), Isochronous (Data is Middle, Data is End, Data is Start, Data is All)</li> <li>Endpoint Type – Don't Care, Control, Isochronous, Bulk, Interrupt</li> </ul> <p>Error trigger – PID Check, CRC5 or CRC16, Any.</p> <hr/> <p>High-speed support only available on MDO4104-3 and MDO4104-6 models.</p> |
| Ethernet (Optional)            | <p>10BASE-T: Trigger on Start Frame Delimiter, MAC Addresses, MAC Q-Tag Control Information, MAC Length/Type, IP Header, TCP Header, TCP/IPV4/MAC Client Data, End of Packet, FCS (CRC) Error.</p> <p>MAC Addresses – Trigger on Source and Destination 48-bit address values.</p> <p>MAC Q-Tag Control Information – Trigger on Q-Tag 32-bit value.</p> <p>MAC Length/Type – Trigger on <math>\leq</math>, <math>&lt;</math>, <math>=</math>, <math>&gt;</math>, <math>\geq</math>, <math>\neq</math> a particular 16-bit value, or inside or outside of a range.</p> <p>IP Header – Trigger on IP Protocol 8-bit value, Source Address, Destination Address.</p> <p>TCP Header – Trigger on Source Port, Destination Port, Sequence Number, and Ack Number.</p> <p>TCP/IPV4/MAC Client Data – Trigger on <math>\leq</math>, <math>&lt;</math>, <math>=</math>, <math>&gt;</math>, <math>\geq</math>, <math>\neq</math> a particular data value, or inside or outside of a range. Selectable number of bytes to trigger on from 1-16. Byte offset options of Don't Care, 0-1499.</p> <hr/> <p>100BASE-TX: Trigger on Start Frame Delimiter, MAC Addresses, MAC Q-Tag Control Information, MAC Length/Type, IP Header, TCP Header, TCP/IPV4/MAC Client Data, End of Packet, FCS (CRC) Error, Idle.</p> <p>MAC Addresses – Trigger on Source and Destination 48-bit address values.</p> <p>MAC Q-Tag Control Information – Trigger on Q-Tag 32-bit value.</p> <p>MAC Length/Type – Trigger on <math>\leq</math>, <math>&lt;</math>, <math>=</math>, <math>&gt;</math>, <math>\geq</math>, <math>\neq</math> a particular 16-bit value, or inside or outside of a range.</p> <p>IP Header – Trigger on IP Protocol 8-bit value, Source Address, Destination Address.</p> <p>TCP Header – Trigger on Source Port, Destination Port, Sequence Number, and Ack Number.</p> <p>TCP/IPV4/MAC Client Data – Trigger on <math>\leq</math>, <math>&lt;</math>, <math>=</math>, <math>&gt;</math>, <math>\geq</math>, <math>\neq</math> a particular data value, or inside or outside of a range. Selectable number of bytes to trigger on from 1-16. Byte offset options of Don't Care, 0-1499.</p>   |
| CAN (Optional)                 | <p>Trigger on Start of Frame, Frame Type (data, remote, error, overload), Identifier (standard or extended), Data, Identifier and Data, End of Frame, Missing ACK, or Bit Stuffing Error on CAN signals up to 1 Mb/s. Data can be further specified to trigger on <math>\leq</math>, <math>&lt;</math>, <math>=</math>, <math>&gt;</math>, <math>\geq</math>, or <math>\neq</math> a specific data value. User-adjustable sample point is set to 50% by default</p>   |
| LIN (Optional)                 | <p>Trigger on Sync, Identifier, Data, Identifier and Data, Wakeup Frame, Sleep Frame, Errors such as Sync, Parity, or Checksum Errors up to 100 Kb/s (by LIN definition, 20 Kb/s)</p>   |
| FlexRay (Optional)             | <p>Trigger on Start of Frame, Type of Frame (Normal, Payload, Null, Sync, Startup), Identifier, Cycle Count, Complete Header Field, Data, Identifier and Data, End of Frame or Errors such as Header CRC, Trailer CRC, Null Frame, Sync Frame, or Startup Frame Errors up to 100 Mb/s</p>   |
| RS-232/422/485/UART (Optional) | <p>Trigger on Tx Start Bit, Rx Start Bit, Tx End of Packet, Rx End of Packet, Tx Data, Rx Data, Tx Parity Error, and Rx Parity Error up to 10 Mb/s</p>  |

| Mode                                  | Description  |
|---------------------------------------|--|
| MIL-STD-1553 (Optional)               | Trigger on Sync, Word Type*1 (Command, Status, Data), Command Word*1 (set RT Address, T/R, Sub-address/Mode, Data Word Count/Mode Code, and Parity individually), Status Word*1 (set RT Address, Message Error, Instrumentation, Service Request Bit, Broadcast Command Received, Busy, Subsystem Flag, Dynamic Bus Control Acceptance (DBCA), Terminal Flag, and Parity individually), Data Word (user-specified 16-bit data value), Error (Sync, Parity, Manchester, Non-contiguous data), Idle Time (minimum time selectable from 4 $\mu$ s to 100 $\mu$ s; maximum time selectable from 12 $\mu$ s to 100 $\mu$ s; trigger on < minimum, > maximum, inside range, outside range). RT Address can be further specified to trigger on =, $\neq$ , <, >, $\leq$ , $\geq$ a particular value, or inside or outside of a range. |
| I <sup>2</sup> S/LJ/RJ/TDM (Optional) | Trigger on Word Select, Frame Sync, or Data. Data can be further specified to trigger on $\leq$ , <, =, >, $\geq$ , $\neq$ a specific data value, or inside or outside of a range<br>Maximum data rate for I <sup>2</sup> S/LJ/RJ is 12.5 Mb/s<br>Maximum data rate for TDM is 25 Mb/s   |
| Parallel                              | Trigger on a parallel bus data value. Parallel bus can be from 1 to 20 bits in size. Binary and Hex radices are supported  |

\*1 Trigger selection of Command Word will trigger on Command and ambiguous Command/Status words. Trigger selection of Status Word will trigger on Status and ambiguous Command/Status words.

### Acquisition Modes

| Mode        | Description   |
|-------------|---|
| Sample      | Acquire sampled values  |
| Peak Detect | Captures glitches as narrow as 800 ps (1 GHz models) or 1.6 ns (500 MHz models) at all sweep speeds |
| Averaging   | From 2 to 512 waveforms included in average   |
| Envelope    | Min-Max envelope reflecting Peak Detect data over multiple acquisitions                             |
| Hi Res      | Real-time boxcar averaging reduces random noise and increases vertical resolution                   |
| Roll        | Scrolls waveforms right to left across the screen at sweep speeds slower than or equal to 40 ms/div |

### Waveform Measurements

| Measurement                               | Description   |
|---|---|
| Cursors                                   | Waveform and Screen   |
| Automatic Measurements – Time Domain      | 29, of which up to eight can be displayed on-screen at any one time. Measurements include: Period, Frequency, Delay, Rise Time, Fall Time, Positive Duty Cycle, Negative Duty Cycle, Positive Pulse Width, Negative Pulse Width, Burst Width, Phase, Positive Overshoot, Negative Overshoot, Peak-to-Peak, Amplitude, High, Low, Max, Min, Mean, Cycle Mean, RMS, Cycle RMS, Positive Pulse Count, Negative Pulse Count, Rising Edge Count, Falling Edge Count, Area and Cycle Area |
| Automatic Measurements – Frequency Domain | 3, of which one can be displayed on-screen at any one time. Measurements include Channel Power, Adjacent Channel Power Ratio (ACPR), and Occupied Bandwidth (OBW)   |
| Measurement Statistics                    | Mean, Min, Max, Standard Deviation  |
| Reference Levels                          | User-definable reference levels for automatic measurements can be specified in either percent or units  |
| Gating                                    | Isolate the specific occurrence within an acquisition to take measurements on, using either the screen or waveform cursors  |
| Waveform Histogram                        | A waveform histogram provides an array of data values representing the total number of hits inside of a user-defined region of the display. A waveform histogram is both a visual graph of the hit distribution as well as a numeric array of values that can be measured.<br>Sources – Channel 1, Channel 2, Channel 3, Channel 4, Ref 1, Ref 2, Ref 3, Ref 4, Math<br>Types – Vertical, Horizontal  |
| Waveform Histogram Measurements           | Waveform Count, Hits in Box, Peak Hits, Median, Max, Min, Peak-to-Peak, Mean, Standard Deviation, Sigma 1, Sigma 2, Sigma 3   |



**Waveform Math**

| Characteristic | Description  |
|----------------|--|
| Arithmetic     | Add, subtract, multiply, and divide waveforms  |
| Math Functions | Integrate, Differentiate, FFT  |
| FFT            | Spectral magnitude<br>FFT Vertical Scale: Linear RMS or dBV RMS<br>FFT Window Settings: Rectangular, Hamming, Hanning, Blackman Harris   |
| Spectrum Math  | Add or subtract frequency domain traces  |
| Advanced Math  | Define extensive algebraic expressions including waveforms, reference waveforms, math functions. Perform math on math using complex equations (FFT, Intg, Diff, Log, Exp, Sqrt, Abs, Sine, Cosine, Tangent, Rad, Deg), scalars, up to two user-adjustable variables and results of parametric measurements (Period, Freq, Delay, Rise, Fall, PosWidth, NegWidth, BurstWidth, Phase, PosDutyCycle, NegDutyCycle, PosOverShoot, NegOverShoot, PeakPeak, Amplitude, RMS, CycleRMS, High, Low, Max, Min, Mean, CycleMean, Area, CycleArea, and trend plots) e.g. $(\text{Intg}(\text{Ch1} - \text{Mean}(\text{Ch1})) \times 1.414 \times \text{VAR1})$ |

**Power Measurements (Optional)**

| Measurement                  | Description  |
|------------------------------|--|
| Power Quality Measurements   | $V_{\text{RMS}}$ , $V_{\text{Crest Factor}}$ , Frequency, $I_{\text{RMS}}$ , $I_{\text{Crest Factor}}$ , True Power, Apparent Power, Reactive Power, Power Factor, Phase Angle |
| Switching Loss Measurements  | Power Loss: $T_{\text{on}}$ , $T_{\text{off}}$ , Conduction, Total<br>Energy Loss: $T_{\text{on}}$ , $T_{\text{off}}$ , Conduction, Total                                      |
| Harmonics                    | THD-F, THD-R, RMS measurements<br>Graphical and table displays of harmonics<br>Test to IEC61000-3-2 Class A and MIL-STD-1399 Section 300A                                      |
| Ripple Measurements          | $V_{\text{ripple}}$ and $I_{\text{ripple}}$  |
| Modulation Analysis          | Graphical display of +Pulse Width, -Pulse Width, Period, Frequency, +Duty Cycle, and -Duty Cycle modulation types  |
| Safe Operating Area          | Graphical display and mask testing of switching device safe operating area measurements  |
| dV/dt and dI/dt Measurements | Cursor measurements of slew rate   |

**Limit/Mask Testing (Optional)**

| Characteristic           | Description  |
|--------------------------|--|
| Included Standard Masks  | ITU-T, ANSI T1.102, USB  |
| Test Source              | Limit Test: Any Ch1 - Ch4 or any R1 - R4<br>Mask Test: Any Ch1 - Ch4   |
| Mask Creation            | Limit test vertical tolerance from 0 to 1 division in 1 m division increments; Limit test horizontal tolerance from 0 to 500 m division in 1 m division increments<br>Load standard mask from internal memory<br>Load custom mask from text file with up to 8 segments |
| Mask Scaling             | Lock to Source ON (mask automatically re-scales with source-channel settings changes)<br>Lock to Source OFF (mask does not re-scale with source-channel settings changes)  |
| Test Criteria Run Until  | Minimum number of waveforms (from 1 to 1,000,000; Infinity)<br>Minimum elapsed time (from 1 second to 48 hours; Infinity)  |
| Violation Threshold      | From 1 to 1,000,000  |
| Actions on Test Failure  | Stop acquisition, save screen image to file, save waveform to file, print screen image, trigger out pulse, set remote interface SRQ  |
| Actions on Test Complete | Trigger out pulse, set remote interface SRQ  |
| Results Display          | Test status, total waveforms, number of violations, violation rate, total tests, failed tests, test failure rate, elapsed time, total hits for each mask segment   |

**Software**

| Software                                      | Description  |
|---|--|
| NI LabVIEW<br>SignalExpress Tektronix Edition | A fully interactive measurement software environment optimized for the MDO4000 Series, enables you to instantly acquire, generate, analyze, compare, import, and save measurement data and signals using an intuitive drag-and-drop user interface that does not require any programming.<br>Standard MDO4000 Series support for acquiring, controlling, viewing, and exporting your live signal data is permanently available through the software. The full version (SIGEXPTE) adds additional signal processing, advanced analysis, mixed signal, sweeping, limit testing, and user-defined step capabilities and is available for a 30-day trial period standard with each instrument. |
| OpenChoice® Desktop                           | Enables fast and easy communication between a Windows PC and the MDO4000 Series, using USB or LAN. Transfer and save settings, waveforms, measurements, and screen images. Included Word and Excel toolbars automate the transfer of acquisition data and screen images from the oscilloscope into Word and Excel for quick reporting or further analysis.   |
| IVI Driver                                    | Provides a standard instrument programming interface for common applications such as LabVIEW, LabWindows/CVI, Microsoft .NET and MATLAB.   |
| e*Scope® Web-based Remote Control             | Enables control of the MDO4000 Series over a network connection through a standard web browser. Simply enter the IP address or network name of the oscilloscope and a web page will be served to the browser.  |
| LXI Class C Web Interface                     | Connect to the MDO4000 Series through a standard web browser by simply entering the oscilloscope's IP address or network name in the address bar of the browser. The web interface enables viewing of instrument status and configuration, status and modification of network settings, and instrument control through the e*scope web-based remote control. All web interaction conforms to LXI Class C specification.  |

**Display Characteristics**

| Characteristic        | Description   |
|-----------------------|---|
| Display Type          | 10.4 in. (264 mm) liquid-crystal TFT color display        |
| Display Resolution    | 1,024 horizontal × 768 vertical pixels (XGA)              |
| Waveform Styles       | Vectors, Dots, Variable Persistence, Infinite Persistence |
| Graticules            | Full, Grid, Solid, Cross Hair, Frame, IRE, and mV         |
| Format                | YT and simultaneous XY/YT                                 |
| Waveform Capture Rate | >50,000 wfms/s maximum                                    |

**Input/Output Ports**

| Port                         | Description   |
|------------------------------|---|
| USB 2.0 High-speed Host Port | Supports USB mass storage devices, printers and keyboard. Two ports on front and two ports on rear of instrument  |
| USB 2.0 Device Port          | Rear-panel connector allows for communication/control of oscilloscope through USBTMC or GPIB (with a TEK-USB-488), and direct printing to all PictBridge-compatible printers  |
| LAN Port                     | RJ-45 connector, supports 10/100/1000 Mb/s  |
| XGA Video Port               | DB-15 female connector, connect to show the oscilloscope display on an external monitor or projector  |
| Probe Compensator Output     | Front-panel pins<br>Amplitude: 2.5 V<br>Frequency: 1 kHz  |
| Auxiliary Out                | Rear-panel BNC connector<br>$V_{OUT} (Hi)$ : $\geq 2.5$ V open circuit, $\geq 1.0$ V 50 $\Omega$ to ground<br>$V_{OUT} (Lo)$ : $\leq 0.7$ V into a load of $\leq 4$ mA; $\leq 0.25$ V 50 $\Omega$ to ground<br><br>Output can be configured to provide a pulse out signal when the oscilloscope triggers, the internal oscilloscope reference clock out, or an event out for limit/mask testing |
| External Reference In        | Time-base system can phase lock to an external 10 MHz reference (10 MHz $\pm 1\%$ )   |
| Kensington Lock              | Rear-panel security slot connects to standard Kensington lock   |
| VESA Mount                   | Standard (MIS-D 100) 100 mm VESA mounting points on rear of instrument  |

**LAN eXtensions for Instrumentation (LXI)**

| Characteristic | Description |
|----------------|-------------|
| Class          | LXI Class C |
| Version        | V1.3        |

**Power Source**

| Characteristic         | Description   |
|------------------------|---|
| Power Source Voltage   | 100 to 240 V $\pm 10\%$                                   |
| Power Source Frequency | 45 to 66 Hz (85 to 264 V)<br>360 to 440 Hz (100 to 132 V) |
| Power Consumption      | 225 W maximum   |

**Physical Characteristics**

| Dimensions              | mm   | in.  |
|-------------------------|--|------|
| Height                  | 229  | 9.0  |
| Width                   | 439  | 17.3 |
| Depth                   | 147  | 5.8  |
| Weight                  | kg   | lb.  |
| Net                     | 5  | 11   |
| Shipping                | 10.7   | 23.6 |
| Rackmount Configuration | 5U   |      |
| Cooling Clearance       | 2 in. (51 mm) required on left side and rear of instrument |      |

**Environmental**

| Characteristic                | Description  |
|-------------------------------|--|
| Temperature                   |  |
| Operating                     | 0 °C to +50 °C   |
| Nonoperating                  | -20 °C to +60 °C   |
| Humidity                      |  |
| Operating                     | High: 40 °C to 50 °C, 10% to 60% Relative Humidity<br>Low: 0 °C to 40 °C, 10% to 90% Relative Humidity |
| Nonoperating                  | High: 40 °C to 60 °C, 5% to 60% Relative Humidity<br>Low: 0 °C to 40 °C, 5% to 90% Relative Humidity   |
| Altitude                      |  |
| Operating                     | 9,843 ft. (3,000 m)  |
| Nonoperating                  | 30,000 ft. (9,144 m)   |
| Regulatory                    |  |
| Electromagnetic Compatibility | EC Council Directive 2004/108/EC   |
| Safety                        | UL61010-1, Second Edition; CSA61010-1 Second Edition, EN61010-1:2001; IEC 61010-1:2001                 |

**Ordering Information****MDO4000 Family**

| Model     | Description   |
|-----------|---|
| MDO4054-3 | Mixed Domain Oscilloscope with (4) 500 MHz analog channels, (16) digital channels, and (1) 3 GHz RF input |
| MDO4054-6 | Mixed Domain Oscilloscope with (4) 500 MHz analog channels, (16) digital channels, and (1) 6 GHz RF input |
| MDO4104-3 | Mixed Domain Oscilloscope with (4) 1 GHz analog channels, (16) digital channels, and (1) 3 GHz RF input   |
| MDO4104-6 | Mixed Domain Oscilloscope with (4) 1 GHz analog channels, (16) digital channels, and (1) 6 GHz RF input   |

**All Models Include:** One passive voltage probe per analog channel (TPP0500 500 MHz, 10X, 3.9 pF for 500 MHz models; TPP1000 1 GHz, 10X, 3.9 pF for 1 GHz models), P6616 16-channel Logic Probe, Logic Probe Accessory Kit (020-2662-xx), Front Cover (200-5130-xx), N-to-BNC Adapter (103-0045-00), User Manual (071-2918-xx), Documentation CD (063-4367-xx), OpenChoice® Desktop Software, NI LabVIEW SignalExpress™ Tektronix Edition Software, Calibration Certificates document measurement traceability to National Metrology Institute(s) – the Quality System this product is manufactured in is ISO9001 registered, power cord, accessory bag (016-2030-xx) and a three-year warranty. Please specify power plug and manual language version when ordering.

## Application Modules

Application modules have licenses which can be transferred between an application module and an oscilloscope. The license may be contained in the module; allowing the module to be moved from one instrument to another. Or, the license can be contained in the oscilloscope; allowing the module to be removed and stored for safekeeping. Transferring the license to an oscilloscope and removing the module permits the use of more than 4 applications simultaneously.

| Module      | Description   |
|-------------|---|
| DPO4AERO    | Aerospace Serial Triggering and Analysis Module. Enables triggering on packet-level information on MIL-STD-1553 buses as well as analytical tools such as digital views of the signal, bus views, packet decoding, search tools, and packet decode tables with time-stamp information.<br>Signal Inputs – Any Ch1 - Ch4, Math, Ref1 - Ref4<br>Recommended Probing – Differential or single ended (only one single-ended signal required)  |
| DPO4AUDIO   | Audio Serial Triggering and Analysis Module. Enables triggering on packet-level information on I <sup>2</sup> S, LJ, RJ, and TDM audio buses as well as analytical tools such as digital views of the signal, bus views, packet decoding, search tools, and packet decode tables with time-stamp information.<br>Signal Inputs – Any Ch1 - Ch4, D0 - D15<br>Recommended Probing – I <sup>2</sup> S, LJ, RJ, TDM: Single ended   |
| DPO4AUTO    | Automotive Serial Triggering and Analysis Module. Enables triggering on packet-level information on CAN and LIN buses as well as analytical tools such as digital views of the signal, bus views, packet decoding, search tools, and packet decode tables with time-stamp information.<br>Signal Inputs – LIN: Any Ch1 - Ch4, D0 - D15; CAN: Any Ch1 - Ch4, (D0 - D15; single-ended probing only)<br>Recommended Probing – LIN: Single ended; CAN: Single ended or differential   |
| DPO4AUTOMAX | Extended Automotive Serial Triggering and Analysis Module. Enables triggering on packet-level information on CAN, LIN, and FlexRay buses as well as analytical tools such as digital views of the signal, bus views, packet decoding, search tools, packet decode tables with time-stamp information, and eye diagram analysis software.<br>Signal Inputs – LIN: Any Ch1 - Ch4, D0 - D15; CAN: Any Ch1 - Ch4, (D0 - D15; single-ended probing only); FlexRay: Any Ch1 - Ch4, (D0 - D15; single-ended probing only)<br>Recommended Probing – LIN: Single ended; CAN, FlexRay: Single ended or differential |
| DPO4COMP    | Computer Serial Triggering and Analysis Module. Enables triggering on packet-level information on RS-232/422/485/UART buses as well as analytical tools such as digital views of the signal, bus views, packet decoding, search tools, and packet decode tables with time-stamp information.<br>Signal Inputs – Any Ch1 - Ch4, (D0 - D15; single-ended probing only)<br>Recommended Probing – RS-232/UART: Single ended; RS-422/485: Differential   |

| Module   | Description   |
|----------|---|
| DPO4EMBD | Embedded Serial Triggering and Analysis Module. Enables triggering on packet-level information on I <sup>2</sup> C and SPI buses as well as analytical tools such as digital views of the signal, bus views, packet decoding, search tools, and packet decode tables with time-stamp information.<br>Signal Inputs – I <sup>2</sup> C: Any Ch1 - Ch4, D0 - D15; SPI: Any Ch1 - Ch4, D0 - D15<br>Recommended Probing – I <sup>2</sup> C, SPI: Single ended   |
| DPO4ENET | Ethernet Serial Triggering and Analysis Module. Enables triggering on packet-level information on 10BASE-T and 100BASE-TX buses as well as analytical tools such as digital views of the signal, bus views, packet decoding, search tools, and packet decode tables with time-stamp information.<br>Signal Inputs – Any Ch1 - Ch4 for single-ended probing; Any Ch1 - Ch4, Math, Ref1 - Ref4 for differential probing<br>Recommended Probing – 10BASE-T: Single ended or differential; 100BASE-TX: Differential   |
| DPO4USB  | USB Serial Triggering and Analysis Module. Enables triggering on packet-level content for low-speed, full-speed, and high-speed USB serial buses. Also enables analytical tools such as digital views of the signal, bus views, packet decoding, search tools, and packet decode tables with time-stamp information for low-speed, full-speed, and high-speed USB serial buses.<br>Signal Inputs – Low-speed and Full-speed: Any Ch1 - Ch4, (D0 - D15; for single-ended probing only); Low-speed, Full-speed, and High-speed: Any Ch1 - Ch4, Math, Ref1 - Ref4<br>Recommended Probing – Low-speed and Full-speed: Single ended or differential; High-speed: Differential<br>USB high-speed supported only on MDO4104-X models |
| DPO4PWR  | Power Analysis Application Module. Enables quick and accurate analysis of power quality, switching loss, harmonics, safe operating area (SOA), modulation, ripple, and slew rate (dI/dt, dV/dt)   |
| DPO4LMT  | Limit and Mask Testing Application Module. Enables testing against limit templates generated from "golden" waveforms and mask testing using custom or standard telecommunications or computer masks   |
| DPO4VID  | HDTV and Custom (nonstandard) Video Triggering Module   |
| MDO4TRIG | Advanced RF Power Level Triggering Module. Enables the power level on the RF input to be used as a source in the following trigger types: Pulse Width, Runt, Timeout, Logic, and Sequence   |

## Instrument Options

### Power Plug Options

| Option   | Description                 |
|----------|-----------------------------|
| Opt. A0  | North America               |
| Opt. A1  | Universal Euro              |
| Opt. A2  | United Kingdom              |
| Opt. A3  | Australia                   |
| Opt. A5  | Switzerland                 |
| Opt. A6  | Japan                       |
| Opt. A10 | China                       |
| Opt. A11 | India                       |
| Opt. A12 | Brazil                      |
| Opt. A99 | No power cord or AC adapter |

### Language Options\*2

| Option   | Description                |
|----------|----------------------------|
| Opt. L0  | English manual             |
| Opt. L1  | French manual              |
| Opt. L2  | Italian manual             |
| Opt. L3  | German manual              |
| Opt. L4  | Spanish manual             |
| Opt. L5  | Japanese manual            |
| Opt. L6  | Portuguese manual          |
| Opt. L7  | Simplified Chinese manual  |
| Opt. L8  | Traditional Chinese manual |
| Opt. L9  | Korean manual              |
| Opt. L10 | Russian manual             |
| Opt. L99 | No manual                  |

\*2 Language options include a translated front-panel overlay for the selected language(s).

### Service Options\*3

| Option  | Description   |
|---------|---|
| Opt. C3 | Calibration Service 3 years   |
| Opt. C5 | Calibration Service 5 years   |
| Opt. D1 | Calibration Data Report   |
| Opt. D3 | Calibration Data Report 3 years (with Opt. C3)                          |
| Opt. D5 | Calibration Data Report 5 Years (with Opt. C5)                          |
| Opt. G3 | Complete Care 3 Years (includes loaner, scheduled calibration and more) |
| Opt. G5 | Complete Care 5 Years (includes loaner, scheduled calibration and more) |
| Opt. R5 | Repair Service 5 years (including warranty)                             |

\*3 Probes and accessories are not covered by the oscilloscope warranty and service offerings. Refer to the datasheet of each probe and accessory model for its unique warranty and calibration terms.

### Recommended Probes

Tektronix offers over 100 different probes to meet your application needs. For a comprehensive listing of available probes, please visit [www.tektronix.com/probes](http://www.tektronix.com/probes).

| Probe    | Description   |
|----------|---|
| TPP0500  | 500 MHz, 10X TekVPI® passive voltage probe with 3.9 pF input capacitance              |
| TPP0502  | 500 MHz, 2X TekVPI passive voltage probe with 3.9 pF input capacitance                |
| TPP0850  | 2.5 kV, 800 MHz, 50X TekVPI passive high-voltage probe                                |
| TPP1000  | 1 GHz, 10X TekVPI passive voltage probe with 3.9 pF input capacitance                 |
| TAP1500  | 1.5 GHz TekVPI active single-ended voltage probe                                      |
| TAP2500  | 2.5 GHz TekVPI active single-ended voltage probe                                      |
| TAP3500  | 3.5 GHz TekVPI active single-ended voltage probe                                      |
| TDP0500  | 500 MHz TekVPI differential voltage probe with $\pm 42$ V differential input voltage  |
| TDP1000  | 1 GHz TekVPI differential voltage probe with $\pm 42$ V differential input voltage    |
| TDP1500  | 1.5 GHz TekVPI differential voltage probe with $\pm 8.5$ V differential input voltage |
| TDP3500  | 3.5 GHz TekVPI differential voltage probe with $\pm 2$ V differential input voltage   |
| TCP0030  | 120 MHz TekVPI 30 Ampere AC/DC current probe  |
| TCP0150  | 20 MHz TekVPI 150 Ampere AC/DC current probe  |
| P5200A   | 1.3 kV, 50 MHz high-voltage differential probe  |
| P5202A*4 | 640 V, 100 MHz high-voltage differential probe  |
| P5205A*4 | 1.3 kV, 200 MHz high-voltage differential probe                                       |
| P5210A*4 | 5.6 kV, 50 MHz high-voltage differential probe  |
| P5100A   | 2.5 kV, 100X high-voltage passive probe   |

\*4 Requires TekVPI® to TekProbe BNC adapter (TPA-BNC).

### Recommended Accessories

| Accessory   | Description   |
|-------------|---|
| 119-4146-00 | Near Field Probe Set, 100 kHz - 1 GHz                               |
| 119-6609-00 | Flexible Monopole Antenna   |
| TPA-N-VPI   | N-to-TekVPI Adapter   |
| 077-0585-xx | Service Manual (English only)                                       |
| SIGEXPT     | NI LabVIEW SignalExpress™ Tektronix Edition Software (Full Version) |
| FPGAView-xx | MSO Support for Altera and Xilinx FPGAs                             |
| TPA-BNC     | TekVPI-to-TekProbe BNC Adapter                                      |
| TEK-USB-488 | GPIO-to-USB Adapter   |
| ACD4000B    | Soft Transit Case   |
| HCTEK54     | Hard Transit Case (Requires ACD4000B)                               |
| RMD5000     | Rackmount Kit   |
| TEK-DPG     | Deskew Pulse Generator  |
| 067-1686-xx | Deskew Fixture  |

### Warranty

Three-year warranty covering all parts and labor, excluding probes.



Product(s) are manufactured in ISO registered facilities.



Product(s) complies with IEEE Standard 488.1-1987, RS-232-C, and with Tektronix Standard Codes and Formats.



Contact Tektronix:

- ASEAN / Australasia (65) 6356 3900
- Austria 00800 2255 4835\*
- Balkans, Israel, South Africa and other ISE Countries +41 52 675 3777
- Belgium 00800 2255 4835\*
- Brazil +55 (11) 3759 7627
- Canada 1 800 833 9200
- Central East Europe and the Baltics +41 52 675 3777
- Central Europe & Greece +41 52 675 3777
- Denmark +45 80 88 1401
- Finland +41 52 675 3777
- France 00800 2255 4835\*
- Germany 00800 2255 4835\*
- Hong Kong 400 820 5835
- India 000 800 650 1835
- Italy 00800 2255 4835\*
- Japan 81 (3) 6714 3010
- Luxembourg +41 52 675 3777
- Mexico, Central/South America & Caribbean 52 (55) 56 04 50 90
- Middle East, Asia, and North Africa +41 52 675 3777
- The Netherlands 00800 2255 4835\*
- Norway 800 16098
- People's Republic of China 400 820 5835
- Poland +41 52 675 3777
- Portugal 80 08 12370
- Republic of Korea 001 800 8255 2835
- Russia & CIS +7 (495) 7484900
- South Africa +41 52 675 3777
- Spain 00800 2255 4835\*
- Sweden 00800 2255 4835\*
- Switzerland 00800 2255 4835\*
- Taiwan 886 (2) 2722 9622
- United Kingdom & Ireland 00800 2255 4835\*
- USA 1 800 833 9200

\* European toll-free number. If not accessible, call: +41 52 675 3777

Updated 10 February 2011



**For Further Information.** Tektronix maintains a comprehensive, constantly expanding collection of application notes, technical briefs and other resources to help engineers working on the cutting edge of technology. Please visit [www.tektronix.com](http://www.tektronix.com)



Copyright © Tektronix, Inc. All rights reserved. Tektronix products are covered by U.S. and foreign patents, issued and pending. Information in this publication supersedes that in all previously published material. Specification and price change privileges reserved. TEKTRONIX and TEK are registered trademarks of Tektronix, Inc. All other trade names referenced are the service marks, trademarks, or registered trademarks of their respective companies.

12 Jul 2011 48W-26875-0

