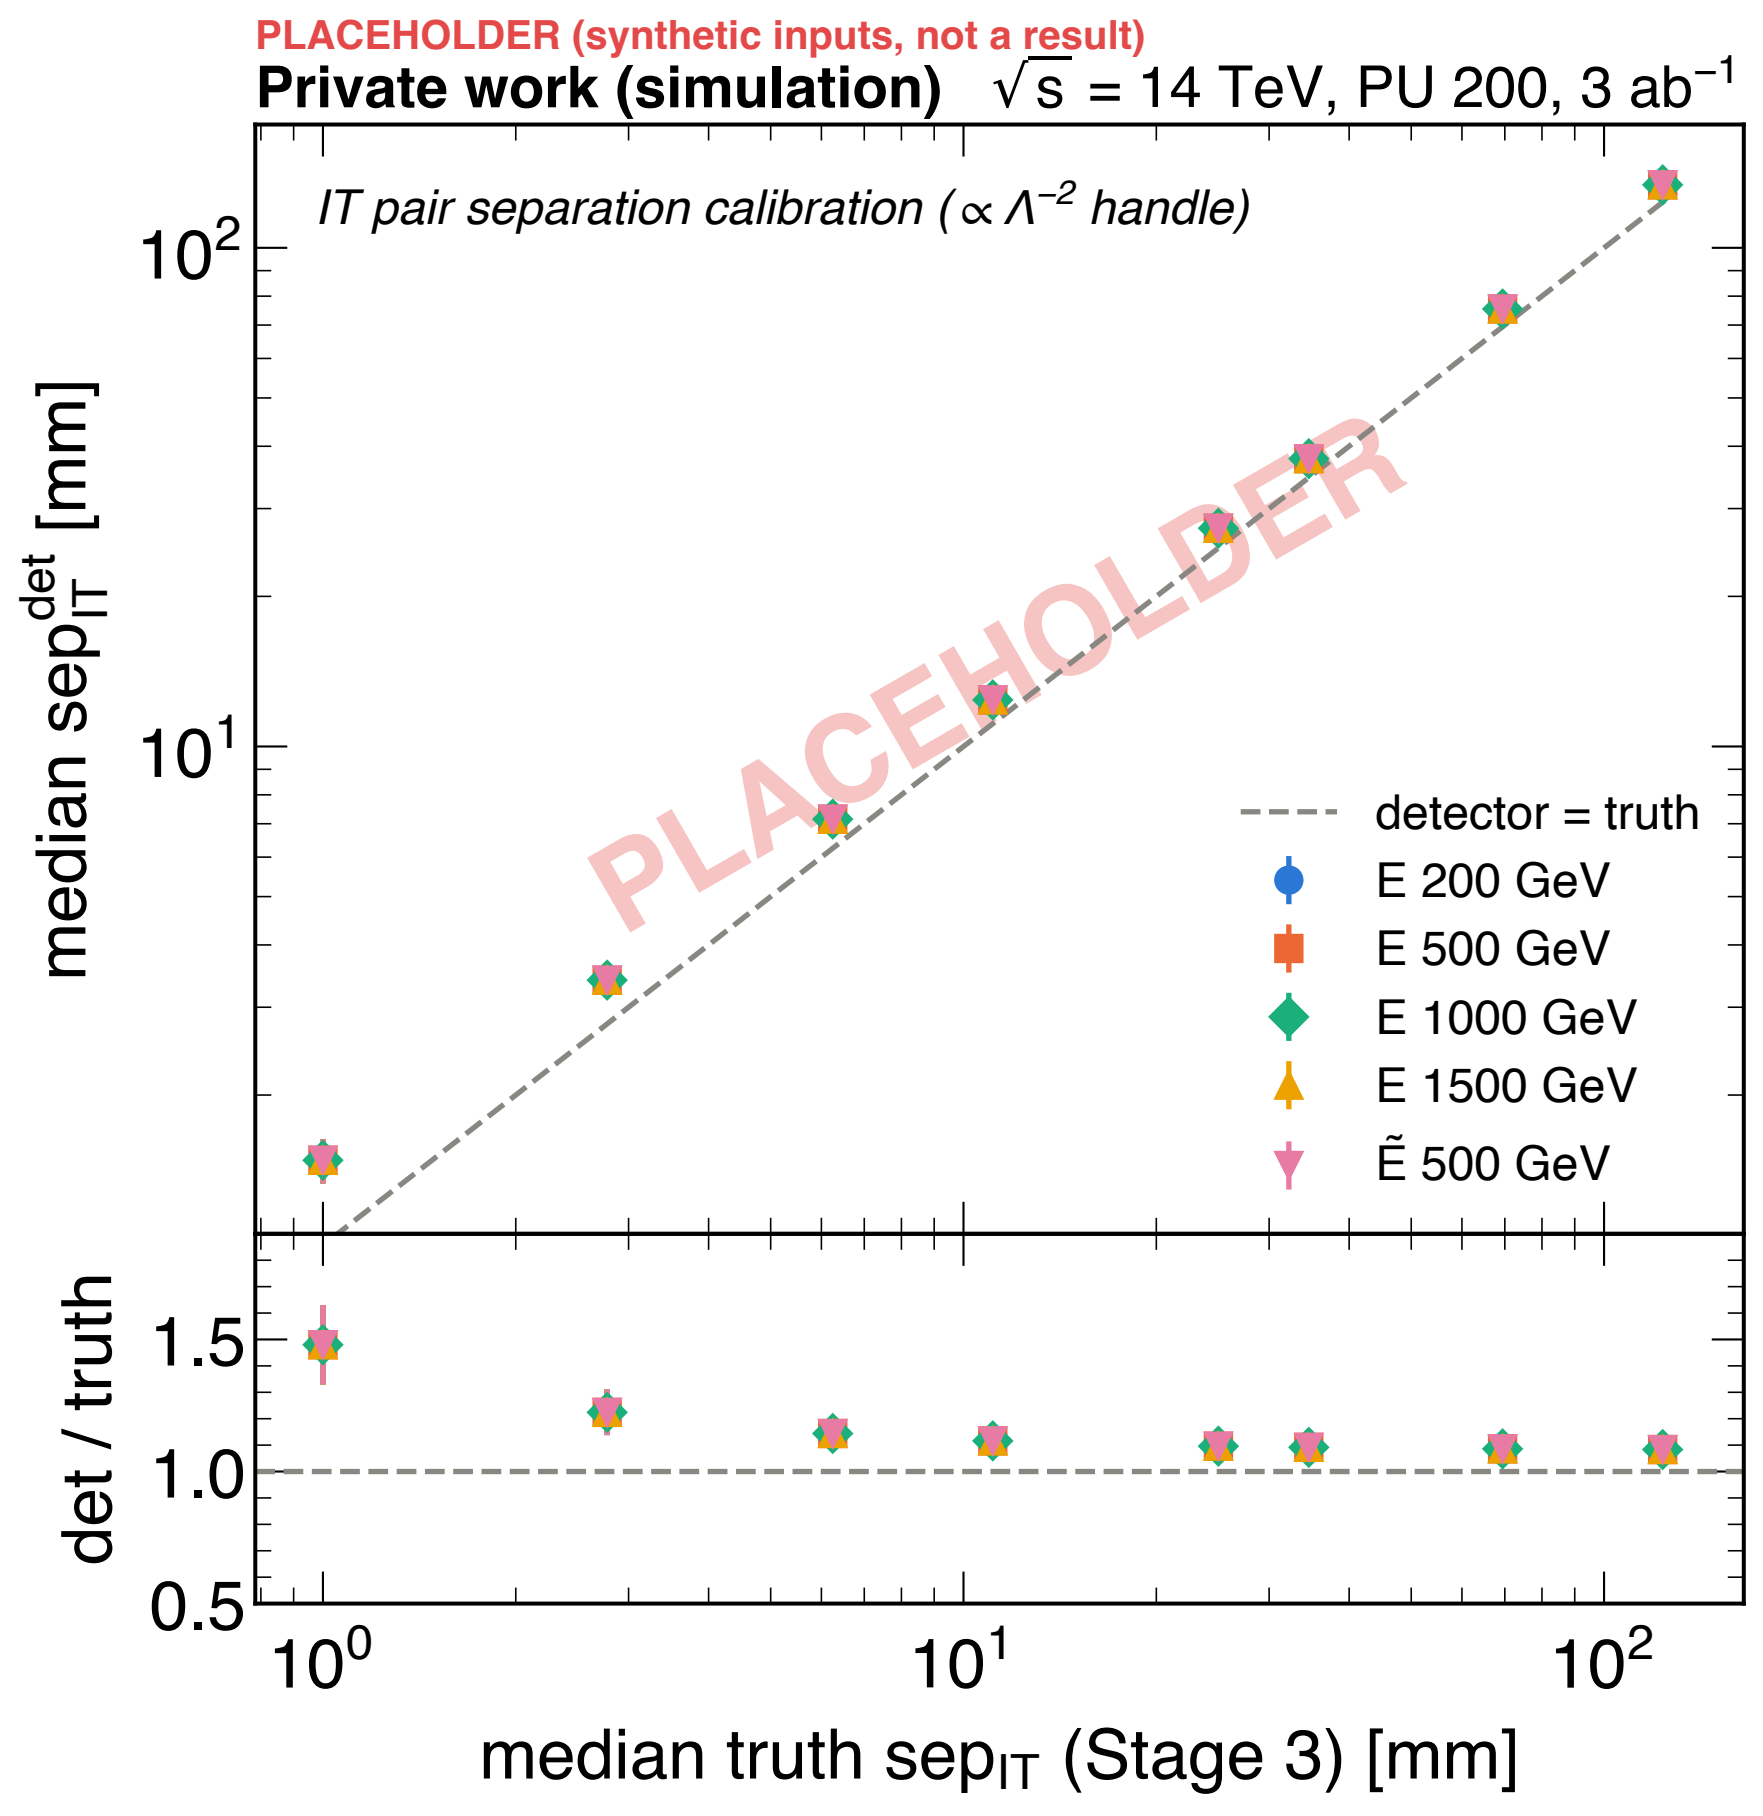
PLACEHOLDER (synthetic inputs, not a result)
Private work (simulation) √s = 14 TeV, PU 200, 3 ab⁻¹
IT pair separation calibration (∝ Λ⁻² handle)
PLACEHOLDER
median sep$_{IT}^{det}$ [mm]
detector = truth
E 200 GeV
E 500 GeV
E 1000 GeV
E 1500 GeV
Ẽ 500 GeV
det / truth
median truth sep$_{IT}$ (Stage 3) [mm]