



UPON PRESSING THE CALIBRATION START BUTTON, TRIGGERS PHASE 1 OF CAL CYCLE AND RESETS VALUES OF 30% AND 0% SAMPLES AND AVERAGES TO 0.

0000

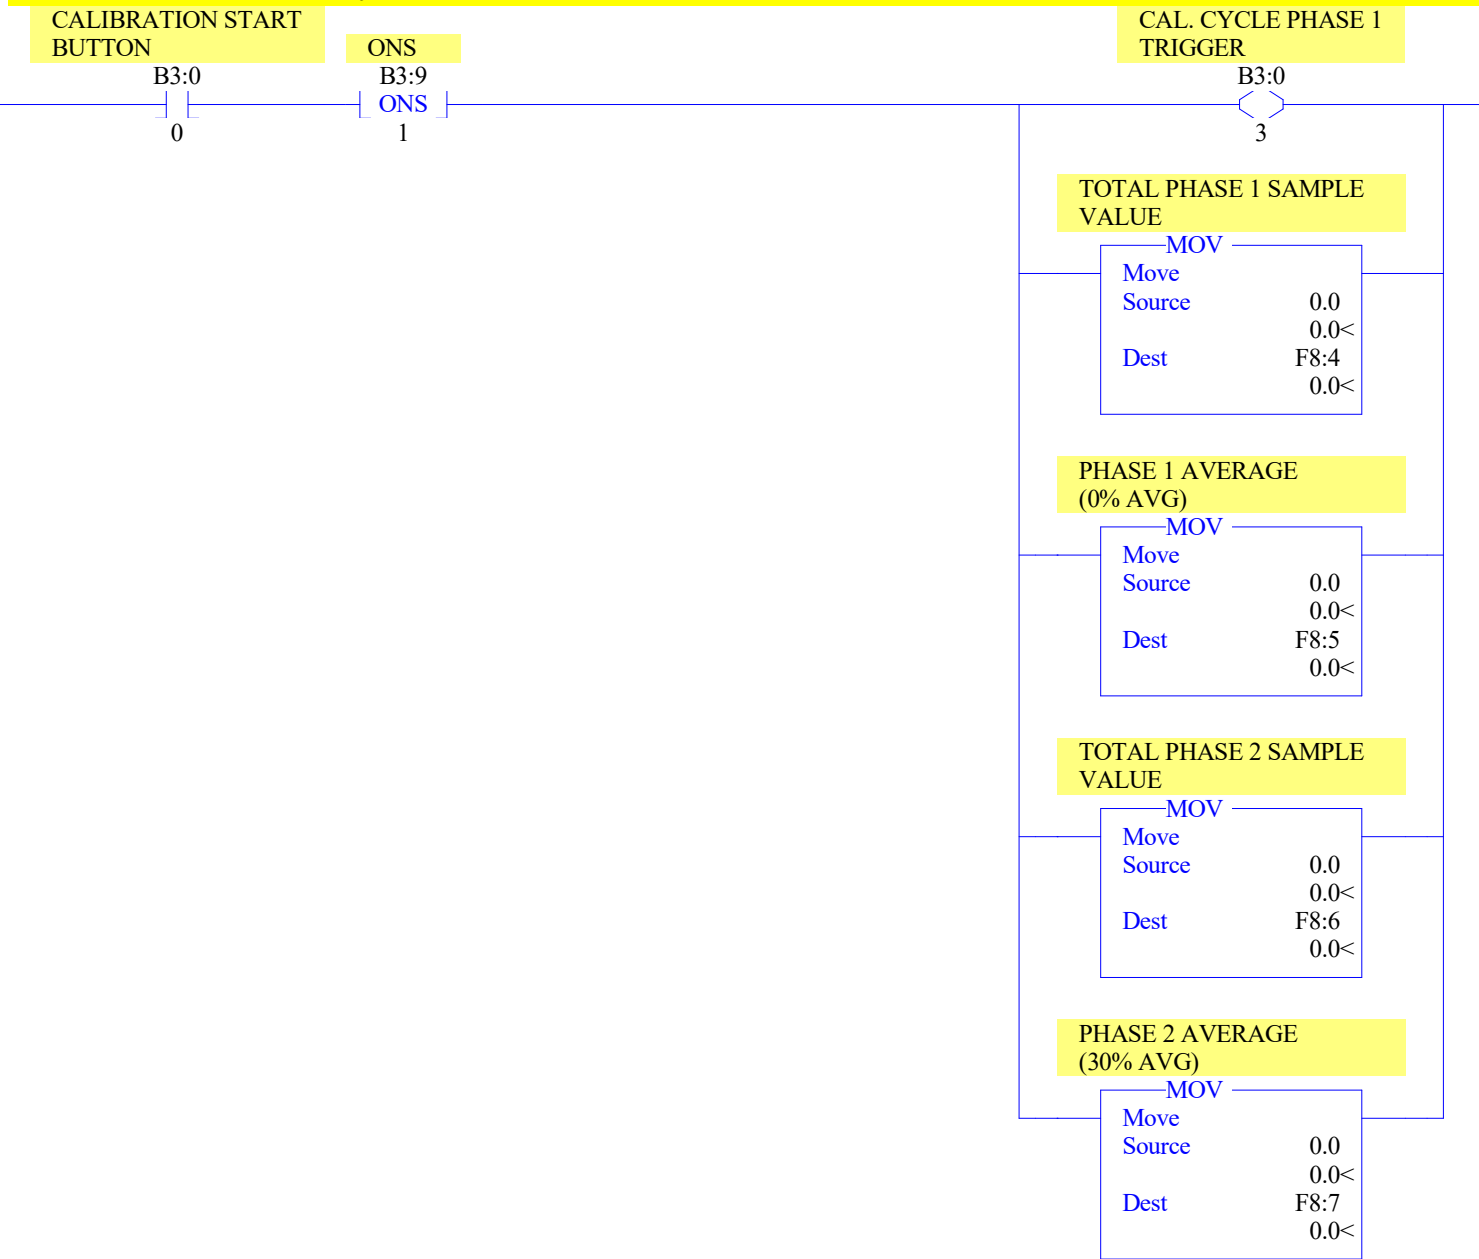

UPON TRIGGER, CAL CYCLE PHASE 1 WILL ENERGIZE AND STAY ENERGIZED UNTIL CAL. PHASE 1 IS COMPLETE.

0001

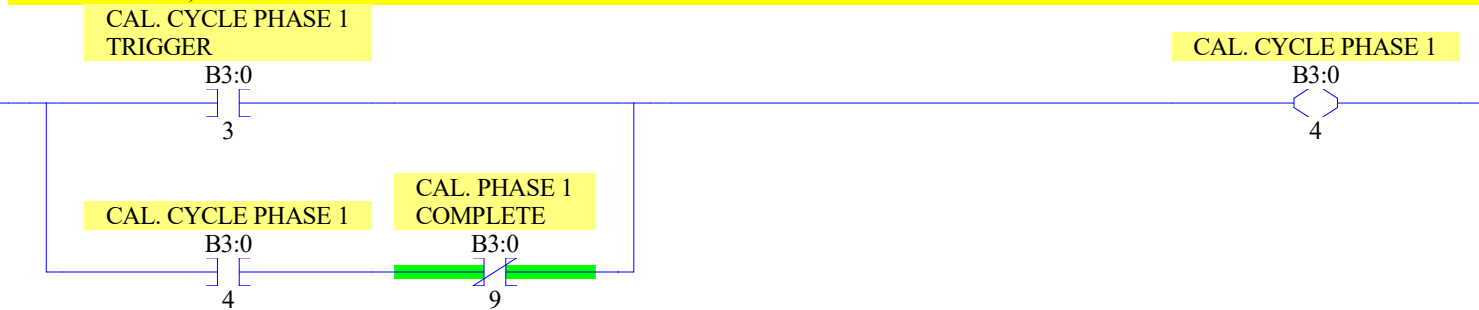

ENTERING CAL PHASE 1 WILL TRIGGER 0% O2 VALVE TO ENERGIZE

0002

