PROFESSIONAL INSTALLATION, OPERATING AND SERVICE MANUAL

MICROBIOLOGICAL FILTER

- ☐ BPUSS4005
  Replacement Filter
  Model # BPUSF4005
- ☐ BPUSS4005BF
  Replacement Filter
  Model # BPUSF4005BF



PLATINUM SERIES

MICROBIOLOGICAL FILTER
Reduces PFAS, Viruses, Cysts, VOCs
Pharmaceuticals, Lead & Bacteria

NSF/ANSI STANDARDS

BPUSF4005 filter and BPUSS4005 system has been tested according to NSF/ANSI 42, 53, 401, P231, P473 and P477 for reduction of the substances specified on the Performance Data Sheet. The concentration of the indicated substances in water leaving the system, as specified in NSF/ANSI 42, 53, 401, P231, P473 and P477 substantiated by test data. This system is certified to NSF/ANSI standard 372 for lead free compliance.

MICROBIOLOGICAL TECHNOLOGY

BRITA|PRO®

TABLE OF CONTENTS

Warning & Important Messages — 1
Product Overview — 2
Operational Parameters — 2
Installation Precautions — 2
Recommended Tools For Installation — 3
Contents of Under Counter System — 3
System / Installation Diagram — 4
Installation Guide — 5
- System Module Mounting — 5
- Filtration System — 5
- Using Quick-Connect Fittings — 6
- Cartridge Installation — 6
- Filtration Connection Using Braided Lines — 7
- System Start up — 7

Trouble Shooting — 8
System Maintenance — 9
- Filter Replacement — 9

Performance Data sheet — 10-14
Optional Parts List — 15-16

⚠ WARNING



Please read carefully before proceeding with installation.

Your failure to follow any attached instructions or operating parameters may lead to the products failure.

Keep this manual for future reference.

⚠ WARNING

Do not use with water that is microbiologically unsafe or of unknown quality without adequate disinfection before or after the system.

⚠ CAUTION

Test the water periodically to verify that the system is performing satisfactorily.

Discard small parts remaining after the installation.

NOTICE

Failure to install the system correctly voids the warranty.

Handle all components of the system with care.

Do not drop, drag or turn components upside down.

IMPORTANT

If you are unsure about installing your Brita PRO™ water filter:

Contact a Brita PRO™ representative or consult a professional plumber.

IMPORTANT

Refer to enclosed warranty for operating parameters to ensure proper use with your water supply.

PRODUCT OVERVIEW

Thank you for your purchase of a Brita PRO™ state of the art Water Treatment system.

Your new system is equipped with a high capacity Microbiological filter. This water filtration unit provides clean, clear, great tasting water to your existing faucet and has a 3,000 base gallon filtration capacity through IAMPO and 6,000 gallon filtration capacity through independent lab testing.

Simple under sink installation, only requiring standard household tools, allows changing of the filter with just a quarter turn.

OPERATIONAL PARAMETERS

NOTICE Installation must comply with state and local plumbing regulations.

Model # BPUSS4005	***Maximum***	***Minimum***
Operating Temperature	100° F (37.8° C)	35° F (1.7° C)
Operating Pressure	100 psi	10 psi
pH Parameters	9	6
Flow Rate	1.6 gpm	

INSTALLATION PRECAUTIONS

NOTICE

- ***You must use pre-treatment (minimum 5 micron) before the microbiological filter to reduce clogging.***
- Ensure water supply is **OFF** before installation or service.
- System is intended to be installed on the cold water line ONLY. Do not use hot water supply.
- DO NOT install if your water lines are susceptible to water hammer.
- System to be used with municipal or well water sources properly treated and tested on a regular basis to ensure suitable and non adverse water conditions, including bacteriological safe quality.
- Filter housing must be protected against freezing temperatures, frost, snow, sleet and ice. Exposure to these elements can damage the housing and lead to water damage.
- This product has a limited service life. We recommend that a record be kept regarding the date of install and any other performance maintenance. Because of the products' limited service life and to prevent costly repairs or possible water damage, ***we strongly recommend that the head be replaced every ten years***.
- Turn off water supply to head and remove the cartridge if it must be left unattended for an extended period of time.
- After prolonged periods of non-use (such as vacation) it is recommended that the system be flushed thoroughly. Let water run 5 - 6 minutes before using
- The filter recommended for use with this system carries a limited service life. Changes in taste, odors, color and/or flow of the water being filtered indicates that the cartridge should be replaced. **Filter life should not extend past one (1) year**.
- Make certain that installation complies with all state and local laws and regulations.
- If you have anything other than flexible hose under your sink, check to see if you need to purchase special fittings prior to starting install.

Recommended Tools for Installation

- Utility knife or tube cutter (if using food-grade poly tubing)
- Variable speed drill
- 1/8 “ (3 mm) drill bit
- Adjustable wrench
- Phillips screwdriver
- Sealant tape (Blue Monster® Teflon tape)

What’s in the Box?

Below are the contents of the Brita PRO™ Microbiological Under Counter System. Please ensure all of the items listed below are contained in the box.

If any of the items are missing, please contact Customer Service prior to installation:
866-985-2900, option 2 for Technical Services

- System Head with Attached Bracket
- Model #BPUSF4005 filter
- Mounting Screws x 3
- 3/8" NPT x 3/8" stem adapter x 2
- 3/8" push-fit x 3/8" male compression x 2


SYSTEM / INSTALLATION DIAGRAM

(A) System Head with attachable bracket

(B) Replacement filter


(C) Mounting bracket (not shown)
Mounting screws (not shown) x 3
3/8" NPT x 3/8" stem adapter (not shown) x 2 (part# BPS0660616)
3/8" push-fit x 3/8" male compression (not shown) x 2 (part# BPO0620916)


(D) Braided supply line 3/8" x 3/8" female compression
(this item is not included in packaging)

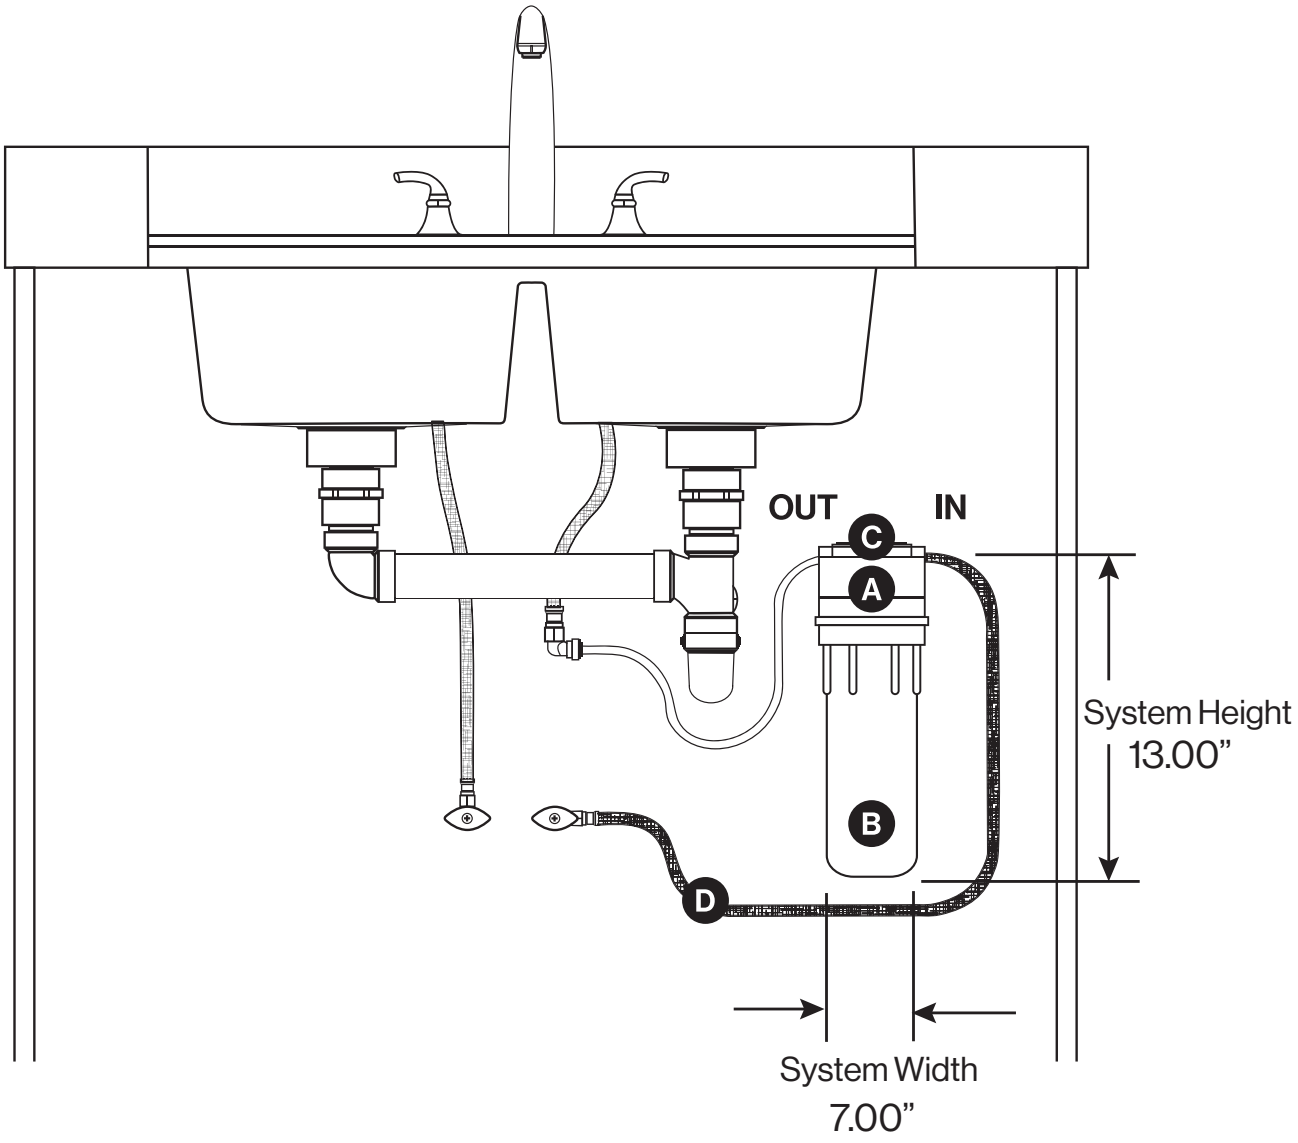

SYSTEM MODULE MOUNTING

1. Remove filter from the head.
2. Mount the system to one side of the cabinet allowing 2.5" of clearance below the filter for easy filter removal and replacement.
3. Using the mounting bracket, mark with a pencil the holes for the mounting screws on the wall surface.
4. Using a 1/8" drill bit, drill pilot holes for the mounting screws. Insert mounting screws into the wall with a screwdriver.

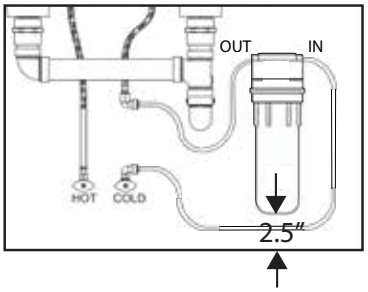


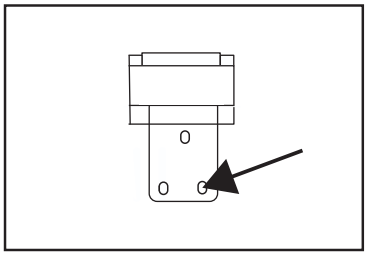


FILTRATION SYSTEM

Connection using food grade poly-tubing

1. Inset a 3/8" NPT thread x 3/8" push fit fitting into the inlet and outlet sides of the head (reference optional part list (BPO0620616B or BPP0620616B). Apply Blue Monster® Teflon sealant tape to the threads of each fitting. Carefully screw the fitting into the inlet and outlet of the filter head (be careful not to cross thread). When applying Teflon tape skip the first two threads which will help reduce the possibility of cross threading the fitting.
2. Determine the lengths of 3/8" tubing needed to connect the system head inlet and outlet (reference directions on next page for cutting and installing tubing). Be sure to allow enough tubing to prevent kinking in the line.
3. Wet one end of the 3/8" plastic tubing with water and push it into the inlet side of the system head approximately 5/8" until it stops. Connect the other end of the tubing to the cold water angle stop valve.
4. Wet one end of the 3/8" plastic tubing with water and push it into the outlet side of the system head approximately 5/8" until it stops. Connect the other end of the tubing to the 3/8" faucet feed line.

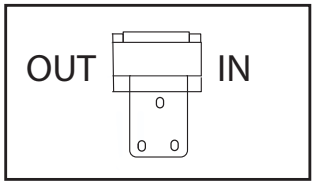

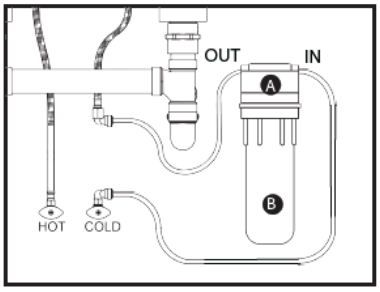


USING QUICK-CONNECT FITTINGS



Cutting


Cut the tube square. It is essential that the outside diameter be free of score marks, and that burrs and sharp edges be removed before inserting into fitting.

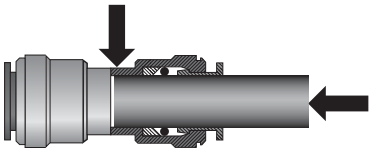

Connecting

Make certain to push the tubing completely into the connector until it comes into contact with the internal tubing stop. The collet (gripper) has stainless steel teeth which hold the tube firmly in position while the O-ring provides a permanent leak proof seal.


Pull on the tube to check that it is secure. The system must be tested prior to leaving the site and/or before use.



Disconnecting


To disconnect, ensure the system is depressurized before removing the tube. Push in collet squarely against the face of the fitting. With the collet held in this position, the tube can be removed. The fitting can then be reused.

CARTRIDGE INSTALLATION

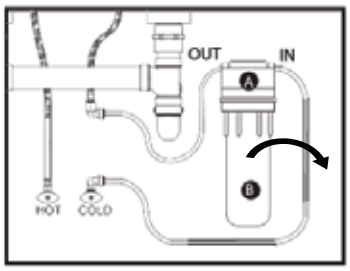

1. Add a thin layer of lubricant to the O-ring on the top of the filter prior to inserting.
2. Insert cartridge and turn 1/4 turn clockwise.

NOTICE **Reference image for inlet and outlet locations.**

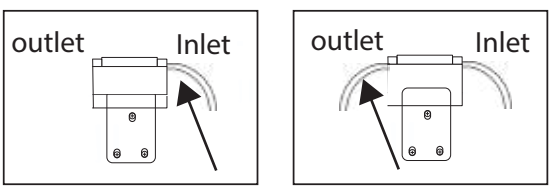

FILTRATION CONNECTION USING BRAIDED LINES

1. Add Blue Monster® Teflon to both 3/8" NPT x 3/8" stem adapters (skipping the first two threads).
2. Attach stem adapters to the inlet and outlet sides of the filter head. Be careful to not cross-thread.
3. Connect the 3/8" push-fit x 3/8" male compression to the 3/8" NPT x 3/8" stem adapter by pushing the push-fit side onto the stem.
4. Turn off water supply.
5. Disconnect water supply line from cold water angle-stop valve.
6. Now connect the supply line to the OUTLET side of the filter and tighten.
7. Connect 3/8" female compression x 3/8" female compression (NOT PROVIDED) to the cold water angle-stop valve, and to the INLET side of the filter and tighten.

SYSTEM START UP

1. Turn on water supply at cold water angle stop. Turn cold water faucet handle to the open position to start the flow of water through the unit. Fully open water faucet handle to the open position and allow water to fully flow for 10 minutes in order to flush out the normal black carbon fines (it will "sputter" until the air is purged out) from the unit. Initially, the water may appear cloudy which is due to tiny air bubbles and it will clear up shortly. Close the faucet when finished.
2. Check for leaks. If you have any leaks, shut off the water supply to your system, tighten any fittings then turn the supply back on.

NOTICE **Check frequently over the next 24 hours to ensure no leaks are present.**

TROUBLESHOOTING

LEAKS BETWEEN THE SYSTEM HEAD AND THE FILTERS

1. Turn off water supply to the filter and dispense water from kitchen faucet until water and airflow stops.
2. Remove cartridge and inspect O-rings to make sure they are in place and clean. Make sure O-rings are not pinched. Add additional lubricant if needed
3. Install cartridge, turn on water supply and check for leaks.

LEAKS AROUND THE FITTINGS

1. Turn off water supply to the filter and dispense water from kitchen faucet until water and airflow stops.
2. While pulling the 3/8" plastic tubing with one hand, press in on the collar around the inlet and/or outlet fitting. Check to make sure that the 3/8" plastic tubing is cut squarely and that it is not scratched or crimped. If the 3/8" plastic tubing is unevenly cut or scratched, cut off 1/2" to 5/8" and re-install tubing.
3. Turn on water supply and check for leaks.

LEAKS FROM THE WATER LINE ADAPTERS

1. Turn off water supply to the filter and dispense water from kitchen faucet until water and airflow stops.
2. Locate the water line adapter
   A. If the 3/8" plastic tubing is leaking, follow the previous steps ("Leaks Around the Fittings").
   B. If the thread between the water line adapter and cold water line is leaking, tighten more securely. If leaking continues, disconnect water line adapter and apply Blue Monster® plumbers tape to threads and tighten.
3. Turn on water supply and check for leaks.

NOTICE If leaks persist, or if there are other leaks on system, turn off water supply. **Contact the Technical Support Team at 828-449-2023**.

SYSTEM MAINTENANCE

It is important to change filters at the recommended interval indicated in this manual. Many contaminants are not detectable by taste. In addition, other bad tastes and odors may become apparent over time if filters are not replaced.

When replacing any of the filter elements, pay special attention to any cleaning instructions.

Should you have any further questions:

WEBSITE: www.britapro.com

CALL: 866-985-2900, option 2 for Technical Services

FILTER REPLACEMENT

Replace the filter every 6 to 12 months

Depending on incoming feed water conditions, replacement time frame may vary

Filter Model Number: **BPUSF4005**

NOTICE **MARK THE DATE THE FILTER IS INSTALLED ON CARTRIDGE LABEL**

1. Turn off incoming water supply to the filtration unit.
2. Open the cold water faucet handle to relieve the water pressure.
3. Remove the filter from the head by turning to the left then pulling downwards. Discard the old filter.
4. Remove new filter cartridge from filter cartridge box
5. Prior to installing a new filter cartridge, apply a thin layer of lubricant to the O-ring of the filter and to the filter head. With the filter label facing approximately 45 degrees to the left, push the filter into the filter head and twist it to the right until the filter locks in and the label on filter is facing the front.
6. Follow start-up procedure.

Single-Stage Filtration System
General Use Conditions

WARNING System to be used with municipal or well water sources treated and tested on regular basis to insure bacteriological safe quality.

DO NOT use with water that is microbiologically unsafe or of unknown quality without adequate disinfection before or after the system. While testing was performed under standard laboratory conditions, actual performance may vary.

- Operating Temperature:
  Maximum: **100° F (38° C)**
  Minimum: **35° F (1.7° C)**
- Operating Water Pressure:
  Maximum: **100-psi**
  Minimum: **10-psi**
- Maximum Flow Rate: **1.6 gpm** (6.056 lpm)
- Rated Capacity PFAS: **3,000 gallons** (IAMPO) and **6,000 gallons** (Independent lab)
- Rated Capacity Pharmaceuticals: **3,000 gallons** (IAMPO) and **6,000 gallons** (Independent lab)

RECOMMENDED REPLACEMENT PARTS AND CHANGE INTERVAL

Depending on incoming feed water conditions replacement time frame may vary.

Description:	FILTER
Model Number:	BPUSF4005
Change Time Frame:	12 months or 3,000 gallons

The BPUSS4005 system has been tested according to NSF/ANSI 42, 53, 401, P231, P473 and P477 for reduction of the substances listed below. The concentration of the indicated substances in water entering the system was reduced to a concentration less than or equal to the permissible limit for water leaving the system, as specified in NSF/ANSI 42, 53, 401, P231, P473 and P477 substantiated by test data. This system is certified to NSF/ANSI standard 372 for 'lead free' compliance.

Not all water will contain contaminants listed. Testing performed under standard laboratory conditions; actual performance may vary. Filter usage must comply with all state and local laws. Filter is only to be used with cold water. Do not use with water that is microbiologically unsafe or of unknown quality without adequate disinfection before or after the system.

Brita PRO™ products are third-party tested and verified to NSF/ANSI standards. The standard(s) tested and certified for each product is identified on all performance data sheets and manuals.

Brita PRO™ NSF Performance Data

Brita PRO products are tested and verified to NSF/ANSI standards. The standard(s) tested and certified for each product is identified on all performance data sheets and manuals. Test data certified by IAPMO R&T.

NSF/ANSI 42 - Aesthetic Effects

Contaminant	Percent Reduction	Influent challenge concentration (mg/L unless specified)	Maximum permissible product water concentration (mg/L unless specified)
CHLORAMINE	>97.5%	3.0 +/- 10%	0.5
CHLORINE	>97.5%	2.0 ± 10%	≥ 50%
Particulate Class I	99.8%	min. 10,000 particles/mL	≥ 85%

NSF/ANSI 53 - Health Effects

Contaminant	Percent Reduction	Influent challenge concentration (mg/L unless specified)	Maximum permissible product water concentration (mg/L unless specified)
ALACHLOR	>98%	0.050	0.001
ARSENIC (pH 6.5)	>97.9%	0.050 ± 10%	0.010
ARSENIC (pH 8.5)	97.6%	0.050 ± 10%	0.010
ASBESTOS	>99%	10^7 to 10 ^{8}fibers/L	99%
ATRAZINE	>97%	0.100	0.003
BENZENE	>99%	0.081	0.001
BROMODICHLOROMETHANE (TTHM)	>99.8%	0.300	0.015
BROMOFORM (TTHM)	>99.8%	0.300	0.015
CARBOFURAN (Furadan)	>99%	0.19	0.001
CARBON TETRACHLORIDE	98%	0.078	0.0018
CHLORDANE	>99.5%	0.040 ± 10%	0.002
CHLOROBENZENE (Monochlorobenzene)	>99%	0.077	0.001
CHLOROPICRIN	99%	0.015	0.0002
CHLOROFORM (TTHM) (surrogate chemical)	>99.8%	0.300	0.015
Cryptosporidium (CYST)	99.95%	minimum 50,000/L	99.95% reduction requirement
CYST	99.99%	min. 50,000/L	99.95%
2, 4-D	98%	0.110	0.0017
DBCP (see Dibromochloropropane)	>99%	0.052	0.00002
1,2-DCA (see 1,2-DICHLOROETHANE)	95%	0.088	0.0048
1,1-DCE (see 1,1-DICHLOROETHYLENE)	>99%	0.083	0.001

Contaminant	Percent Reduction	Influent challenge concentration (mg/L unless specified)	Maximum permissible product water concentration (mg/L unless specified)
DIBROMOCHLOROMETHANE	>99.8%	0.300	0.015
DIBROMOCHLOROPROPANE (DBCP)	>99%	0.052	0.00002
o-DICHLOROBENZENE (1,2 Dichlorobenzene)	>99%	0.080	0.001
p-DICHLOROBENZENE (para-Dichlorobenzene)	>98%	0.040	0.001
1,2-DICHLOROETHANE (1,2-DCA)	95%	0.088	0.0048
1,1-DICHLOROETHYLENE (1,1-DCE)	>99%	0.083	0.001
CIS-1,2-DICHLOROETHYLENE	>99%	0.170	0.0005
TRANS-1,2- DICHLOROETHYLENE	>99%	0.086	0.001
1,2-DICHLOROPROPANE	>99%	0.080	0.001
CIS-1,3- DICHLOROPROPYLENE	>99%	0.079	0.001
DINOSEB	99%	0.170	0.0002
EDB (see ETHYLENE DIBROMIDE)	>99%	0.044	0.00002
ENDRIN	99%	0.053	0.00059
Entamoeba (see CYSTS)	99.95%	minimum 50,000/L	99.95% reduction requirement
ETHYLBENZENE	>99%	0.088	0.001
ETHYLENE DIBROMIDE (EDB)	>99%	0.044	0.00002
Furadan (see CARBOFURAN)	>99%	0.19	0.001
Giardia Lamblia (see CYST)	>99.95%	minimum 50,000/L	99.95% reduction requirement
HALOACETONITRILES (HAN)			
BROMOCHLOROACETONITRILE	98%	0.022	0.0005
DIBROMOACETONITRILE	98%	0.024	0.0006
DICHLOROACETONITRILE	98%	0.0096	0.0002
TRICHLOROACETONITRILE	98%	0.015	0.0003
HALOKETONES (HK):			
1,1-DICHLORO-2-PROPANONE	99%	0.0072	0.0001
1,1,1-TRICHLORO-2-PROPANONE	96%	0.0082	0.0003
HEPTACHLOR	>99%	0.25	0.00001
HEPTACHLOR EPOXIDE	98%	0.0107	0.0002
HEXACHLOROBUTADIENE	>98%	0.044	0.001
HEXACHLOROCYCLOPENTADIENE	>99%	0.060	0.000002
LEAD (pH 6.5)	>99.3%	0.15 ± 10%	0.010
LEAD (pH 8.5)	>99.3%	0.15 ± 10%	0.010
LINDANE	>99%	0.055	0.00001
MERCURY (pH 6.5)	>96.6%	0.006 ± 10%	0.002
MERCURY (pH 8.5)	>96.7%	0.006 ± 10%	0.002
METHOXYCHLOR	>99%	0.050	0.0001
Methylbenzene (see TOLUENE)	>99%	0.078	0.001
Monochlorobenzene (see CHLOROBENZENE)	>99%	0.077	0.001
MTBE (methyl tert-butyl ether)	97%	0.015 ± 20%	0.005
POLYCHLORINATED BIPHENYLS (PCBs , Aroclor 1260)	>99.9%	0.01 +/- 10%	0.0005
PCB	>97%	0.01 ± 10%	0.0005
PCE (see TETRACHLOROETHYLENE)	>99%	0.081	0.001
PENTACHLOROPHENOL	>99%	0.096	0.001
Perchlorobutadiene (see HEXACHLOROBUTADIENE)	>98%	0.044	0.001
Propylene Dichloride (see 1,2 -DICHLOROPROPANE)	>99%	0.080	0.001
RADON	95%	4000 ± 1000 pCi/L	300 pCi/L
SIMAZINE	>97%	0.120	0.004
Silvex (see 2,4,5-TP)	99%	0.270	0.0016

Contaminant	Percent Reduction	Influent challenge concentration (mg/L unless specified)	Maximum permissible product water concentration (mg/L unless specified)
STYRENE (Vinylbenzene)	>99%	0.150	0.0005
1,1,1-TCA (see 1,1,1 - TRICHLOROETHANE)	95%	0.084	0.0046
TCE (see TRICHLOROETHYLENE)	>99%	0.180	0.0010
1,1,2,2- TETRACHLOROETHANE	>99%	0.081	0.001
TETRACHLOROETHYLENE	>99%	0.081	0.001
TOLUENE (Methylbenzene)	>99%	0.078	0.001
TOXAPHENE	>95%	0.015 ± 10%	0.003
Toxoplasma (see CYSTS)	99.95%	minimum 50,000/L	99.95% reduction requirement
2,4,5-TP (Silvex)	99%	0.270	0.0016
TRIBROMOACETIC ACID	>99%	0.042	0.001
1,2,4 TRICHLOROBENZENE (Unsymtrichlorobenzene)	>99%	0.160	0.0005
1,1,1-TRICHLOROETHANE (1,1,1-TCA)	95%	0.084	0.0046
1,1,2-TRICHLOROETHANE	>99%	0.150	0.0005
TRICHLOROETHYLENE (TCE)	>99%	0.180	0.0010
TRIHALOMETHANES (TTHM) (Ch lorofo rm; Bromofo rm; Bromodichloromethane; Dibromochloromethane)	>99.8%	0.300	0.015
TURBIDITY	99.0%	11 ± 1 NTU	0.5 NTU
Unsym-Trichlorobenzene	>99%	0.160	0.0005
Vinylbenzene (see STYRENE)	>99%	0.150	0.0005
XYLENES (TOTAL)	>99%	0.070	0.001

Standard 401- Emerging Contaminants

Contaminant	Percent Reduction	Influent challenge concentration (mg/L unless specified)	Maximum permissible product water concentration (mg/L unless specified)
Group I			
Atenolol	>96.4%	200 ± 20%	0.00003
Carbamazepine	>98.5%	1400 ± 20%	0.0002
DEET	>98.6%	1401 ± 20%	0.0002
Linuron	>96.5%	140 ± 20%	0.00002
Meprobamate	>95.3%	400 ± 20%	0.00006
Metolachlor	>98.7%	1400 ± 20%	0.0002
Trimethoprim	>96.8%	140 ± 20%	0.00002
Group II			
TCEP (Group 2)	>98.0%	5000 ± 20%	0.0007
TCPP (Group 2)	>97.9%	5000 ± 20%	0.0007
Group III			
Bisphenol A (Group 3)	>99.0%	2000 ± 20%	0.0003
Estrone (Group 3)	>96.6%	140 ± 20%	0.00002
Ibuprofen (Group3)	>95.1%	400 ± 20%	0.00006
Naproxen (Group 3)	>96.4%	140 ± 20%	0.00002
Nonyl phenol (Group 3)	>95.6%	1400 ± 20%	0.0002
Phenytoin (Group 3)	>95.4%	200 ± 20%	0.00003

NSF/ANSI Protocol P231 - Viruses & Bacteria

Contaminant	Percent Reduction	Influent challenge concentration (mg/L unless specified)	Maximum permissible product water concentration (mg/L unless specified)
Bacteria, R. Terringena (ATCC-33257)	≥ 99.9999%	2.8 x 107/100 mL	
Virus, MS2 (ATCC-15597-B1)	≥ 99.99%	4.3 x 10^4/mL	

NSF Protocol P473 - PFOA/PFOS

Contaminant	Percent Reduction	Influent challenge concentration (mg/L unless specified)	Maximum permissible product water concentration (mg/L unless specified)
PFOA/PFOS	>99.5%	0.0015 ± 10%***	0.00007

NSF Protocol P477 - Microcystin

Contaminant	Percent Reduction	Influent challenge concentration (mg/L unless specified)	Maximum permissible product water concentration (mg/L unless specified)
Microcystin	99.5%	0.004 ± 10%	0.0003

OPTIONAL PARTS LIST

Single Stage Fittings

Product Number	Description	Visual	Bag QTY
BPU0620906B	Plastic Female connection 3/8 compression to 3/8 tubing 3/8 x 9/16 - 24 UNEF = 3/8 Compression Threads		10
BPSEI0112U9-US	Male Connector - 3/8" Tube x 9/16"- 24 UNEF		10
BPSEI6012U9-US	3/8 connection to supply valve or cold water faucet line Female Connector - 3/8 x 9/16 - 24 UNEF		10
BPP0620616B	'IN' and 'OUT' 90° fitting for 1 stage Polypropylene Fixed Elbow 3/8 x 3/8 NPTF		10
BPO0620616B	'IN' and 'OUT' straight fitting Polypropylene Male Connector 3/8 x 3/8 NPTF		10

Single Stage Fittings

BPT0620666B	90° for 'IN' and 'OUT' straight fitting 3.8 x 3.8 Plug in Elbow		10
BPU0420706B	RO faucet connection Polypropylene Faucet Connector 1/4 x 7/16-24 UNS		10
BPL0605005 BPL0605006	3/8 in. x 500 ft. Polyethylene Tubing Coil *(also available in black - UV resistant)*		1
BPASVPP1LF	Polypropylene Angle Stop Adapter Valve, 3/8 x 3/8 x 1/4 - Low Lead		1
BPASVPP2LF	Polypropylene Angle Stop Adapter Valve, 3/8 x 3/8 x 3/8 - Low Lead		1

All Components Certified by IAPMO R&T to NSF/ANSI 58 for material and structural integrity requirements only, and to NSF/ANSI 372 for lead free compliance.



Brita PRO by Protect Plus Pro LLC

420 3rd Avenue NW • Hickory, NC 28601 • (866) 985-2900
www.britapro.com

The BRITA | PRO™ trademark and logo are registered trademarks of Brita LP and are used under license by Protect Plus, LLC. All rights reserved.