

- Quart DVT QA Test -

HU Linearity ROIs: Air: -1000.0, Poly: -47.0, Acrylic: 106.0, Teflon: 963.0

HU Passed?: True

Measured Slice Thickness (mm): 2.795

Slice Thickness Passed? False


Uniformity ROIs: Top: 89.0, Right: 92.0, Bottom: 98.0, Left: 96.0, Center: 98.0

Uniformity Passed?: True


Geometric width: {'horizontal mm': 159.67995923047522, 'vertical mm': 159.78829435127977}

High-Contrast distance (mm): 0.600


HU Linearity

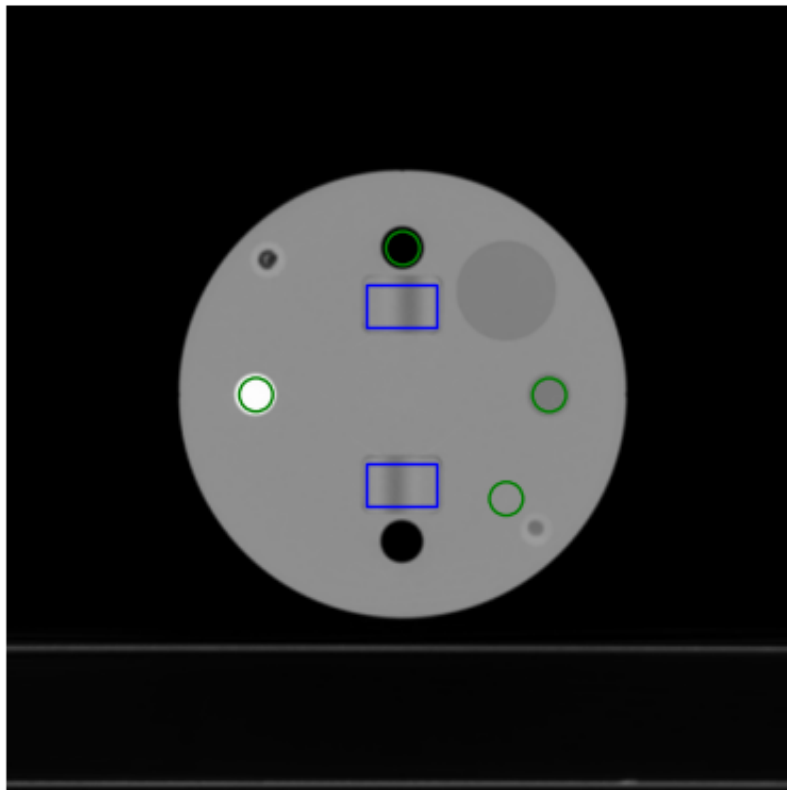

HU Uniformity

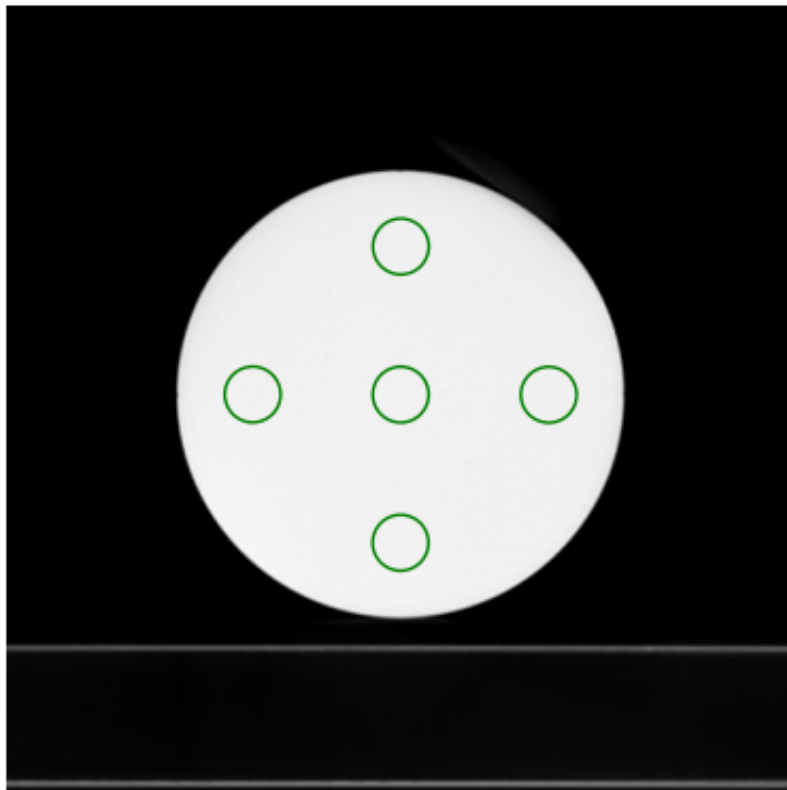

Geometric Distortion

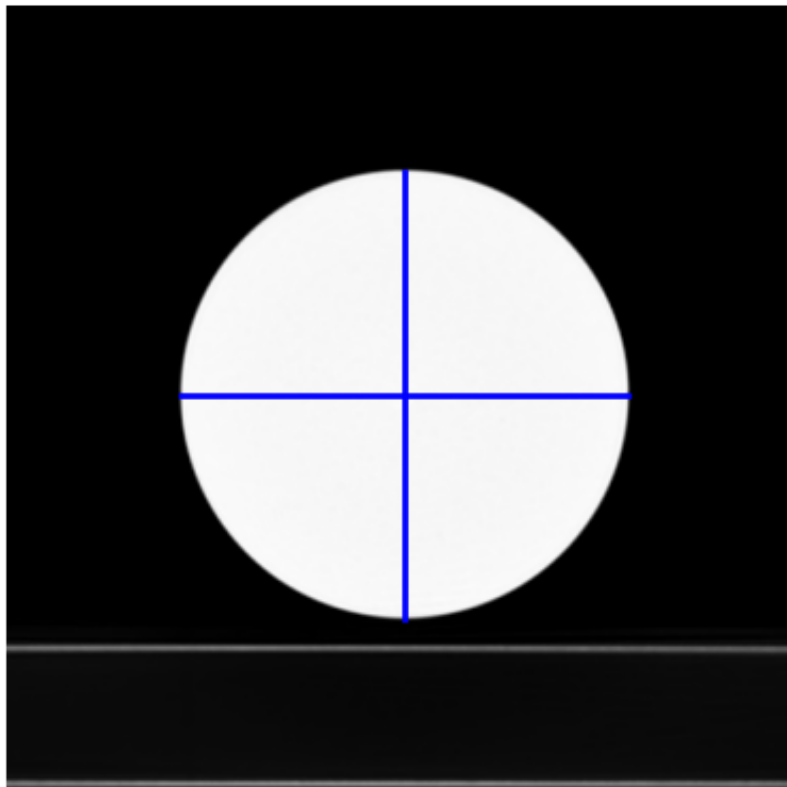

Side View

