

Sample Average Report

Schedule Name : 2015.10.1
Accessory : ABC-210

Comment

[HF-210]

Heater Temp.

Inlet : 799 °C

Outlet : 899 °C

Gas Flow

Ar : 300 ml/min

O2 : 300 ml/min

[Blank]

-PMT sensitivity : Low (For High Concentration)

System Blank : 2.1 Blank are deducted from Sample.

Solvent Blank 1 : ---

Solvent Blank 2 : ---

Solvent Blank 3 : ---

[Calibration]

Formula	Slope(A)	Slope(B)	Intercept(C)	Correlation
---------	----------	----------	--------------	-------------

[ND/TN] - Low (For High Concentration)

Calibration ID : <None>

Y=BX+C	---	169.4875	-0.8	0.999832
--------	-----	----------	------	----------

[Sample Average Data]

Sample ID	Area	Concentration	n	RSD	RSD(%)
-----------	------	---------------	---	-----	--------

[ND/TN]


200ng	33.0	93.349 ppm	1	***	***
T015X01L607(E015G001	27.6	30.877 ppm	4	8.995	29.13
T015X01L610(E014X024	145.2	145.252 ppm	4	96.787	66.63
T015X01L607(E015D017	9.2	8.754 ppm	4	2.403	27.45
T015X01L610(E014Z005	13.9	13.708 ppm	4	1.472	10.74

Sample Report


[Sample Chart]

Schedule Name : 2015.10.1


No.12 Date : 2015/10/1 下午 01:42
Sample ID : 200ng
Area : 33.0 Low

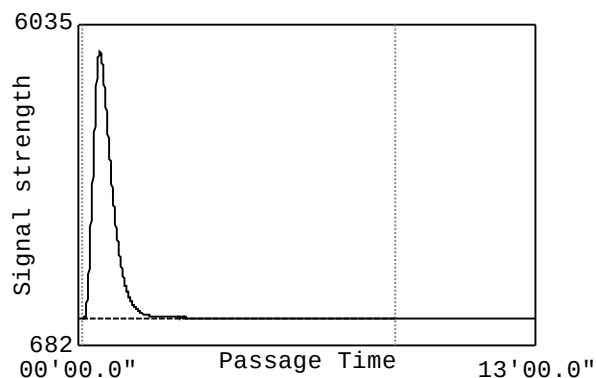


No.13 Date : 2015/10/1 下午 04:36
Sample ID : T015X01L607(E015G001)
Area : 29.3 Low

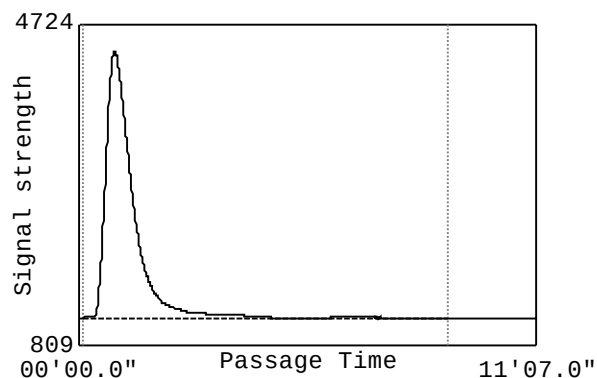


No.14 Date : 2015/10/1 下午 04:47
Sample ID : T015X01L607(E015G001)
Area : 31.0 Low

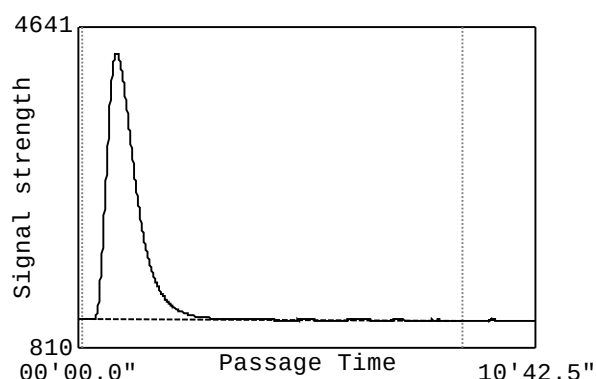


No.15 Date : 2015/10/1 下午 04:58
Sample ID : T015X01L607(E015G001)
Area : 19.3 Low

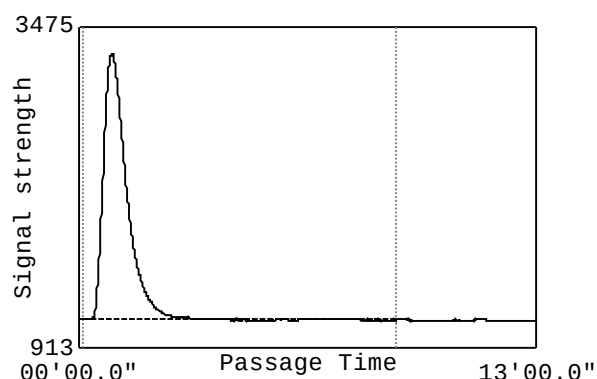

No.16 Date : 2015/10/1 下午 05:16
Sample ID : T015X01L607(E015G001)
Area : 30.6 Low

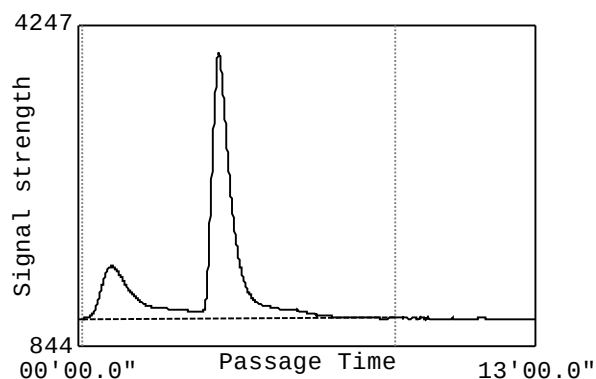

No.17 Date : 2015/10/1 下午 08:45
Sample ID : T015X01L610(E014X024)
Area : 16.9 Low

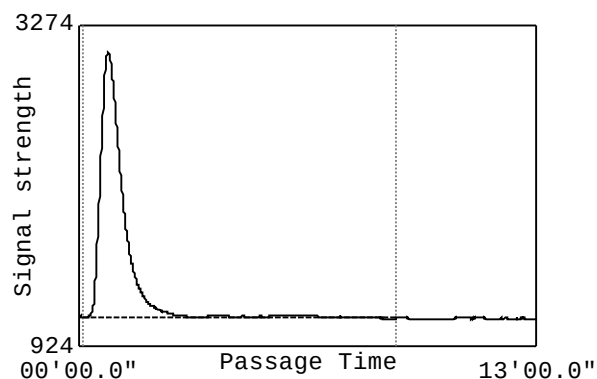


Sample Report


[Sample Chart]

Schedule Name : 2015.10.1


No.18 Date : 2015/10/1 下午 09:30
Sample ID : T015X01L610(E014X024)
Area : 95.8 Low

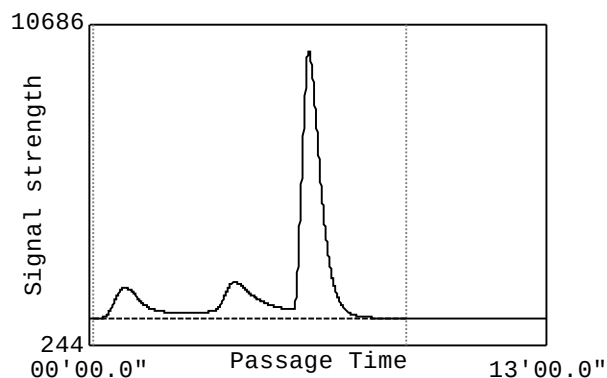


No.19 Date : 2015/10/1 下午 09:52
Sample ID : T015X01L610(E014X024)
Area : 248.4 Low

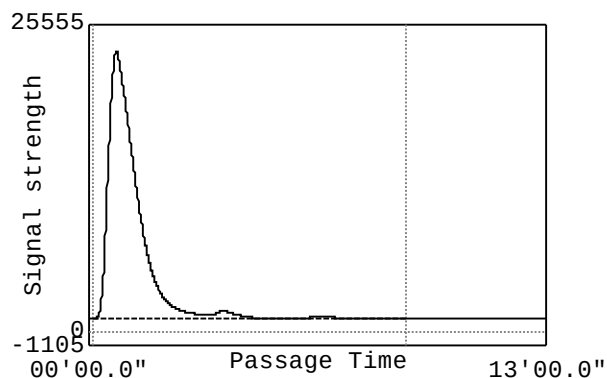


No.20 Date : 2015/10/1 下午 10:08
Sample ID : T015X01L610(E014X024)
Area : 219.9 Low

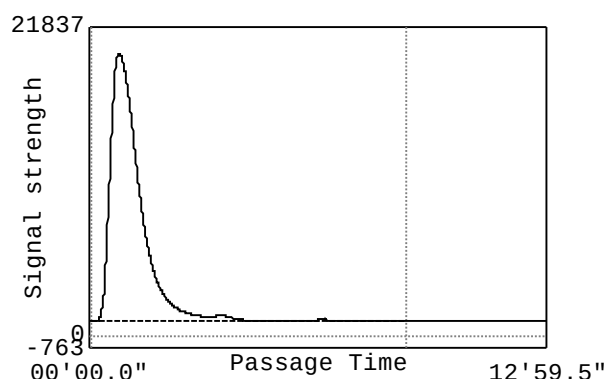


No.21 Date : 2015/10/1 下午 10:30
Sample ID : T015X01L607(E015D017)
Area : 9.1 Low

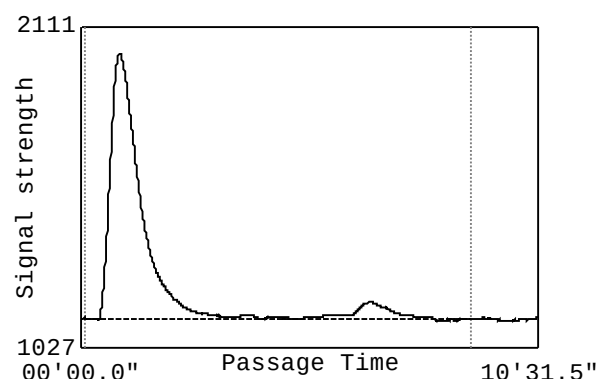

No.22 Date : 2015/10/1 下午 10:41
Sample ID : T015X01L607(E015D017)
Area : 6.0 Low

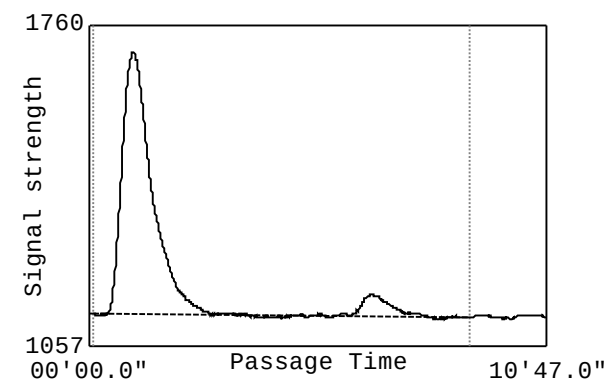

No.23 Date : 2015/10/1 下午 10:51
Sample ID : T015X01L607(E015D017)
Area : 13.5 Low

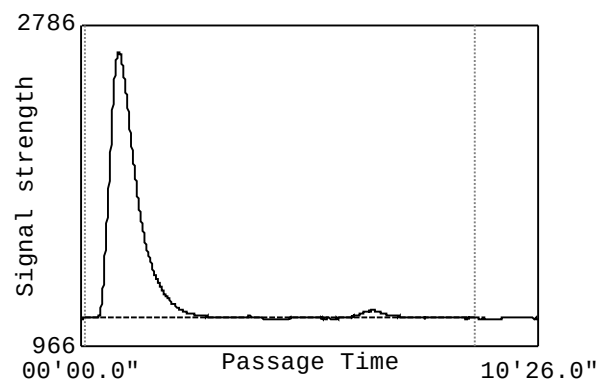


Sample Report


[Sample Chart]

Schedule Name : 2015.10.1


No.24 Date : 2015/10/1 下午 11:02
Sample ID : T015X01L607(E015D017)
Area : 8.3 Low

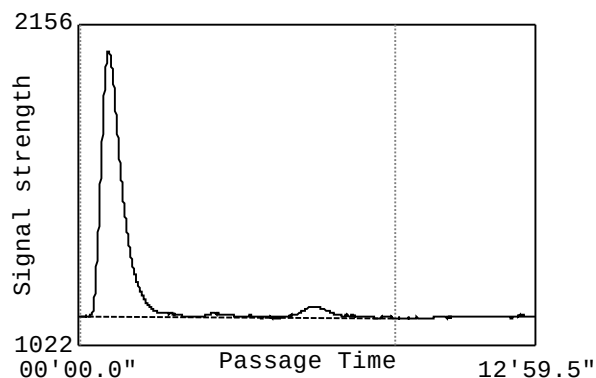


No.25 Date : 2015/10/2 上午 02:04
Sample ID : T015X01L610(E014Z005)
Area : 12.2 Low

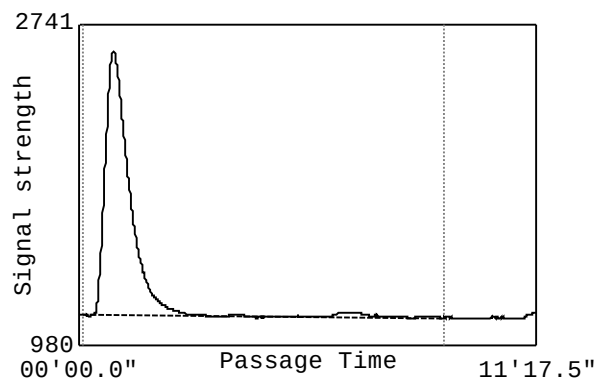

No.26 Date : 2015/10/2 上午 02:16
Sample ID : T015X01L610(E014Z005)
Area : 11.0 Low

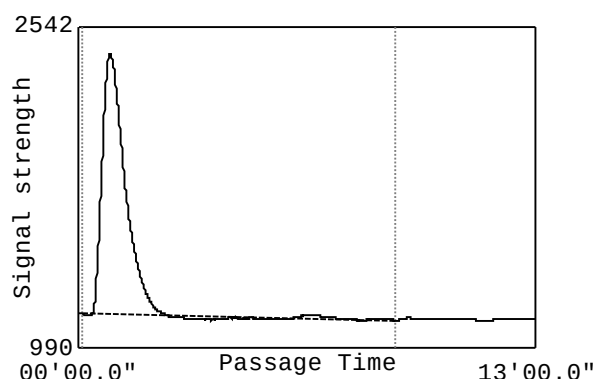

No.27 Date : 2015/10/2 上午 02:44
Sample ID : T015X01L610(E014Z005)
Area : 14.3 Low

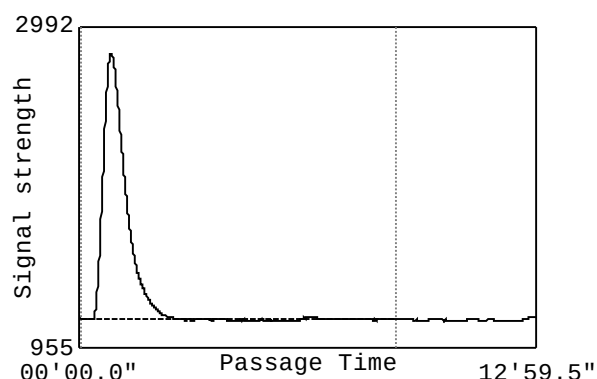

No.28 Date : 2015/10/2 上午 03:04
Sample ID : T015X01L610(E014Z005)
Area : 18.2 Low

