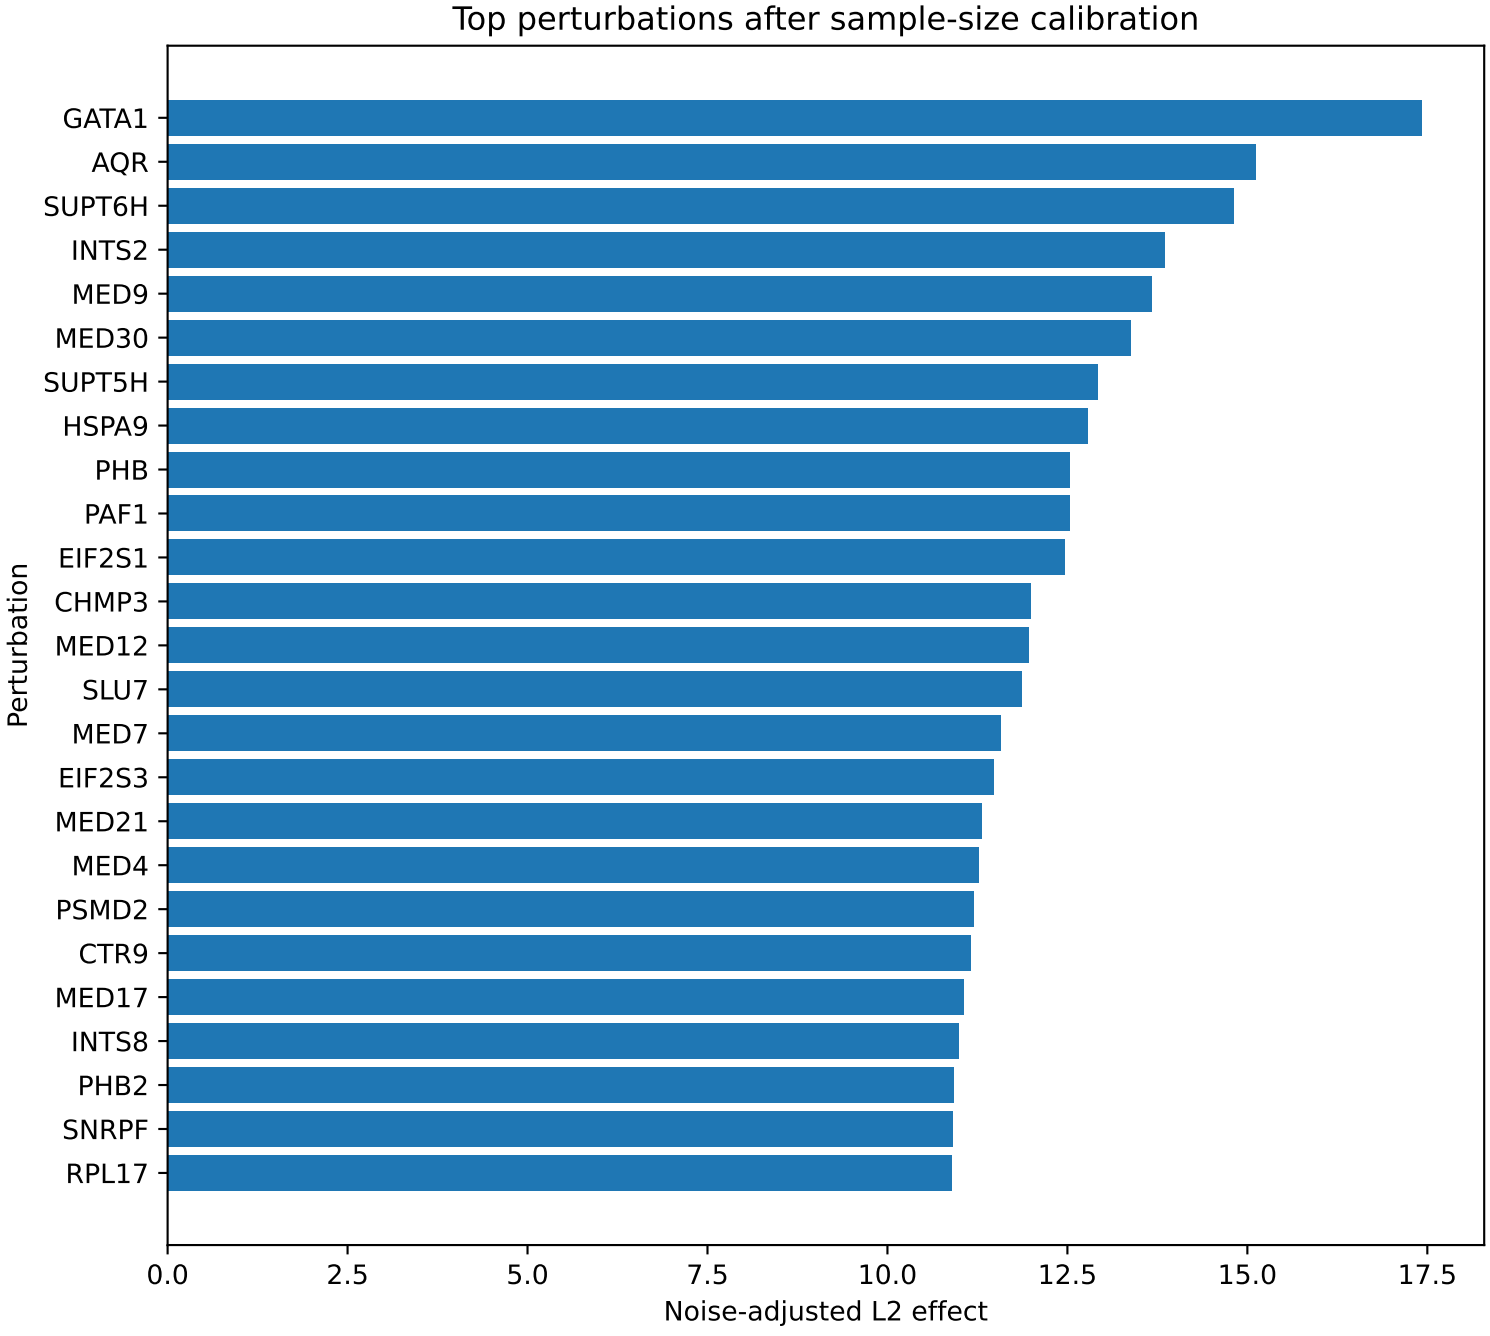
Top perturbations after sample-size calibration
GATA1
AQR
SUPT6H
INTS2
MED9
MED30
SUPT5H
HSPA9
PHB
PAF1
EIF2S1
CHMP3
MED12
SLU7
MED7
EIF2S3
MED21
MED4
PSMD2
CTR9
MED17
INTS8
PHB2
SNRPF
RPL17
Perturbation
0.0
2.5
5.0
7.5
10.0
12.5
15.0
17.5
Noise-adjusted L2 effect