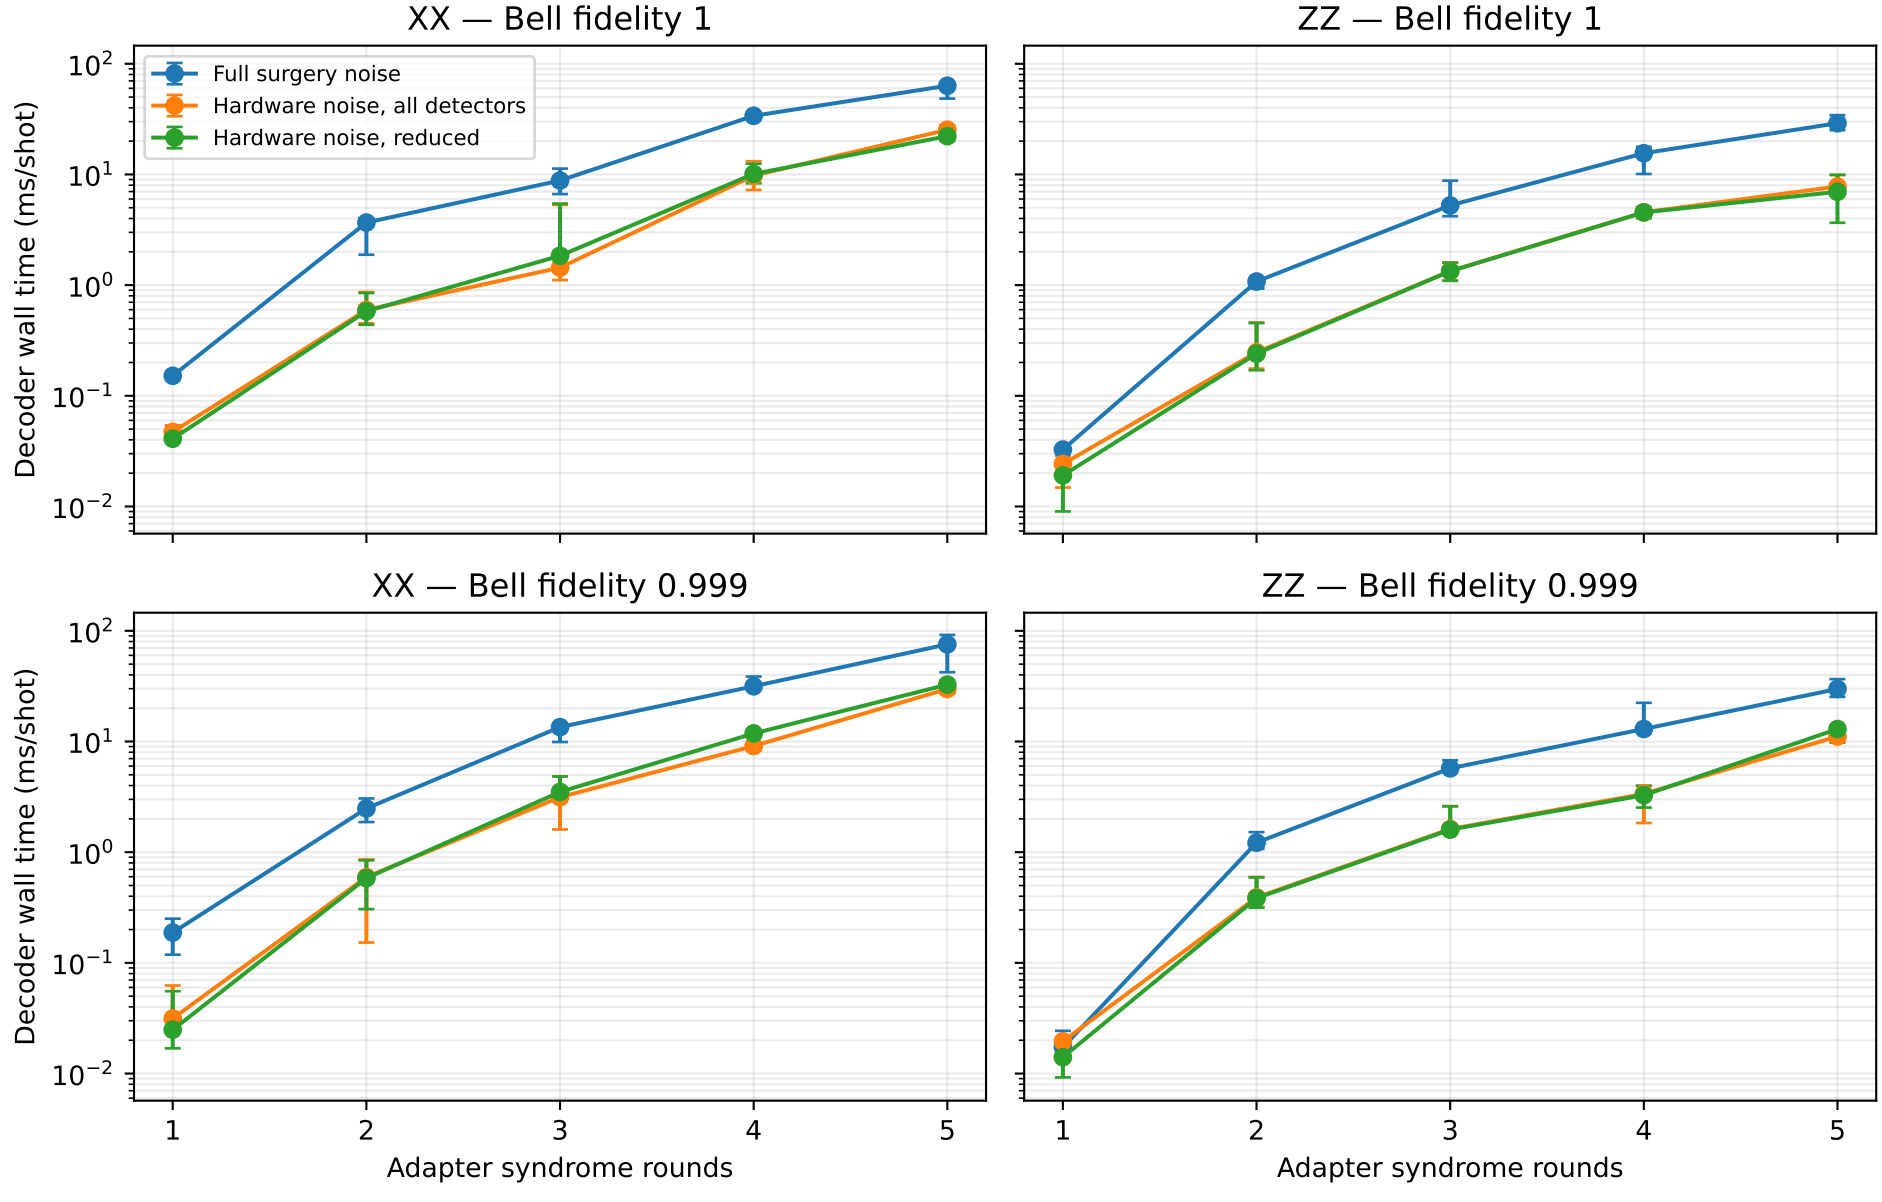
Fresh serial BP+OSD benchmark — median and min–max range
3 batches × 256 shots; hardware models use paired samples
XX — Bell fidelity 1
ZZ — Bell fidelity 1
XX — Bell fidelity 0.999
ZZ — Bell fidelity 0.999
Full surgery noise
Hardware noise, all detectors
Hardware noise, reduced
Decoder wall time (ms/shot)
Adapter syndrome rounds