


Accuracy for the training set, Sigmoid activation



Accuracy for the test set, Sigmoid activation

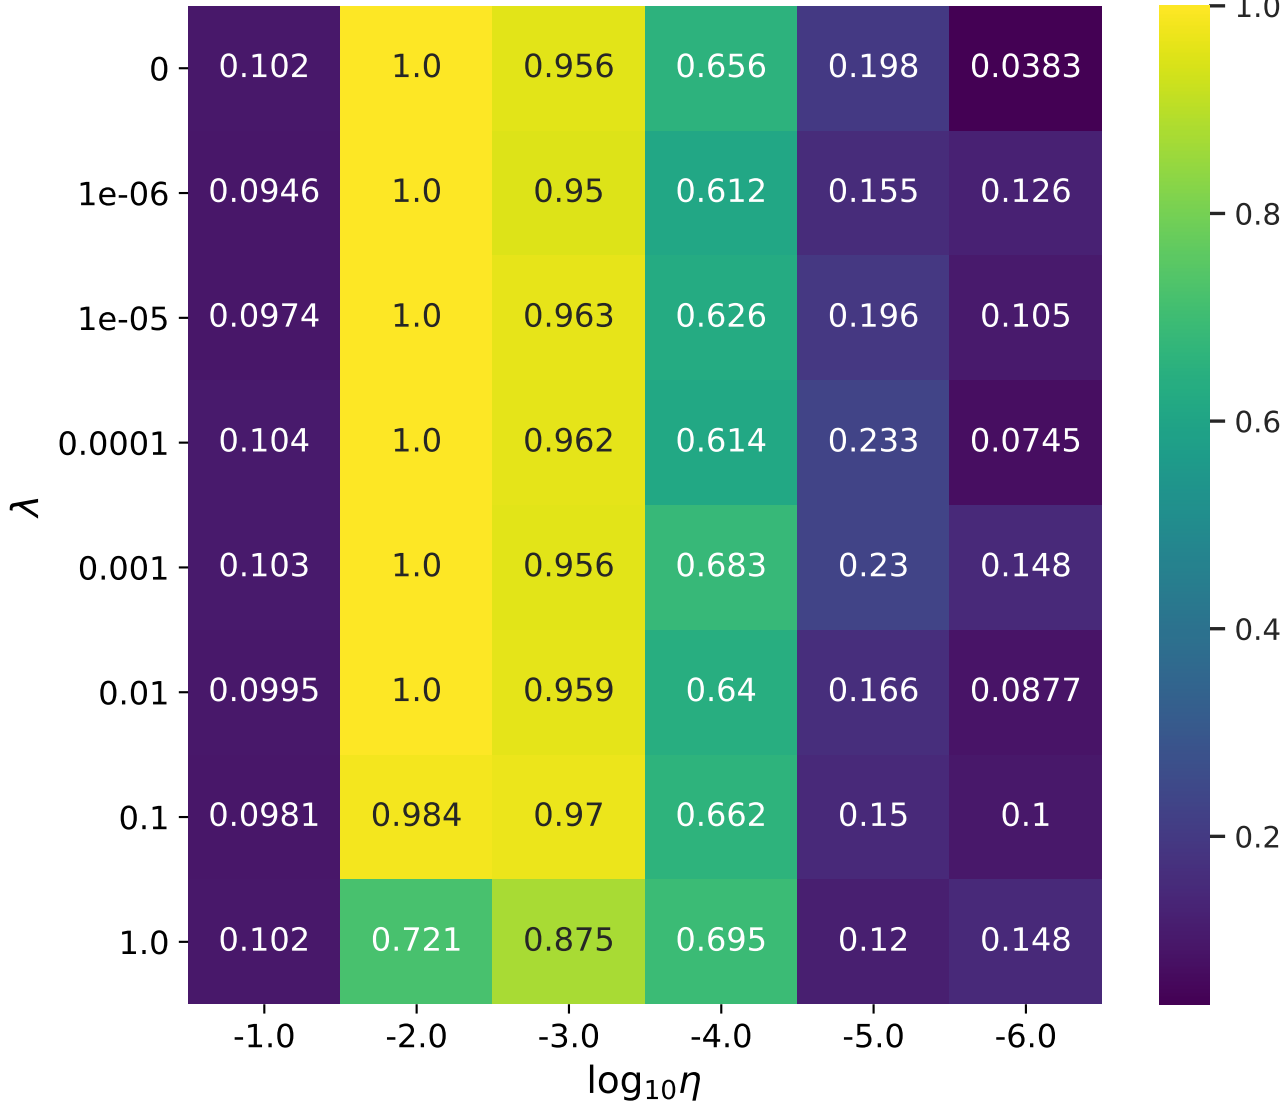