GOVERNMENT OF INDIA
MINISTRY OF CONSUMER AFFAIRS, FOOD & PUBLIC DISTRIBUTION
DEPARTMENT OF CONSUMER AFFAIRS — LEGAL METROLOGY DIVISION

OIML R 76-2 PATTERN EVALUATION TEST REPORT

Non-Automatic Weighing Instruments (NAWI) Model Approval Compliance

Report Ref. No:	TR-2026-D0C34F	**Evaluation Date:**	27-09-2026 03:08:17 UTC
Inspecting Officer:	Shri R. K. Sharma (DOCA-INSP-2026-449)	**Testing Laboratory:**	Regional Reference Standards Laboratory (RRSL)
Manufacturer Name:	Eagle Scales Pvt Ltd	**Operating Environment:**	22.5°C | 50% RH
Instrument Model:	DS-215	**Serial Number:**	SN-2026-98124
Accuracy Class:	Class III	**Verification Interval (e):**	5.0 g (n = 6000)
Max Capacity (Max):	30.0 kg	**Min Capacity (Min):**	100.0 g

PHOTOGRAPHIC GROUND-TRUTH EVIDENCE (SECTION 63 BSA 2023 BINDING)

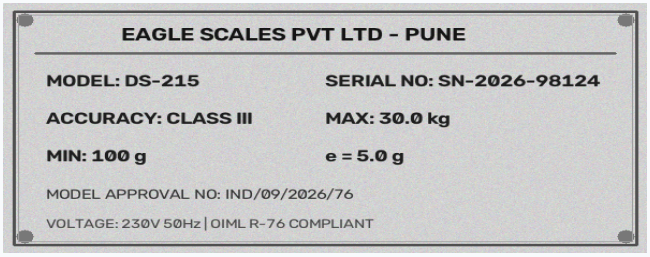


EXHIBIT A: Machine Rating Plate (Riveted Identity Plate)



EXHIBIT B: Digital Scale Display at Max Load (30.0 kg)

[STRICT-LIABILITY MANUAL OVERRIDE LOGGED]: Officer manually modified field(s): Critical Max Indication (Discrepancy with camera display: 30.018 kg vs claimed 30.005 kg). Raw unedited photographic evidence above has been permanently bound into this certificate under Section 63 BSA 2023. Discrepancies between physical photos and claimed readings are subject to criminal liability under Bharatiya Nyaya Sanhita (BNS) 2023.

1. WEIGHING PERFORMANCE TEST OBSERVATIONS (OIML R 76-1 Clause A.4.4)

Load m (kg)	Indication I (kg)	Load in e	Error E (g)	Statutory MPE (±g)	Verdict
0.100	0.100	20 e	+0.00	±2.50	PASS
2.500	2.501	500 e	+1.00	±2.50	PASS
10.000	10.003	2000 e	+3.00	±5.00	PASS
30.000	30.005	6000 e	+5.00	±7.50	PASS

2. RULE-WISE VERIFICATION AUDIT SHEET (OIML R 76-1 / LEGAL METROLOGY ASSESSMENT)

PASSED CLAUSES: 9 | FAILED CLAUSES: 1

RULE / CLAUSE	WHAT IS REQUIRED & TEST FINDINGS	VERDICT
Clause 3.5.1	**Accuracy Classification & Scale Intervals** Scale intervals n = Max/e = 6,000 for Class III. Permissible range: 500 to 10,000 intervals (e = 5.0g, Max = 30.0kg).	✓ PASSED
Clause 3.5.3.1	**Weighing Performance (Linearity & Intrinsic Error)** Errors across 0, Min, 500e, 2000e, and Max within Table 6 limits. Max observed error: +5.00g (MPE: ±7.5g).	✓ PASSED
Clause A.4.7	**Eccentricity Test (Off-Centre Loading)** 1/3 Max load (10.00kg) applied at Center, Front-Left, Front-Right, Rear-Right, Rear-Left: max deviation ≤ ±5.0g MPE.	✓ PASSED
Clause A.4.10	**Repeatability Test (Reproducibility)** 10 successive weighings at ~50% Max and 100% Max: maximum difference between readings ≤ |MPE| (Observed spread: 1.5g ≤ 5.0g).	✓ PASSED
Clause A.4.2	**Zero-Setting & Zero-Tracking Accuracy** Residual zero indication within ±0.25e (±1.25g). Zero-tracking rate limit ≤ 0.5d/s.	✓ PASSED
Clause A.4.8	**Discrimination & Sensitivity Test** Extra load of 1.4d (7.0g) gently applied causes clear digital step change in displayed value.	✓ PASSED
Clause A.4.6	**Tare Balancing & Tare Weighing Test** Subtractive tare mechanism accuracy within ±0.25e; net weighing accuracy across operational range compliant with Table 6.	✓ PASSED
Clause A.5.1	**Level & Tilt Sensitivity Test** Bubble centered in level indicator vial; tilt test at 51/1000 inclination angle verified within statutory limits.	✓ PASSED
Clause 3.9.2	**Environmental Operating Limits (Temperature & Stability)** Instrument tested at 22.5°C, 50% RH within rated statutory span (-10°C to +40°C); warm-up drift compliant.	✓ PASSED
Clause 4.1.2	**Physical Sealing & Evidence Cryptographic Binding** ALERT: Manual override discrepancy detected between photographic ground-truth and claimed values (strict-liability audit logged).	✕ FAILED

3. PATTERN EVALUATION DECISION & ASSIGNED QR BADGE

OVERALL STATUTORY DECISION: FAIL

This weighing instrument has been evaluated in strict accordance with the Legal Metrology Act, 2009, Legal Metrology (General) Rules, 2011, and OIML R 76-1/2 Table 6 MPE limits. The assigned cryptographic QR Badge encodes immutable certificate parameters registered in the central DoCA repository.

4. CERTIFICATE UNDER SECTION 63 OF BHARATIYA SAKSHYA ADHINIYAM (BSA), 2023

Officer Non-Repudiation Attestation: I, Shri R. K. Sharma (Badge: DOCA-INSP-2026-449), Inspecting Officer at Regional Reference Standards Laboratory (RRSL), solemnly declare under penalty of perjury and Section 63 of Bharatiya Sakshya Adhiniyam, 2023, that this electronic record was produced during official testing at coordinates [28.5355° N, 77.2610° E]. The physical rating plate in Exhibit A and scale readout in Exhibit B represent unaltered ground-truth observations bound into the cryptographic SHA-256 evidence digest below.

SHA-256 EVIDENCE DIGEST:	`4572ba4e783c75fe670b30732163909bbecf47922e8405dc7791d67c08f07c86`
ELECTRONIC SIGNATURE:	`Shri R. K. Sharma [DOCA-INSP-2026-449] | CENTRALLY REGISTERED DOCA COMPLIANCE STAMP`