GOVERNMENT OF INDIA
MINISTRY OF CONSUMER AFFAIRS, FOOD & PUBLIC DISTRIBUTION
DEPARTMENT OF CONSUMER AFFAIRS — LEGAL METROLOGY DIVISION

OIML R 76-2 PATTERN EVALUATION TEST REPORT

Non-Automatic Weighing Instruments (NAWI) Model Approval Compliance

Report Ref. No:	TR-2026-TEST01	**Evaluation Date:**	26-09-2026 08:04:42 UTC
Inspecting Officer:	Insp. Rajesh Sharma (RRSL-DOCA-2026-449)	**Testing Laboratory:**	Regional Reference Standards Lab (RRSL)
Manufacturer Name:	Eagle Scales Pvt Ltd	**Operating Environment:**	22.5 C | 50% RH
Instrument Model:	DS-215	**Serial Number:**	SN-2026-98124
Accuracy Class:	Class III	**Verification Interval (e):**	5.0 g (n = 6000)
Max Capacity (Max):	30.0 kg	**Min Capacity (Min):**	100.0 g

PHOTOGRAPHIC GROUND-TRUTH EVIDENCE (SECTION 63 BSA 2023 BINDING)

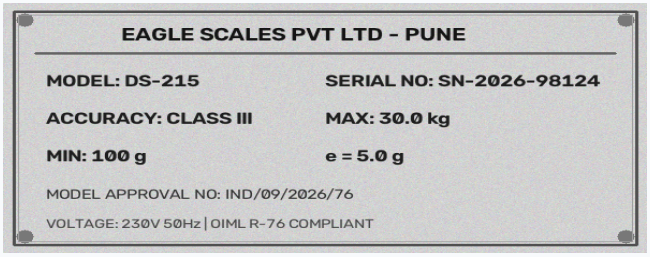


EXHIBIT A: Machine Rating Plate (Riveted Identity Plate)



EXHIBIT B: Digital Scale Display at Max Load (30.0 kg)

[AUTOMATED OCR VERIFIED]: Extracted instrument specifications and digital display values match optical recognition. Raw photographic pixels cryptographically sealed without manual override.

1. WEIGHING PERFORMANCE TEST OBSERVATIONS (OIML R 76-1 Clause A.4.4)

Load m (kg)	Indication I (kg)	Load in e	Error E (g)	Statutory MPE (±g)	Verdict
0.100	0.100	20 e	+0.00	±2.50	**PASS**
2.500	2.502	500 e	+2.00	±2.50	**PASS**
10.000	10.004	2000 e	+4.00	±5.00	**PASS**
20.000	20.005	4000 e	+5.00	±7.50	**PASS**
30.000	30.005	6000 e	+5.00	±7.50	**PASS**

3. PATTERN EVALUATION DECISION & ASSIGNED QR BADGE

OVERALL STATUTORY DECISION: PASS

This weighing instrument has been evaluated in strict accordance with the Legal Metrology Act, 2009, Legal Metrology (General) Rules, 2011, and OIML R 76-1/2 Table 6 MPE limits. The assigned cryptographic QR Badge encodes immutable certificate parameters registered in the central DoCA repository.

4. CERTIFICATE UNDER SECTION 63 OF BHARATIYA SAKSHYA ADHINIYAM (BSA), 2023

Officer Non-Repudiation Attestation: I, Insp. Rajesh Sharma (Badge: RRSL-DOCA-2026-449), Inspecting Officer at Regional Reference Standards Laboratory, solemnly declare under penalty of perjury and Section 63 of Bharatiya Sakshya Adhiniyam, 2023, that this electronic record was produced during official testing at coordinates [18.5204° N, 73.8567° E (RRSL Pune)]. The physical rating plate in Exhibit A and scale readout in Exhibit B represent unaltered ground-truth observations bound into the cryptographic SHA-256 evidence digest below.

SHA-256 EVIDENCE DIGEST:	`9f8132662f37bb59a7abc3e53c723c2b57bf1fae88eea4c2e0d16137f204c1c9`
ELECTRONIC SIGNATURE:	`Insp. Rajesh Sharma [RRSL-DOCA-2026-449] | CENTRALLY REGISTERED DOCA COMPLIANCE STAMP`