DentSurg PRO

PREDICTABILITY AND SAFETY. PATIENT SATISFACTION

Designed to achieve maximum performance and efficient, allows working in hard-to-reach areas, does not cut soft tissues and causes fewer damages, providing a better d 7 mm provide the best user experience, the DentSurg Pro provides precise cuts and postoperative course and predictability for you and your patient

- 7-inch screen
- Adjustable LED lighting up to 70 lumens
- Remote software update
- Handpieces and irrigation system fully autoclavable
- Favorites function
- Saline support
- Low noise level
- Portable
- Automatic dual voltage



Diamond tips - DLC

Process known as Diamond Like Carbon - DLC- of CVDentus®, is a patented technology and is applied as a film on the tips of the surgical line, promoting


wear resistance, reduction of the coefficient of friction and it also has bactericidal effect.

Manufactured in titanium alloy, a noble material used in aircraft and satellites, it has characteristics that make it ideal for manufacturing ultrasonic tips.

It has low weight and excellent properties physico-chemical mechanical wear resistance at high temperatures and also corrosion resistance.




The thicknesses of the active part are manufactured starting from 0.28 mm and diameters that ensure precision and no unnecessary wear, allowing high-performance and safe osteotomies.

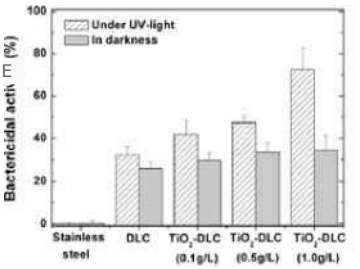

ADDITIVE DLC WITH TITANIUM DIOXIDE (TiO2) NANOPARTICLES REDUCES ACTIVITY

D BACTERIAL UP TO 75%


Investigation into the antibacterial property and bacterial adhesion of diamond-like carbon films F.R. Marciano a.b.*, L.F. Bonetti c, J.F. Mangolin d, N.S. Da-Silva d, E.J. Corat a, V.J. Trava-Airoldi a

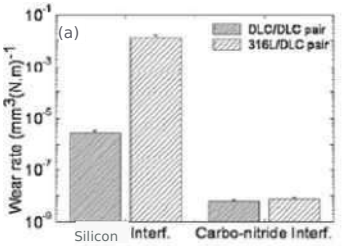

DLC HAS A COEFFICIENT EXTREMELY LOW, NEAR TEFLON. ENSURING LESS TISSUE DAMAGE AND LESS HEAT GENERATION

Friction and wear maps of titanium alloy against 3-C:H2O% (DLC) film P.A. Rad□ ab* L.V. Santos a, L.F Boneti a.b, GC.

Rodrigues a, MJ Trava-Airold□a




THE DLC PROTECTS THE PIECE'S SERVICE LIFE, PROTECTING IT FROM ELECTRO-CHEMICAL CORROSION.

Crystalline diamond particles into diamond-like carbon films: The influence of the particle sizes on the electrothermical corrosion resistance F.R. Marciano a.b.*, E.C. Almeida a, D.A. Lima-Oliveira a, E.J. Corat a.b., V.J. Trava-Airoldi a

Bone cutting




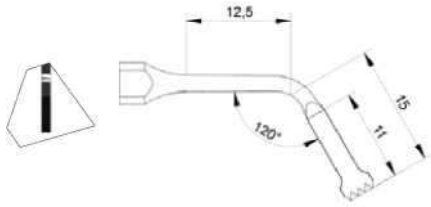

Code SF11
0.5 mm

- High efficiency in bone cutting.




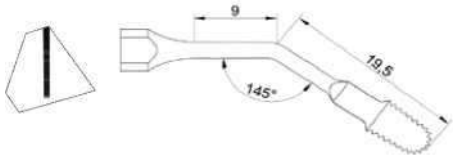

Code SFR4
0.45 mm

- High efficiency in bone cutting / Serrated for anteroposterior cutting.



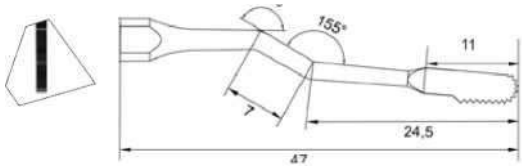

Code SFR42
0.60 mm

- High efficiency in bone cutting in hard-to-reach areas.






Code SFR43
0.40 mm

- High efficiency in bone cutting in hard-to-reach areas.




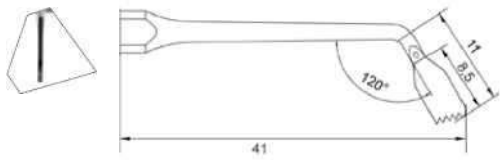

Code SF32
0.30 mm

- Serrated for anteroposterior cutting in hard-to-reach areas.




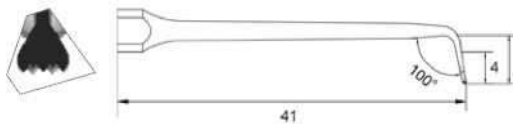

Code SF32-O
0.40 mm

- Serrated for transversal cutting in hard-to-reach areas.




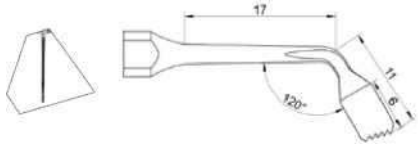

Code SF38
0.28mm

- Slotted for cutting anterior-posterior.






Code SF38-O
0.28mm

- Slotted for cutting in the orthogonal and collection of autogenous material.




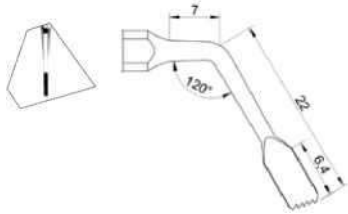

Code SF3
0.28mm

- Slotted for cutting anterior-posterior.




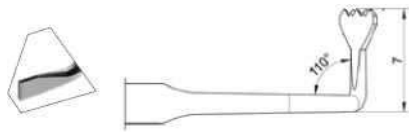

Code SF3-L
0.40mm

- Slotted for cutting. Angulated stem to the left for areas of difficult access.



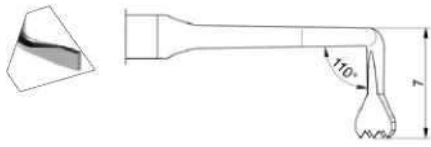


Code SF3-R
0.40mm

- Slotted for cutting. Stem angulated to the right for areas of difficult access.

Bone cut - Delicate regions



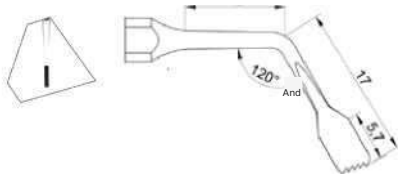

Code SF3F
0.40mm


- Microdrill for cutting in areas near nerves, membranes and other soft tissues.

Bone scraping

Code SE9G 3
Ø.9mm

- Scraping and regularization of the bone surface.




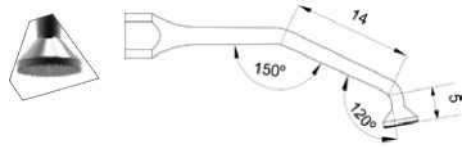

Code SE9F
Ø 3.9mm

- Scraping for finishing and regularization of the bone surface.






2015

Code SFS3-O
0.40mm

- It has no saw. Performs a scraping uniform.



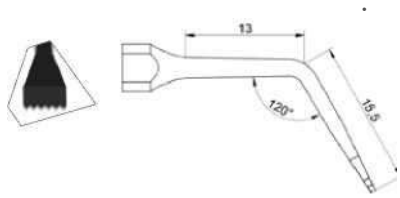


Code SF3F-O 0.40mm

- Microdrill for collection of autologous material.

Detachment of soft tissue




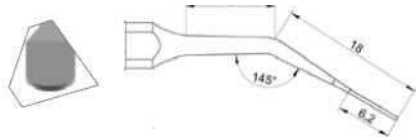

Code. SLTV- O
0.40mm

Bone perforation






Code. STR1
0 0.6mm

• Has mm markings to help in the measurement of depth.




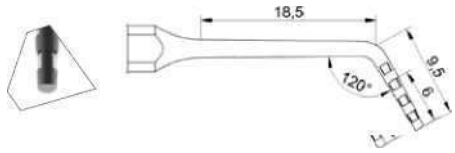

Code. STR4
0 1.5mm

• Conical trunk shape. Has depth marks depth: - 1 - 2mm - 3 - 4mm - 5 – 6mm - 7 – 8mm




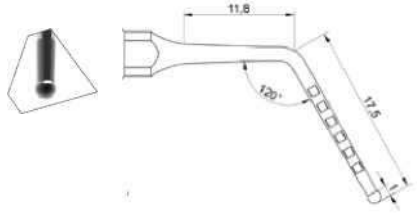

Code. SR2
0 1.3mm

• Conical trunk shape with a sphere in the active part. It has depth marks on: - 4 - 5 - 6 - 7 - 8 – 9 - 10 – 11 - 12 – 13 - 14 – 15 - 16 – 17




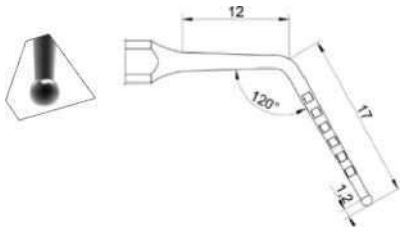

Code SR4
Ø 1.5mm

• Spherical for bone wear. It has mm markings to aid in the measurement of depth.





Code SR9
Ø 2.5mm

• Spherical for wear bone.



Code SF2
1.0mm

• Has 3.5mm of active area depth