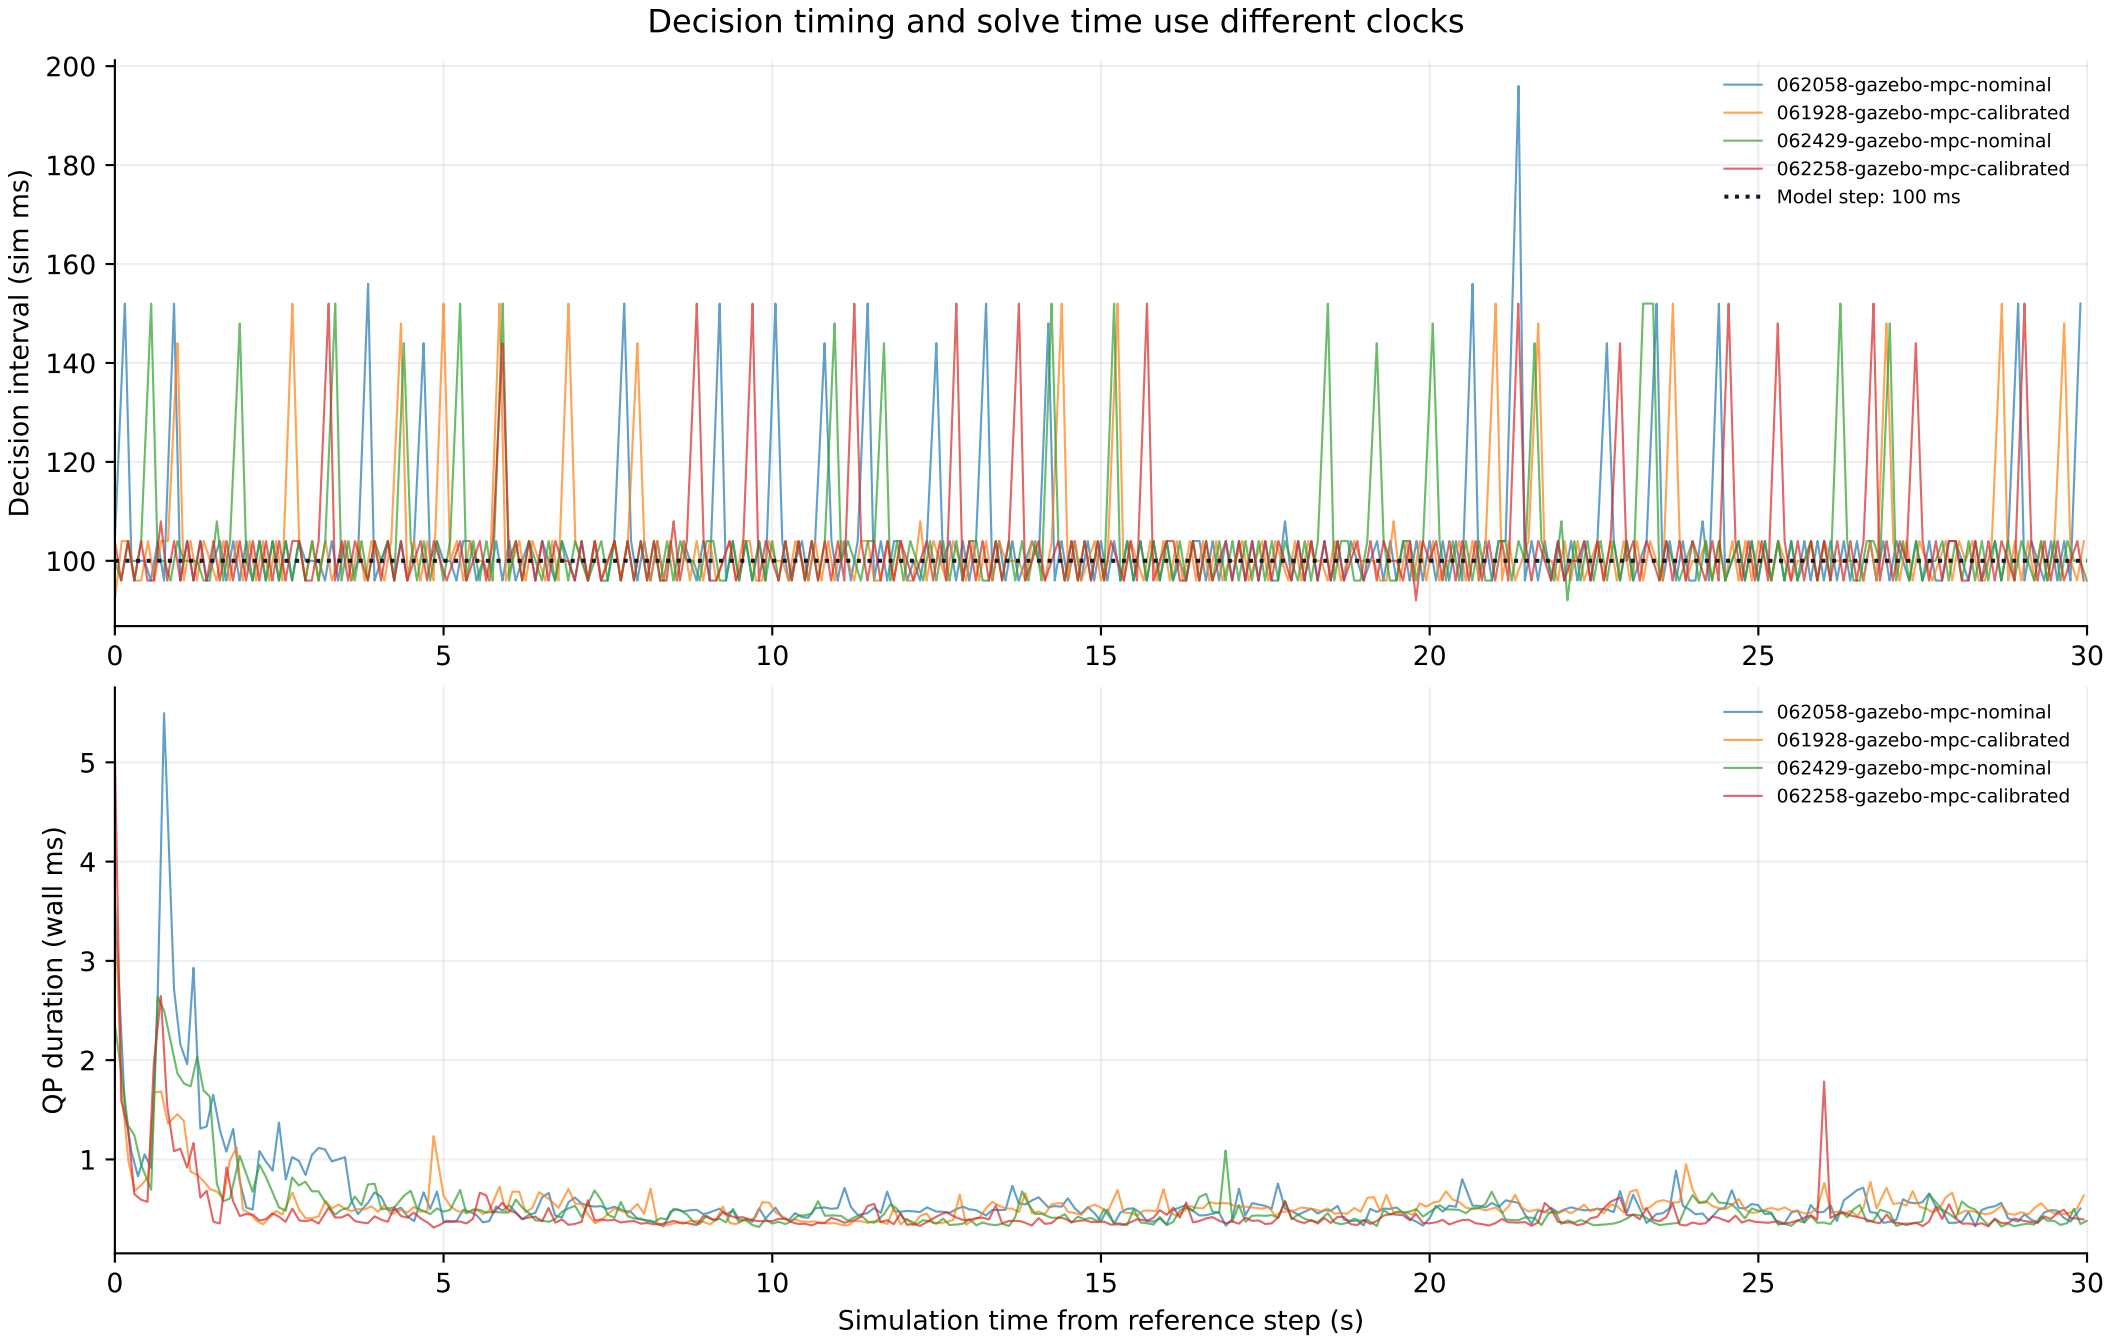
Decision timing and solve time use different clocks
Decision interval (sim ms)
200
180
160
140
120
100
062058-gazebo-mpc-nominal
061928-gazebo-mpc-calibrated
062429-gazebo-mpc-nominal
062258-gazebo-mpc-calibrated
Model step: 100 ms
0
5
10
15
20
25
30
QP duration (wall ms)
5
4
3
2
1
062058-gazebo-mpc-nominal
061928-gazebo-mpc-calibrated
062429-gazebo-mpc-nominal
062258-gazebo-mpc-calibrated
0
5
10
15
20
25
30
Simulation time from reference step (s)